

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041321\
 Data File : P0076964.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Apr 2021 16:52
 Operator : AJ/MA
 Sample : M2014-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 16128

Manual Integrations
 APPROVED

Ankita
 4/14/2021 1:53:36 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 14 03:48:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 02 05:20:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.900	3.896	1315380	646720	14.142	12.887
2) SA Decachlor...	10.866	9.137	483506	245514	5.220	5.059m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041321\
Data File : P0076964.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Apr 2021 16:52
Operator : AJ/MA
Sample : M2014-04
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
16128


Manual Integrations
APPROVED

Ankita
4/14/2021 1:53:36 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 14 03:48:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 02 05:20:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

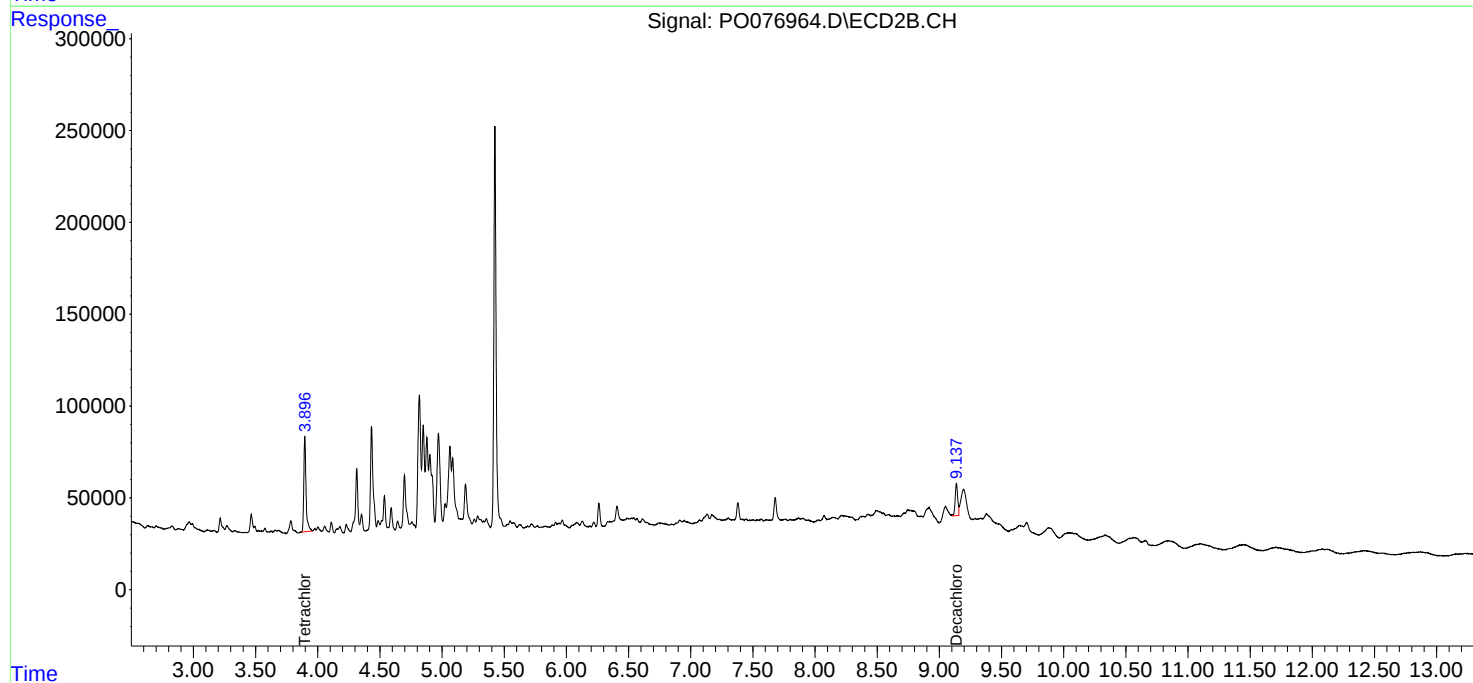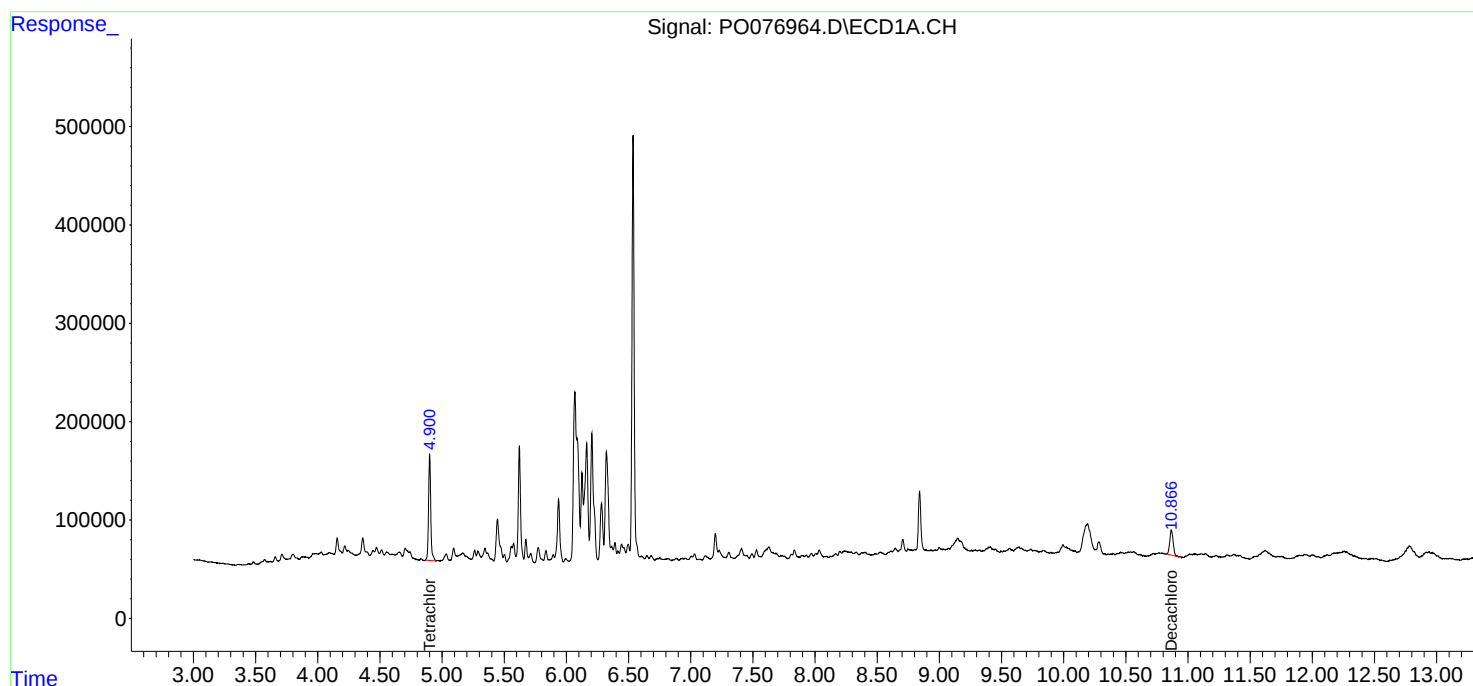

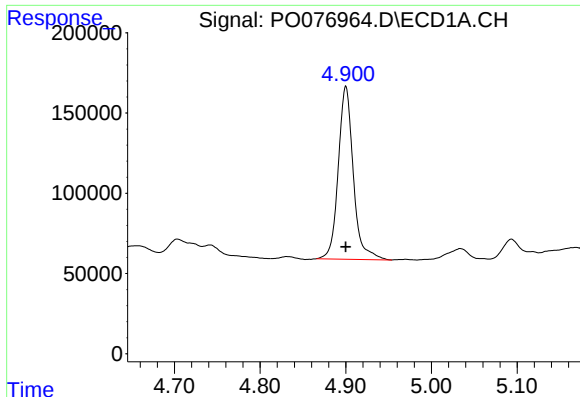


#1 Tetrachloro-m-xylene

R.T.: 4.900 min
Delta R.T.: 0.000 min
Response: 1315380
Conc: 14.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
16128


Manual Integrations
APPROVED

Ankita
4/14/2021 1:53:36 PM

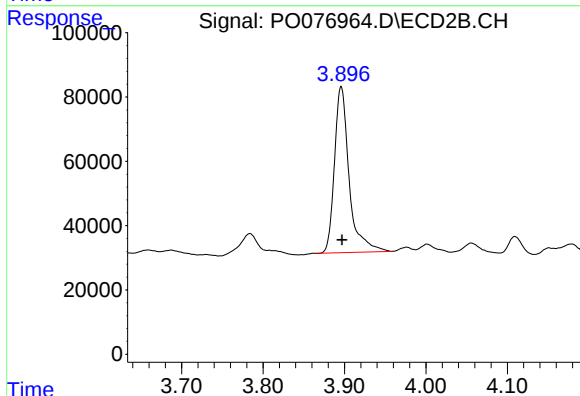


#1 Tetrachloro-m-xylene

R.T.: 3.896 min
Delta R.T.: -0.001 min
Response: 646720
Conc: 12.89 ng/ml

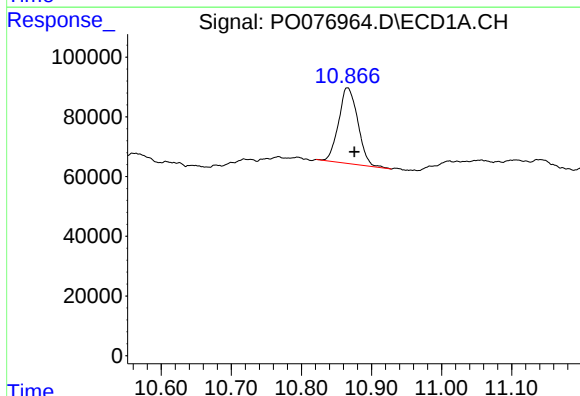

#2 Decachlorobiphenyl

R.T.: 10.866 min
Delta R.T.: -0.010 min
Response: 483506
Conc: 5.22 ng/ml

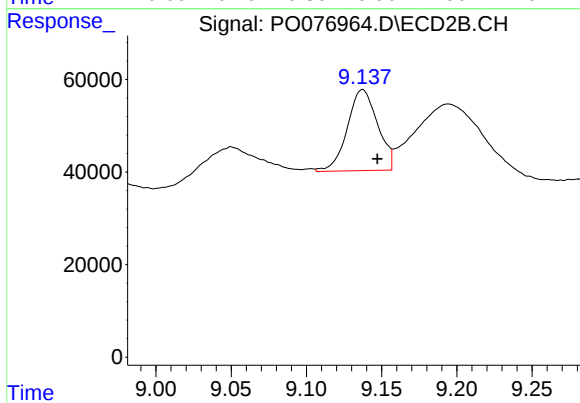

#2 Decachlorobiphenyl

R.T.: 9.137 min
Delta R.T.: -0.010 min
Response: 245514
Conc: 5.06 ng/ml m