

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041323\
 Data File : P0094191.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Apr 2023 11:42
 Operator : YP/AJ
 Sample : 02291-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 23330

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/14/2023
 Supervised By :Ankita Jodhani 04/14/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 22:47:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 04 06:20:55 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.421	3.626	24002716	10596569	6.421m	8.321 #
2) SA Decachlor...	10.251	8.646	18372589	7293380	8.213	7.295

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO041323\
Data File : PO094191.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Apr 2023 11:42
Operator : YP/AJ
Sample : 02291-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
23330


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/14/2023
Supervised By :Ankita Jodhani 04/14/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 22:47:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO040323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 04 06:20:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

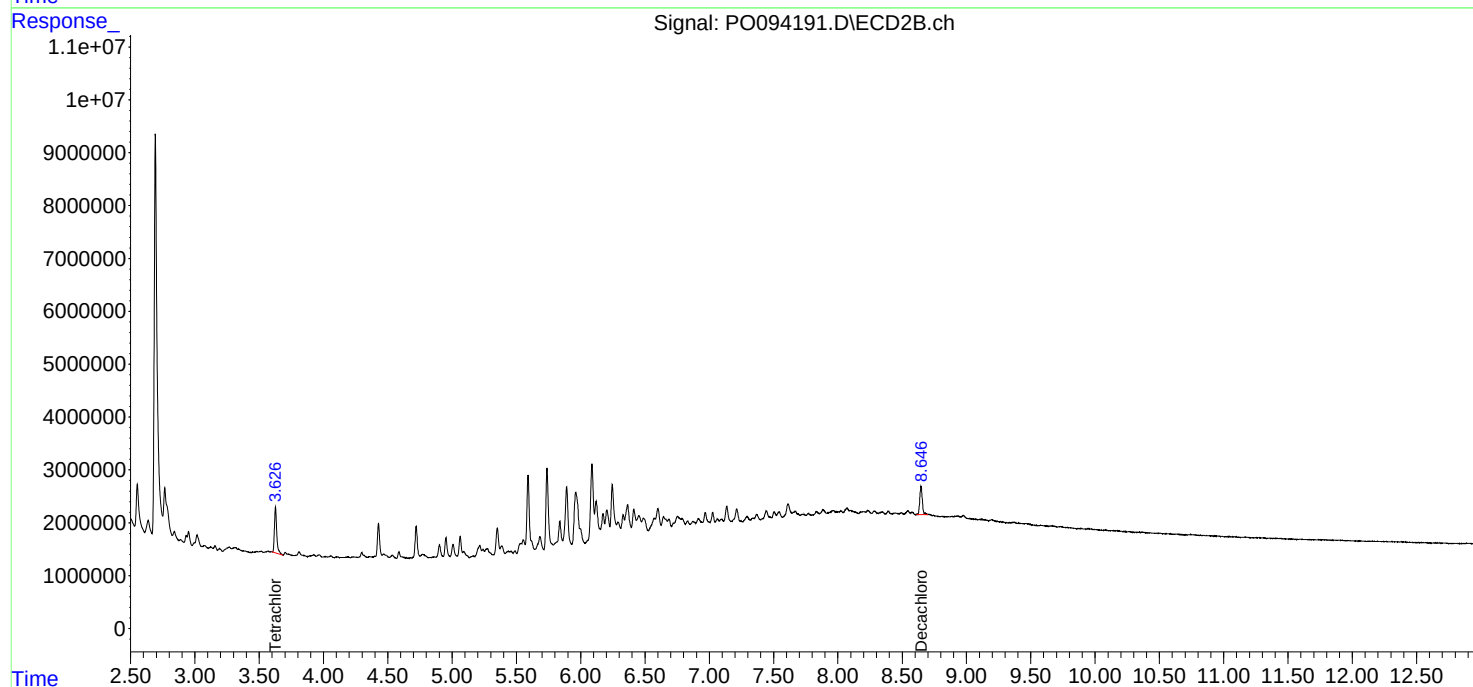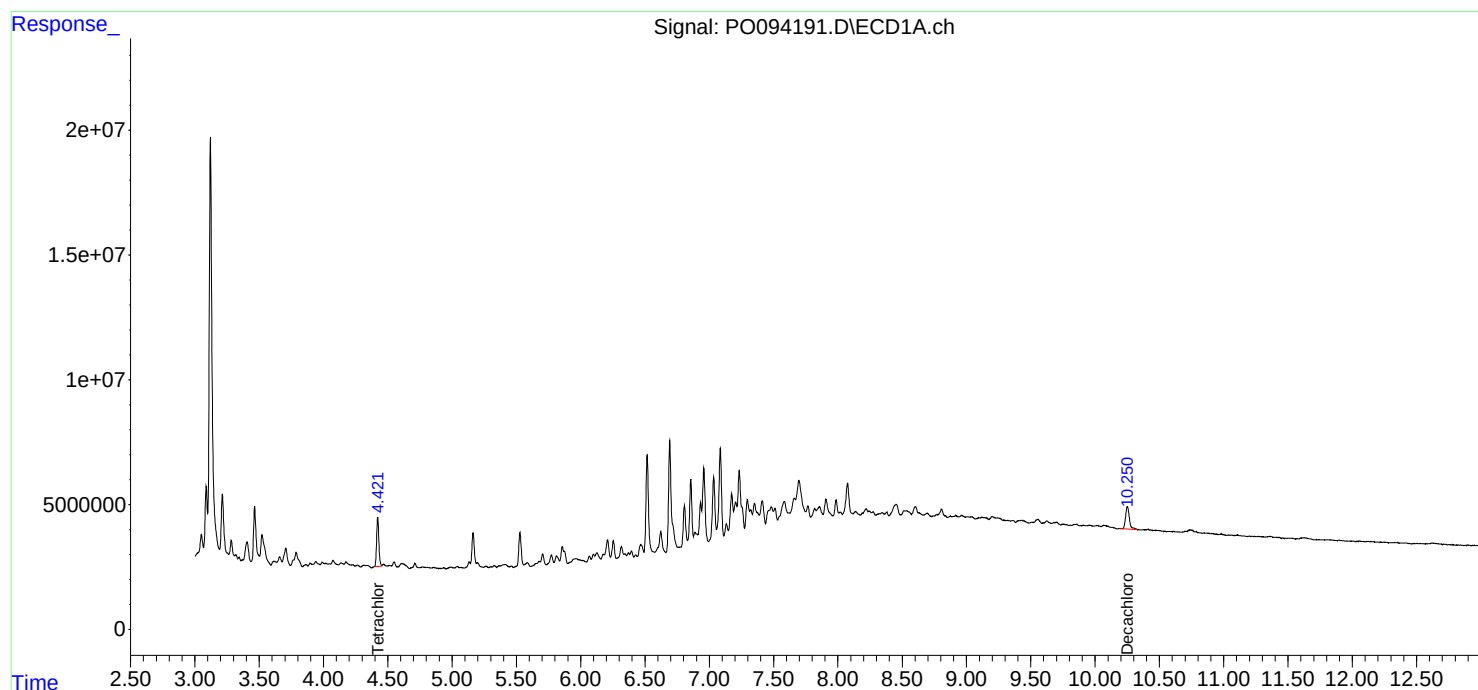

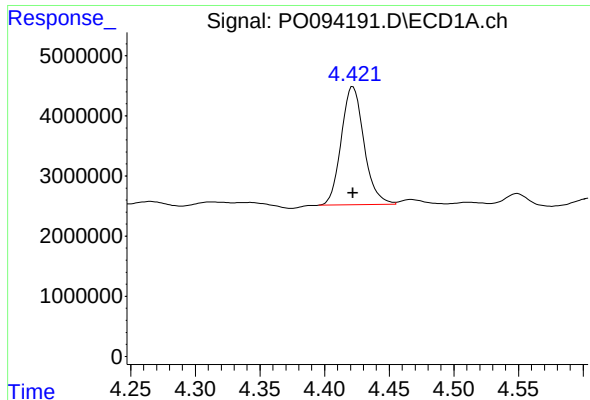


#1 Tetrachloro-m-xylene

R.T.: 4.421 min
Delta R.T.: 0.000 min
Response: 24002716
Conc: 6.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
23330


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/14/2023
Supervised By :Ankita Jodhani 04/14/2023

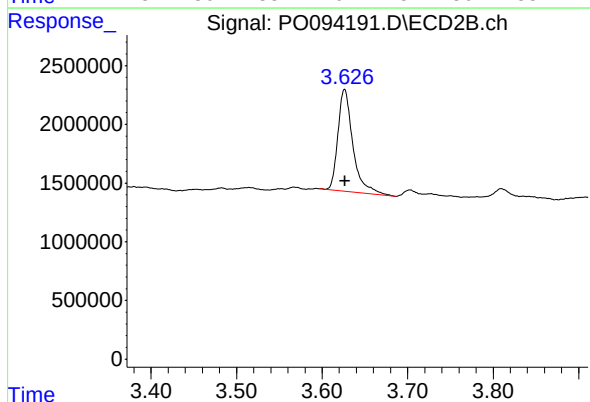


#1 Tetrachloro-m-xylene

R.T.: 3.626 min
Delta R.T.: 0.000 min
Response: 10596569
Conc: 8.32 ng/ml

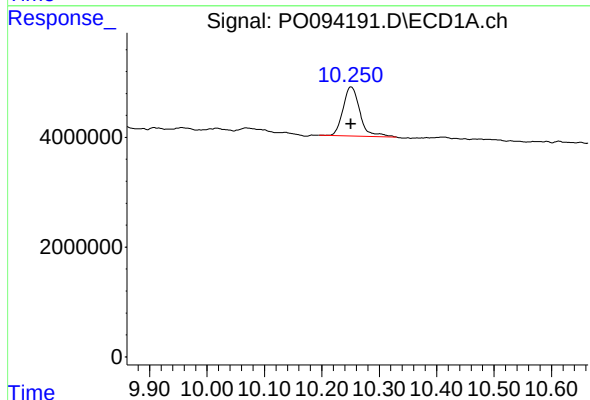

#2 Decachlorobiphenyl

R.T.: 10.251 min
Delta R.T.: 0.000 min
Response: 18372589
Conc: 8.21 ng/ml

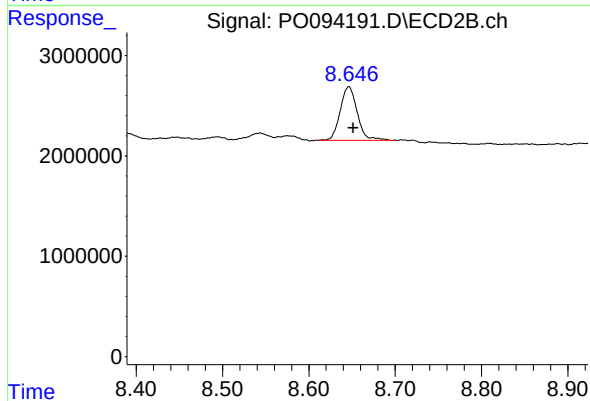

#2 Decachlorobiphenyl

R.T.: 8.646 min
Delta R.T.: -0.005 min
Response: 7293380
Conc: 7.29 ng/ml