

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041323\
 Data File : P0094204.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Apr 2023 16:19
 Operator : YP/AJ
 Sample : 02292-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 IDW-SO-G2-041123

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 23:05:14 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 04 06:20:55 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.422	3.626	69180069	28582728	18.506	22.446
2) SA Decachlor...	10.252	8.647	45733129	22148603	20.445	22.153

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO041323\
Data File : PO094204.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Apr 2023 16:19
Operator : YP/AJ
Sample : 02292-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
IDW-SO-G2-041123

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 23:05:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO040323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 04 06:20:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

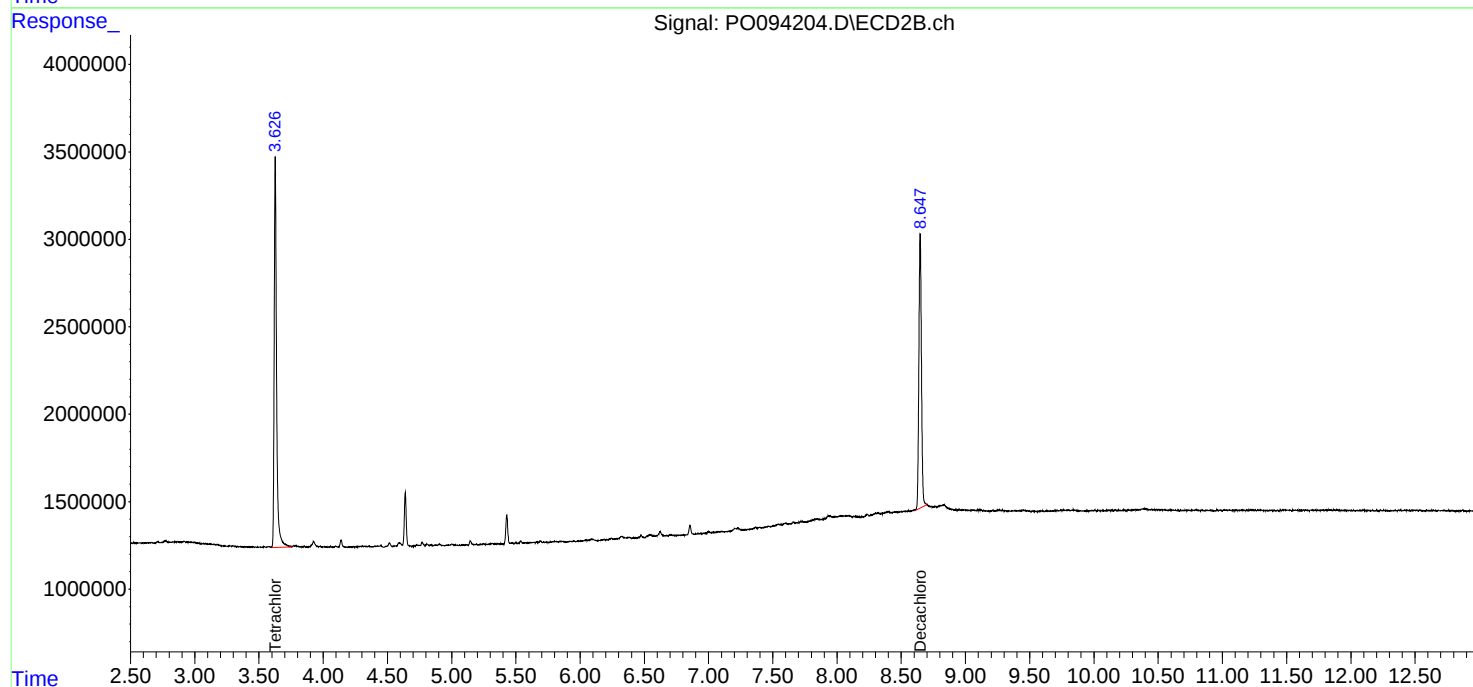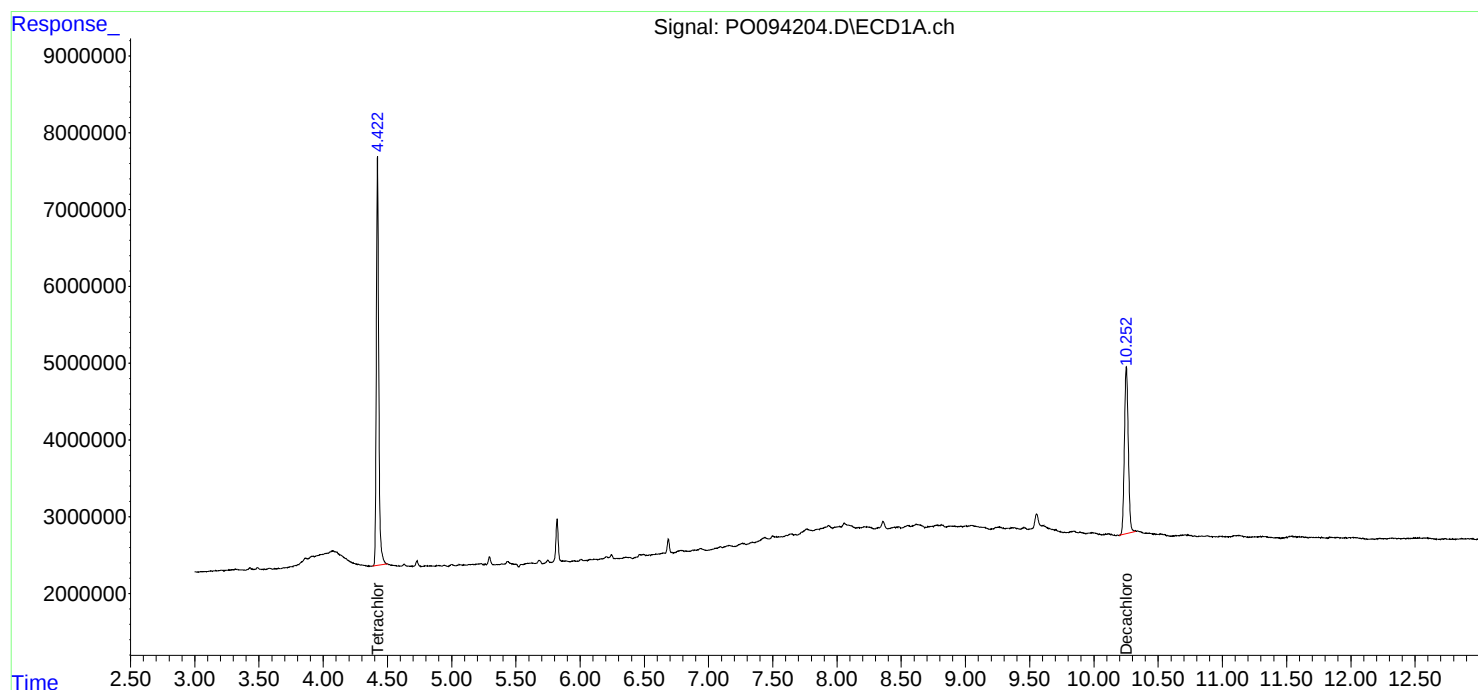


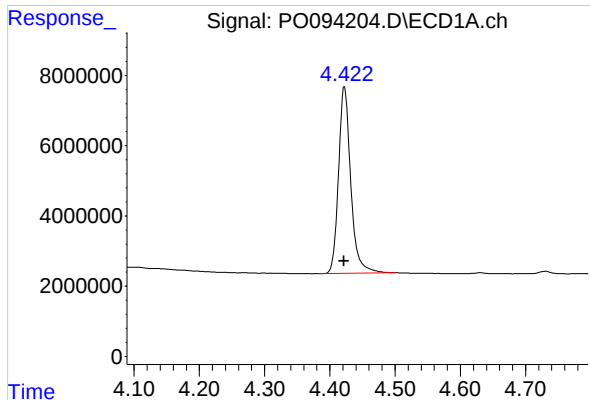

#1 Tetrachloro-m-xylene


R.T.: 4.422 min
Delta R.T.: 0.000 min
Response: 69180069
Conc: 18.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
IDW-SO-G2-041123

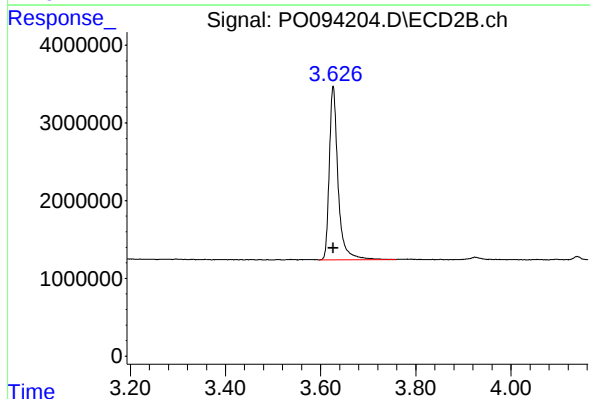


#1 Tetrachloro-m-xylene

R.T.: 3.626 min
Delta R.T.: 0.000 min
Response: 28582728
Conc: 22.45 ng/ml

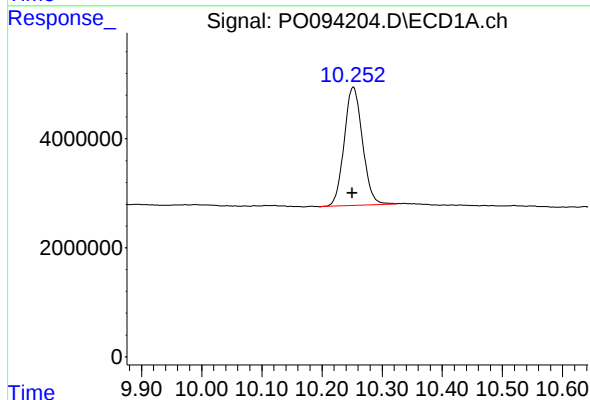

#2 Decachlorobiphenyl

R.T.: 10.252 min
Delta R.T.: 0.002 min
Response: 45733129
Conc: 20.44 ng/ml

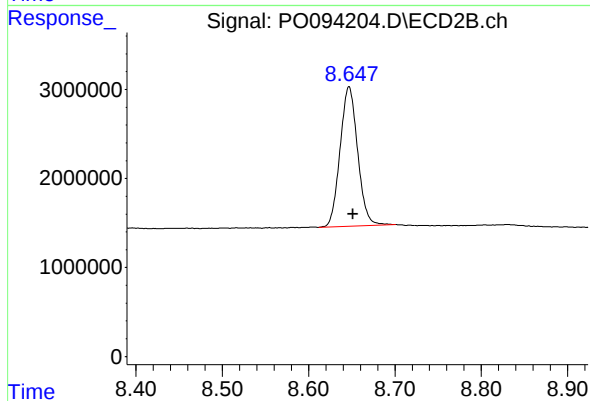

#2 Decachlorobiphenyl

R.T.: 8.647 min
Delta R.T.: -0.005 min
Response: 22148603
Conc: 22.15 ng/ml