

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041323\
 Data File : P0094216.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Apr 2023 20:30
 Operator : YP/AJ
 Sample : 02310-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 VNJ-228

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/14/2023
 Supervised By :Ankita Jodhani 04/14/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 23:13:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 04 06:20:55 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.418	3.622	76571289	25185290	20.483m	19.778
2) SA Decachlor...	10.245	8.641	54973314	22132018	24.575	22.137

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO041323\
Data File : PO094216.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Apr 2023 20:30
Operator : YP/AJ
Sample : 02310-01
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
VNJ-228


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/14/2023
Supervised By :Ankita Jodhani 04/14/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 23:13:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO040323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 04 06:20:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

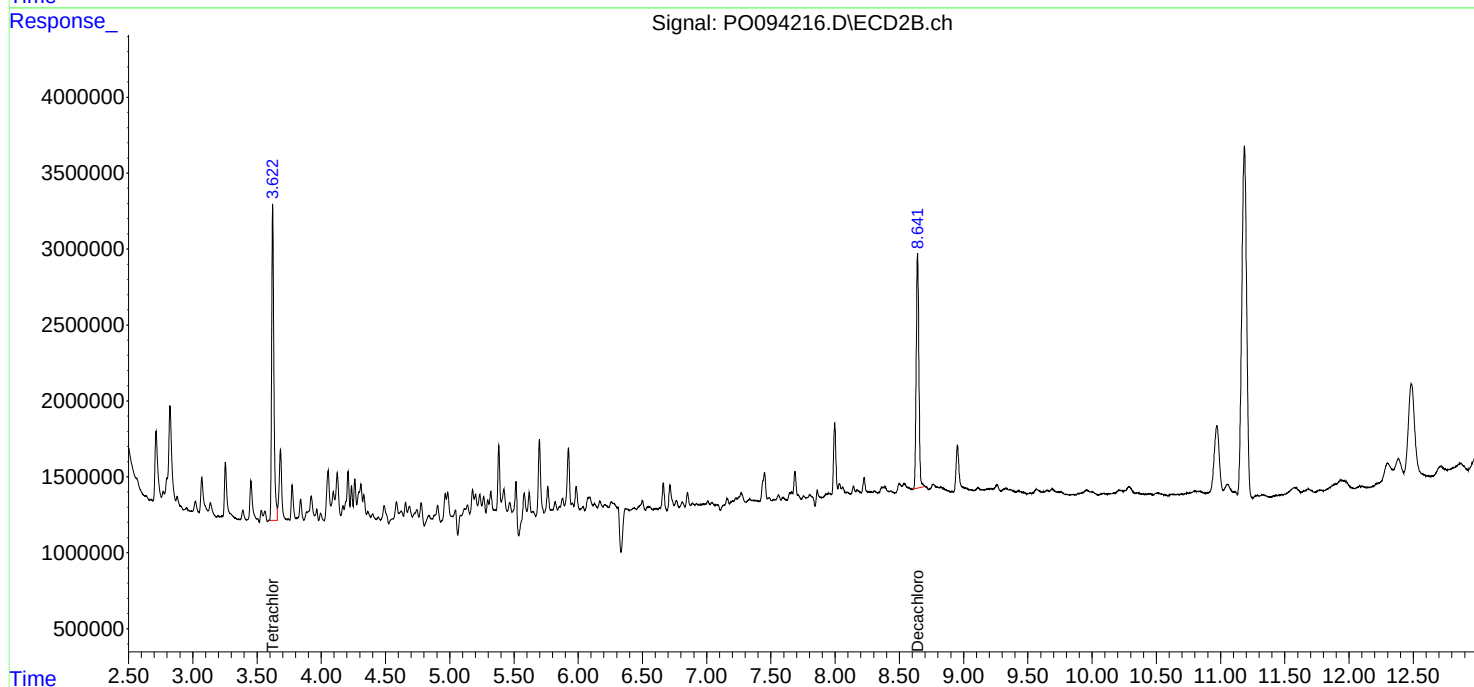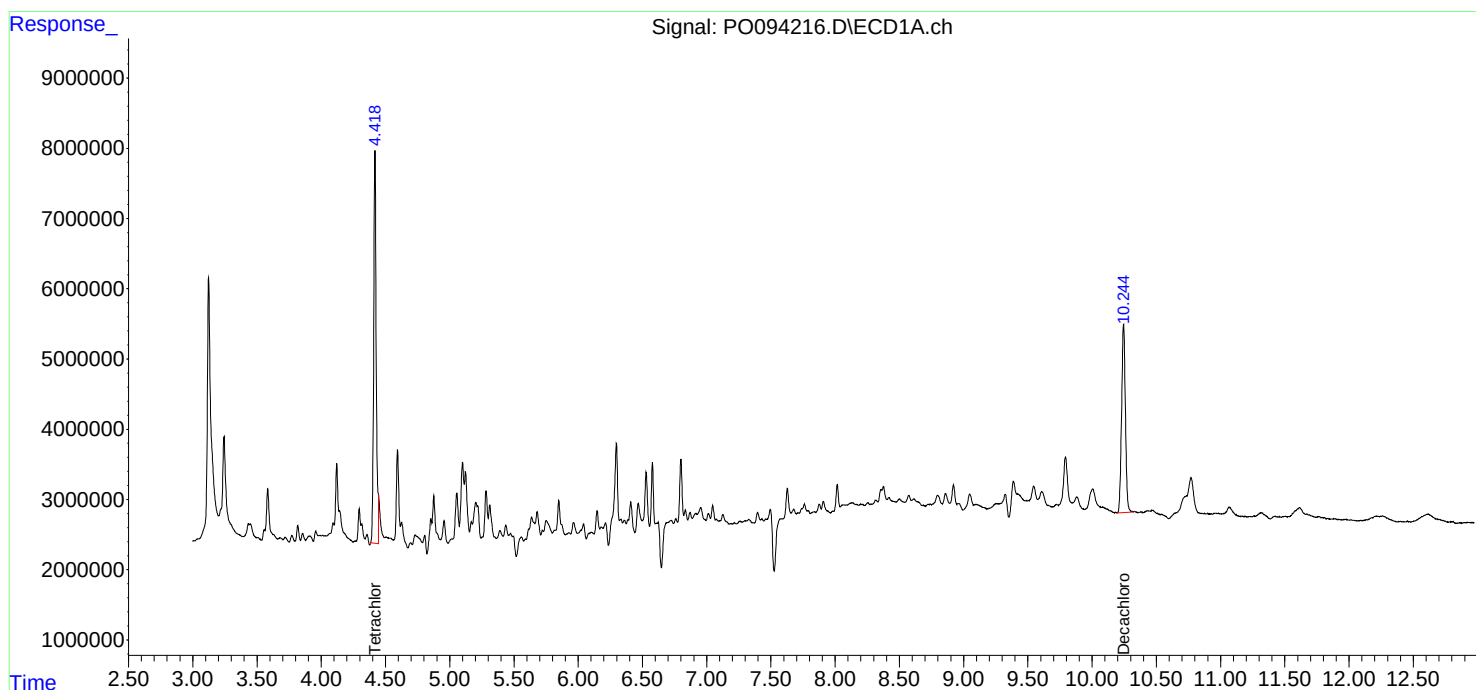

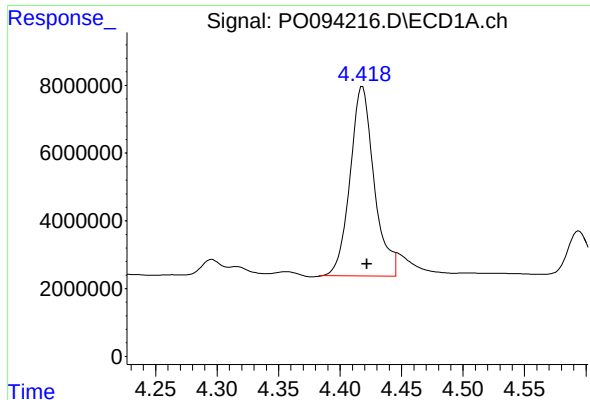


#1 Tetrachloro-m-xylene

R.T.: 4.418 min
Delta R.T.: -0.004 min
Response: 76571289
Conc: 20.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
VNJ-228


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/14/2023
Supervised By :Ankita Jodhani 04/14/2023

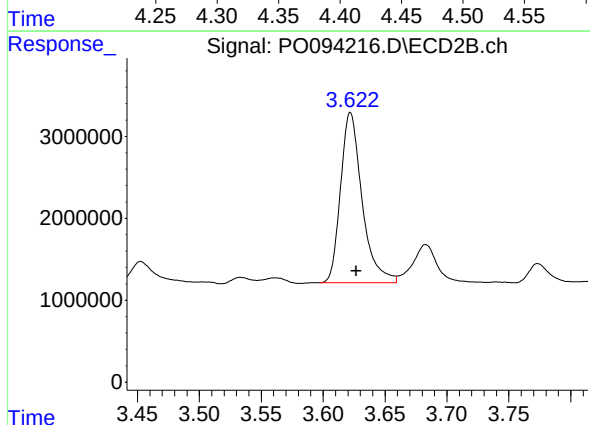


#1 Tetrachloro-m-xylene

R.T.: 3.622 min
Delta R.T.: -0.005 min
Response: 25185290
Conc: 19.78 ng/ml

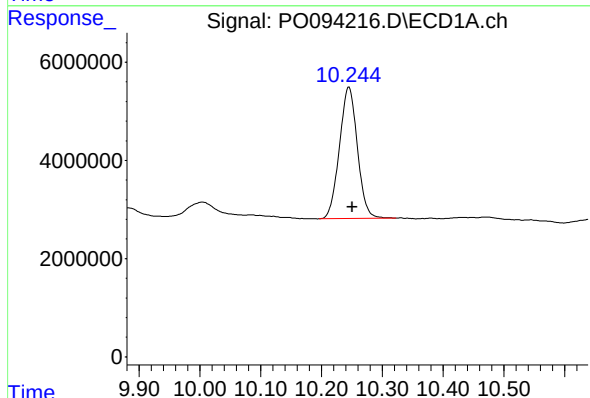

#2 Decachlorobiphenyl

R.T.: 10.245 min
Delta R.T.: -0.006 min
Response: 54973314
Conc: 24.58 ng/ml

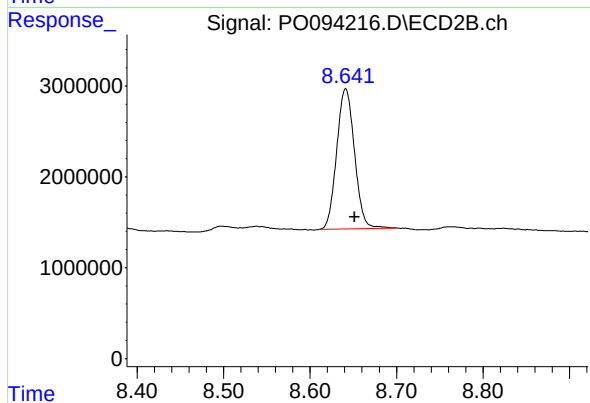

#2 Decachlorobiphenyl

R.T.: 8.641 min
Delta R.T.: -0.010 min
Response: 22132018
Conc: 22.14 ng/ml