

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041324\
Data File : P0102799.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Apr 2024 13:29
Operator : YP/AJ
Sample : P2062-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
31551

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/15/2024
Supervised By :Ankita Jodhani 04/15/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 15:25:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 19 08:56:28 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.262	3.377	92198195	52991693	20.912	18.417m
2) SA Decachlor...	9.797	8.241	55874330	34835082	20.124	19.202

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO041324\
Data File : PO102799.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Apr 2024 13:29
Operator : YP/AJ
Sample : P2062-02
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
31551


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/15/2024
Supervised By :Ankita Jodhani 04/15/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 15:25:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 19 08:56:28 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

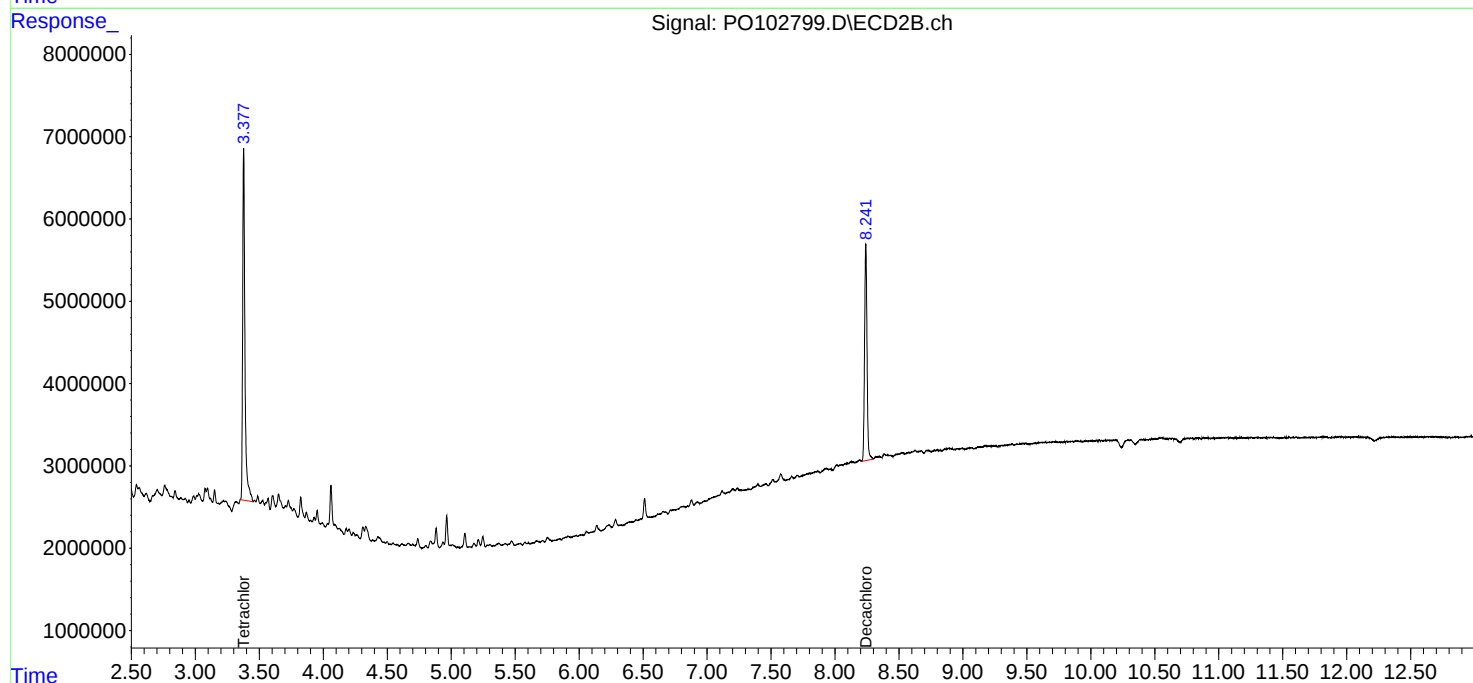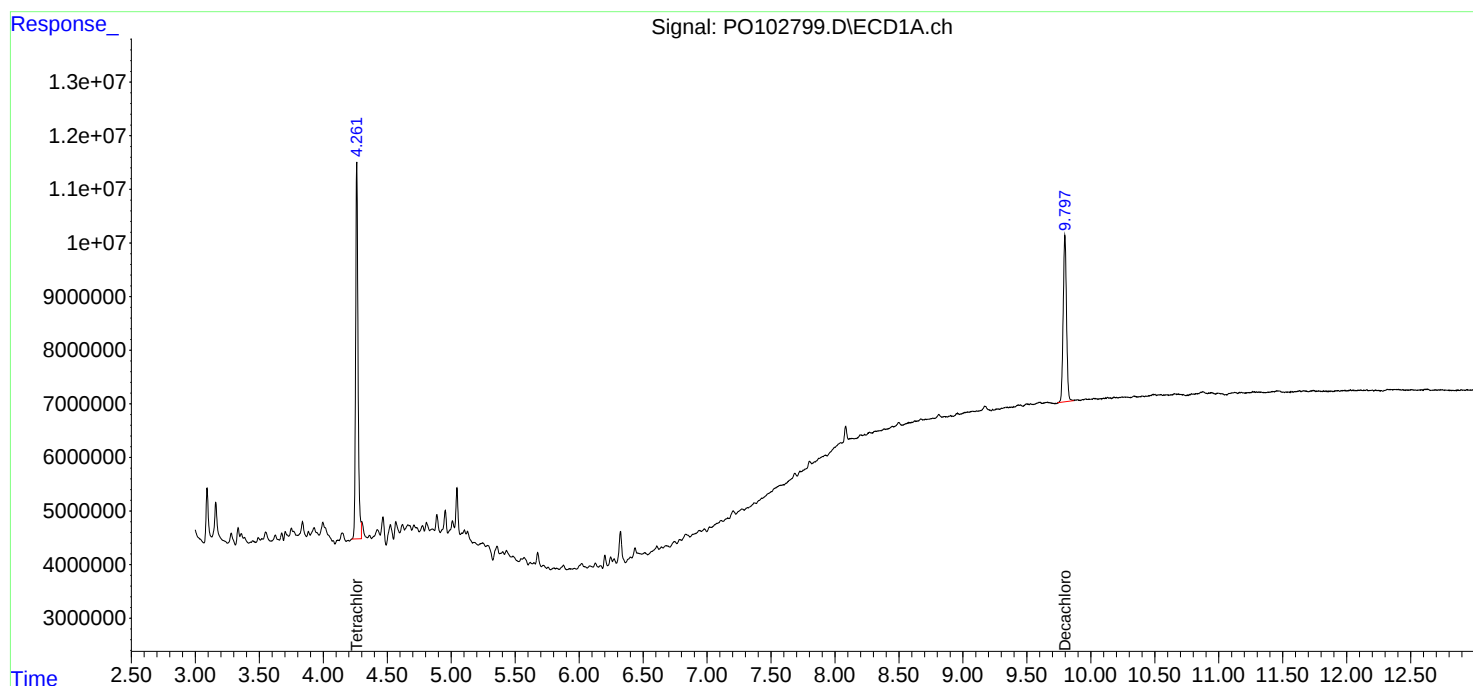

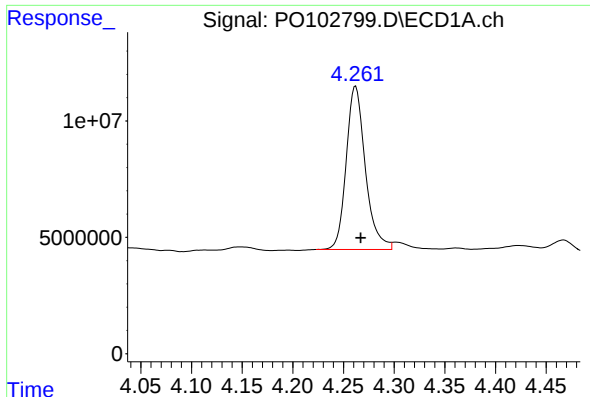


#1 Tetrachloro-m-xylene

R.T.: 4.262 min
Delta R.T.: -0.005 min
Response: 92198195
Conc: 20.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
31551


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/15/2024
Supervised By :Ankita Jodhani 04/15/2024

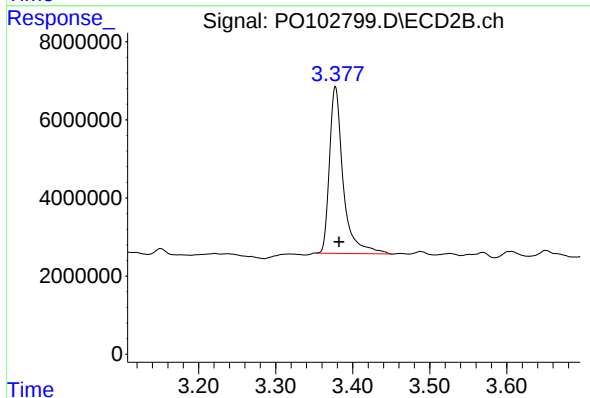


#1 Tetrachloro-m-xylene

R.T.: 3.377 min
Delta R.T.: -0.005 min
Response: 52991693
Conc: 18.42 ng/ml m

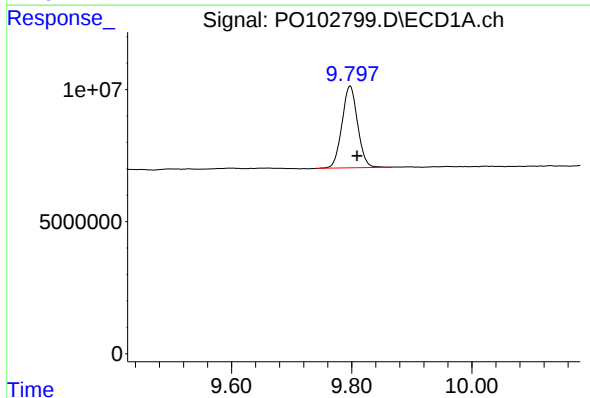

#2 Decachlorobiphenyl

R.T.: 9.797 min
Delta R.T.: -0.011 min
Response: 55874330
Conc: 20.12 ng/ml

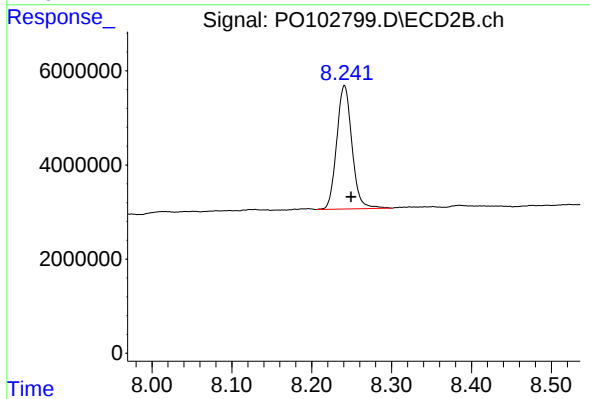

#2 Decachlorobiphenyl

R.T.: 8.241 min
Delta R.T.: -0.008 min
Response: 34835082
Conc: 19.20 ng/ml