

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041423\
 Data File : P0094255.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2023 19:09
 Operator : YP/AJ
 Sample : 02347-09
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 20230338-COMP-16

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/17/2023
 Supervised By :Ankita Jodhani 04/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 14 22:38:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 04 06:20:55 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.417	3.621	63357428	22801704	16.949m	17.906
2) SA Decachlor...	10.245	8.642	30682347	13937263	13.716	13.940

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO041423\
Data File : PO094255.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2023 19:09
Operator : YP/AJ
Sample : 02347-09
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
20230338-COMP-16


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/17/2023
Supervised By :Ankita Jodhani 04/17/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 14 22:38:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO040323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 04 06:20:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

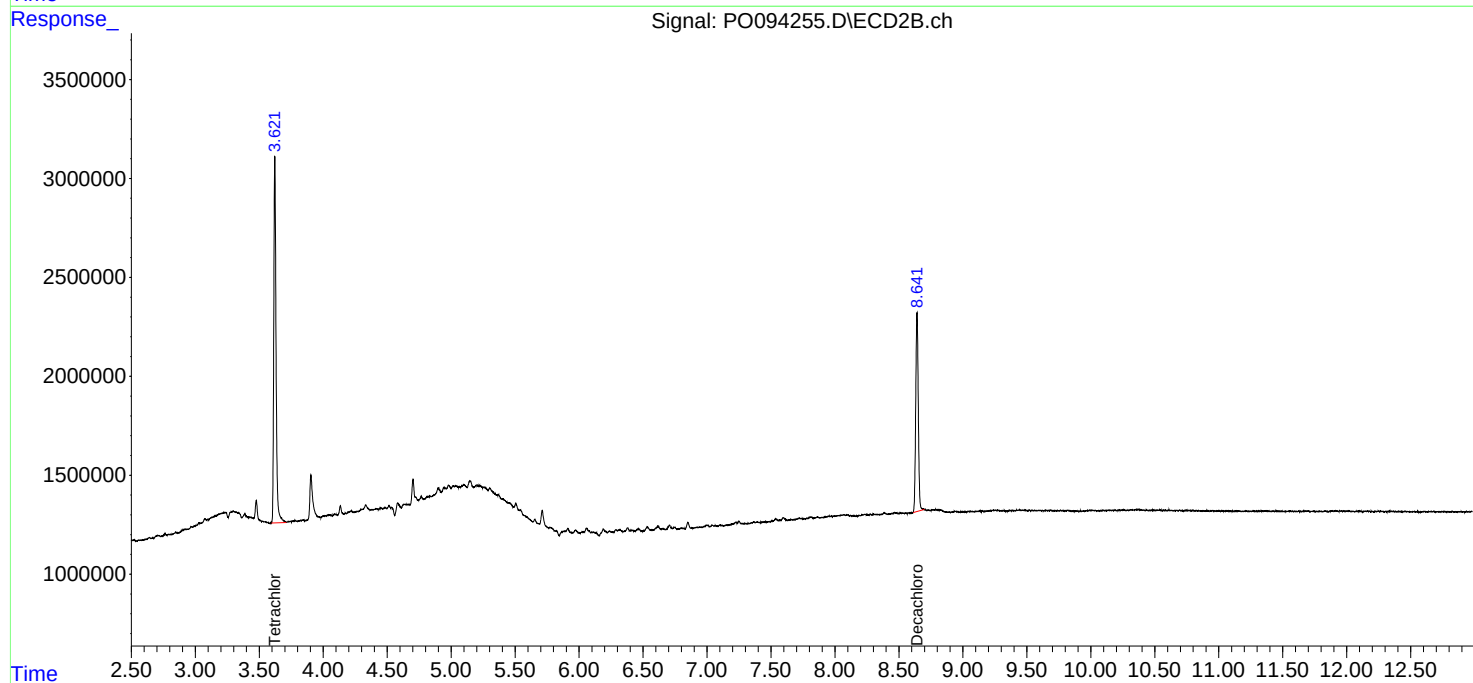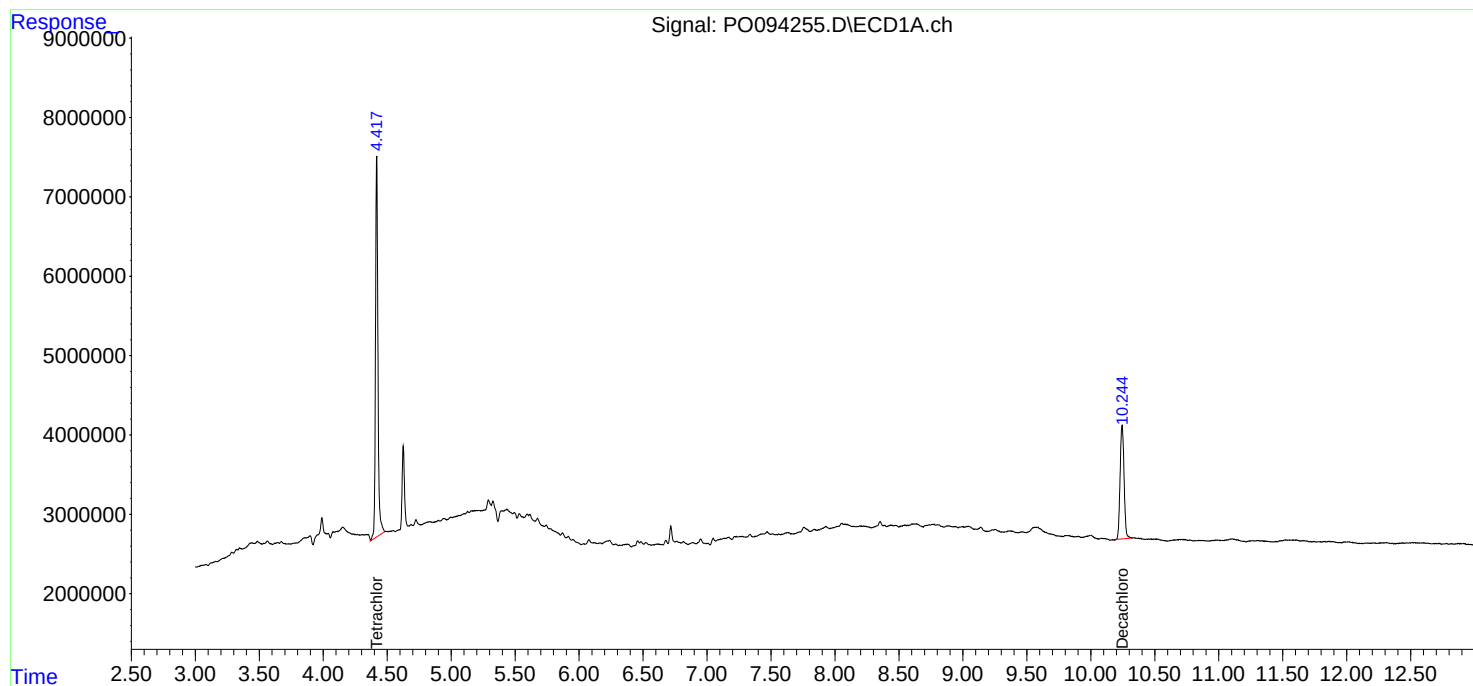

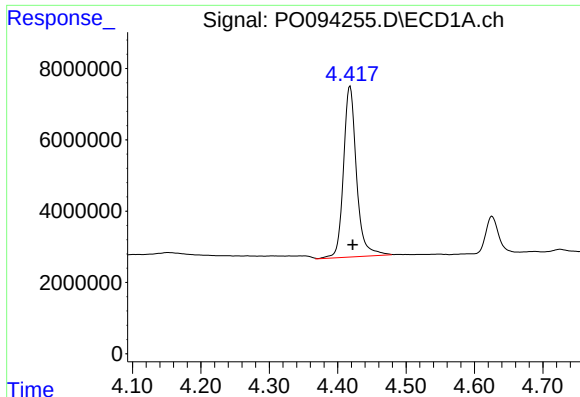


#1 Tetrachloro-m-xylene

R.T.: 4.417 min
Delta R.T.: -0.005 min
Response: 63357428
Conc: 16.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
20230338-COMP-16


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/17/2023
Supervised By :Ankita Jodhani 04/17/2023

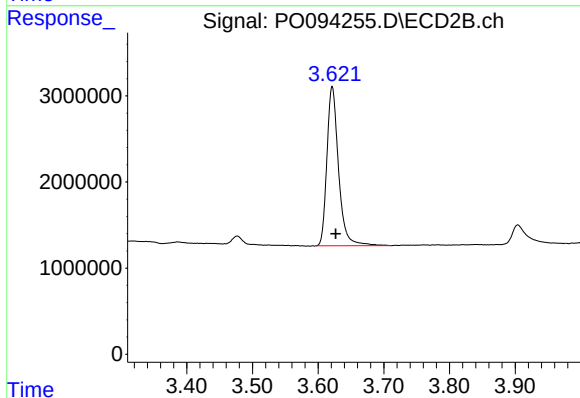


#1 Tetrachloro-m-xylene

R.T.: 3.621 min
Delta R.T.: -0.005 min
Response: 22801704
Conc: 17.91 ng/ml

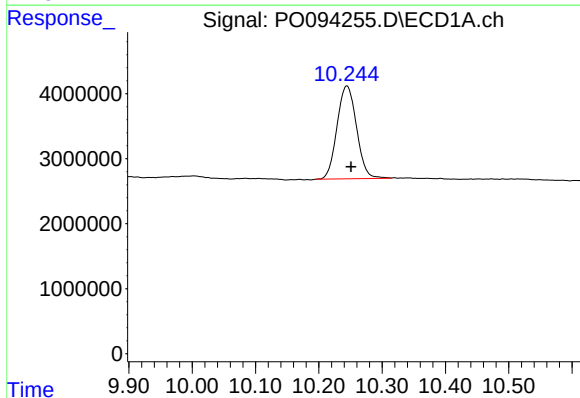

#2 Decachlorobiphenyl

R.T.: 10.245 min
Delta R.T.: -0.006 min
Response: 30682347
Conc: 13.72 ng/ml

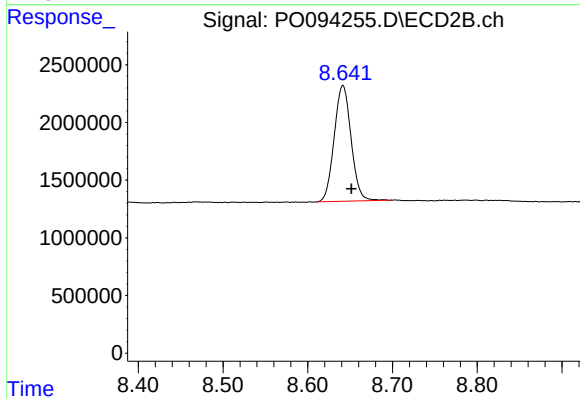

#2 Decachlorobiphenyl

R.T.: 8.642 min
Delta R.T.: -0.010 min
Response: 13937263
Conc: 13.94 ng/ml