

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041521\
 Data File : P0076998.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Apr 2021 12:39
 Operator : AJ/MA
 Sample : M2048-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 13:27:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 02 05:20:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.898	3.894	2476248	1314911	26.622	26.203
2)	SA Decachlor...	10.867	9.136	1868368	807922	20.172	16.649
Target Compounds							
8)	L2 AR-1221-1	5.151	0.000	718883	0	794.553	N.D. #
20)	L4 AR-1242-5	7.227f	0.000	154084	0	78.714	N.D. #
25)	L5 AR-1248-5	7.227f	0.000	154084	0	44.707	N.D. #
34)	L7 AR-1260-4	0.000	7.553	0	14207	N.D.	5.679 #
35)	L7 AR-1260-5	0.000	7.785	0	26695	N.D.	4.526 #
37)	L8 AR-1262-2	0.000	7.785	0	26695	N.D.	4.408 #
40)	L8 AR-1262-5	0.000	8.669f	0	123759	N.D.	62.488 #
44)	L9 AR-1268-4	0.000	8.669f	0	123759	N.D.	56.031 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041521\
Data File : P0076998.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Apr 2021 12:39
Operator : AJ/MA
Sample : M2048-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 13:27:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 02 05:20:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

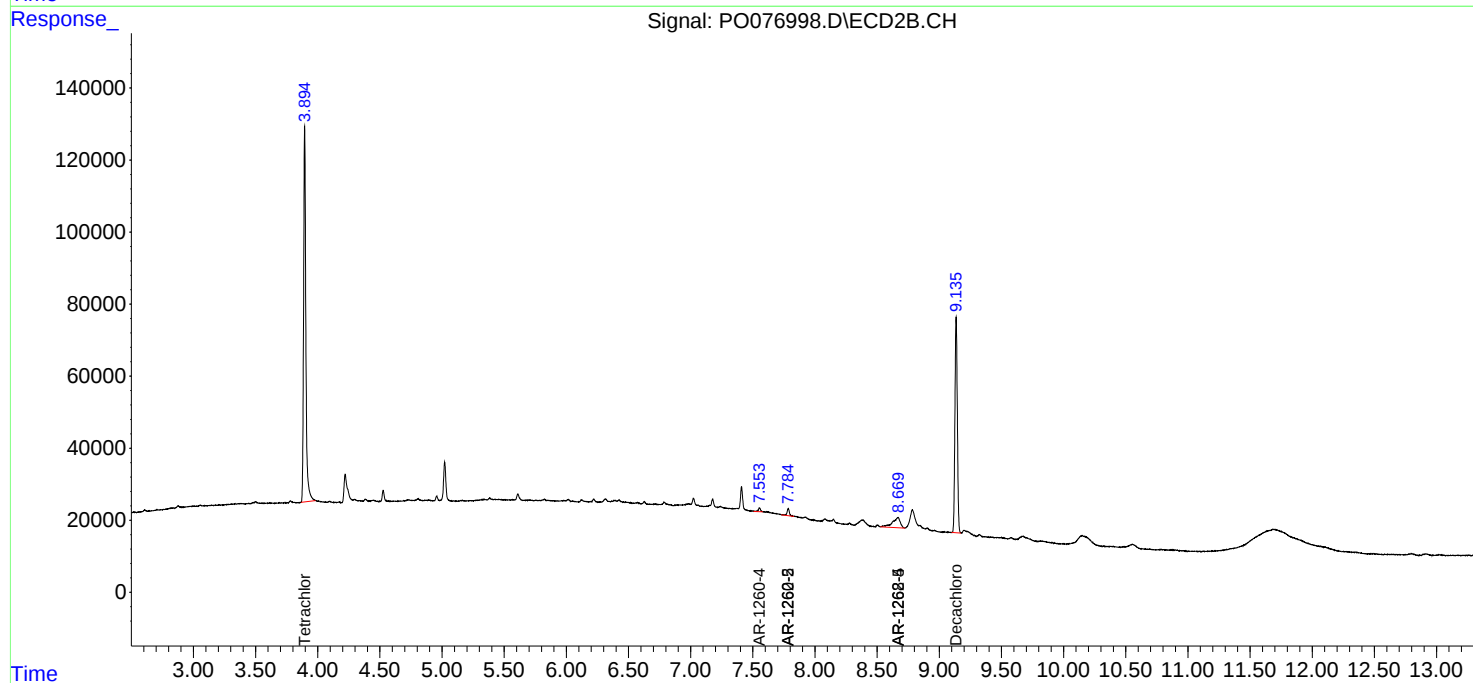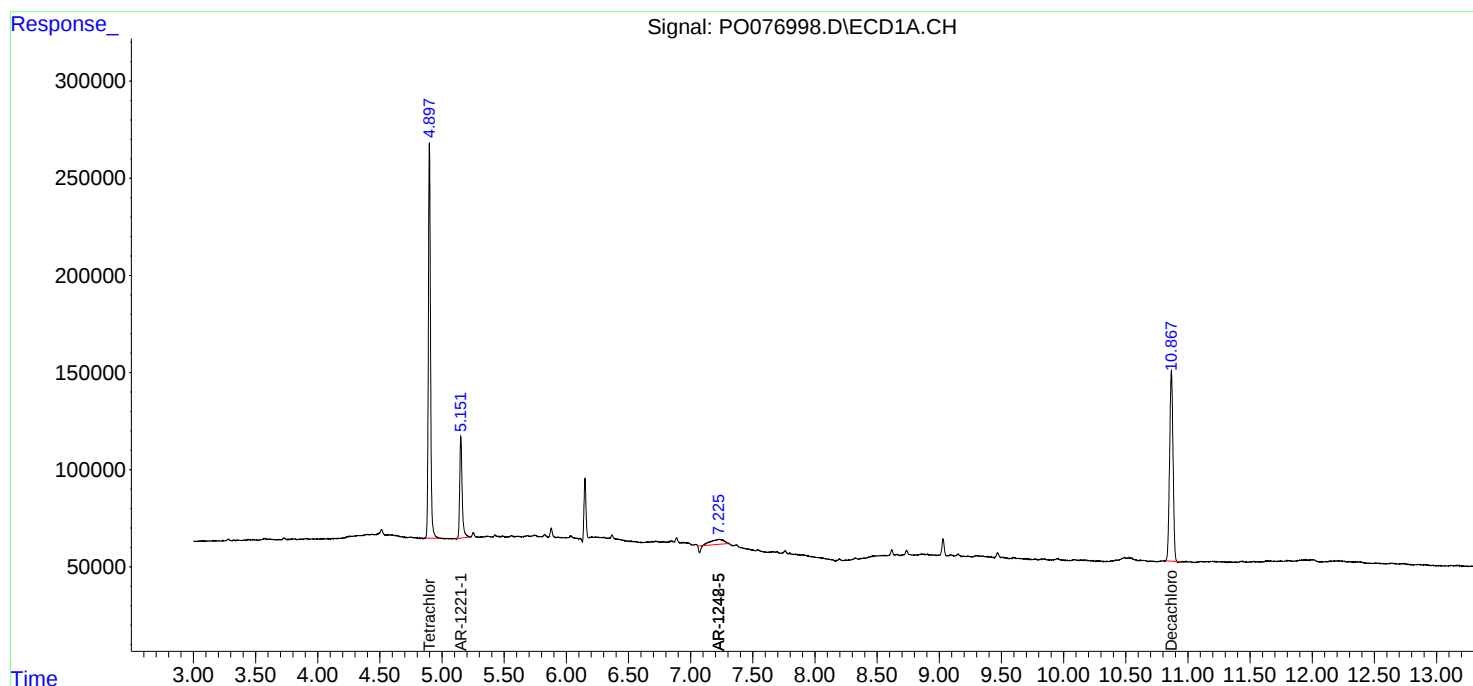


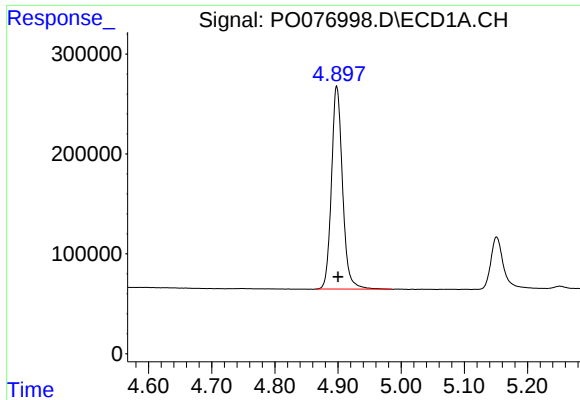

#1 Tetrachloro-m-xylene


R.T.: 4.898 min
Delta R.T.: -0.002 min
Response: 2476248
Conc: 26.62 ng/ml

Instrument :
ECD_O
ClientSampleId :

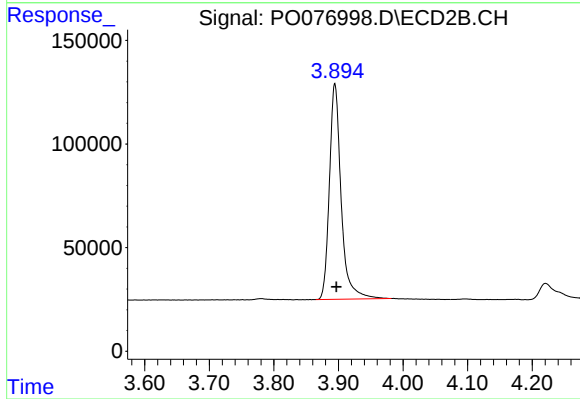


#1 Tetrachloro-m-xylene

R.T.: 3.894 min
Delta R.T.: -0.003 min
Response: 1314911
Conc: 26.20 ng/ml

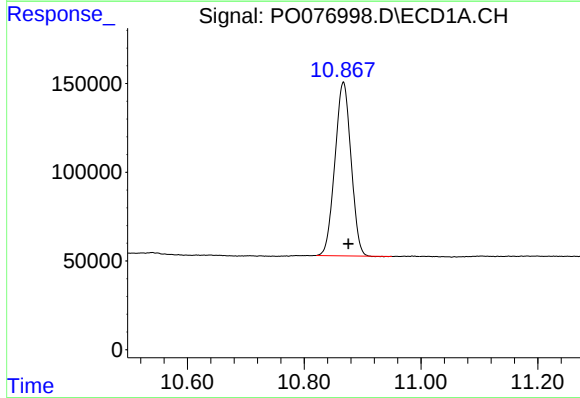


#2 Decachlorobiphenyl

R.T.: 10.867 min
Delta R.T.: -0.009 min
Response: 1868368
Conc: 20.17 ng/ml

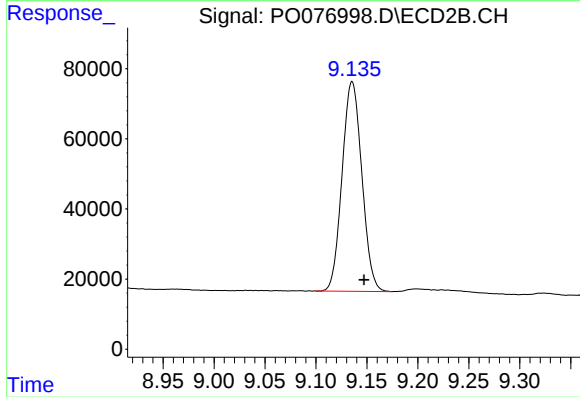

#2 Decachlorobiphenyl


R.T.: 9.136 min
Delta R.T.: -0.012 min
Response: 807922
Conc: 16.65 ng/ml

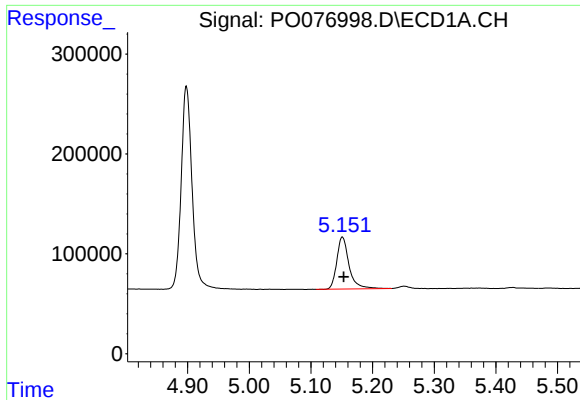

#8 AR-1221-1


R.T.: 5.151 min
Delta R.T.: -0.002 min
Response: 718883
Conc: 794.55 ng/ml

Instrument :
ECD_O
ClientSampleId :

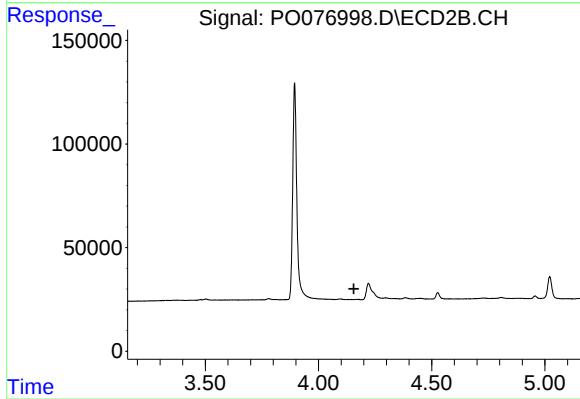


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.157 min
Response: 0
Conc: N.D.

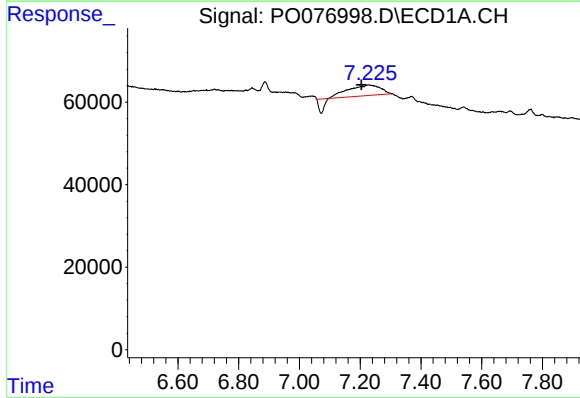


#20 AR-1242-5

R.T.: 7.227 min
Delta R.T.: 0.023 min
Response: 154084
Conc: 78.71 ng/ml

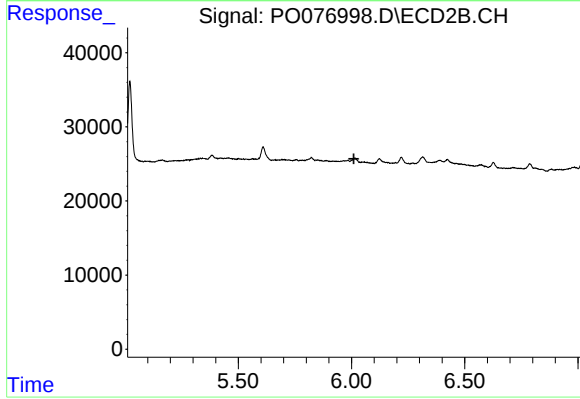

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 6.011 min
Response: 0
Conc: N.D.

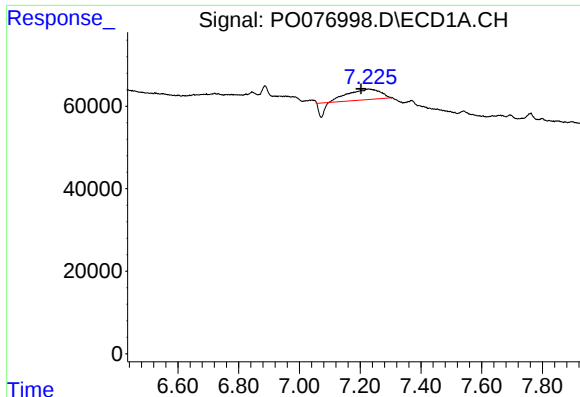

#25 AR-1248-5


R.T.: 7.227 min
Delta R.T.: 0.024 min
Response: 154084
Conc: 44.71 ng/ml

Instrument :
ECD_O
ClientSampleId :

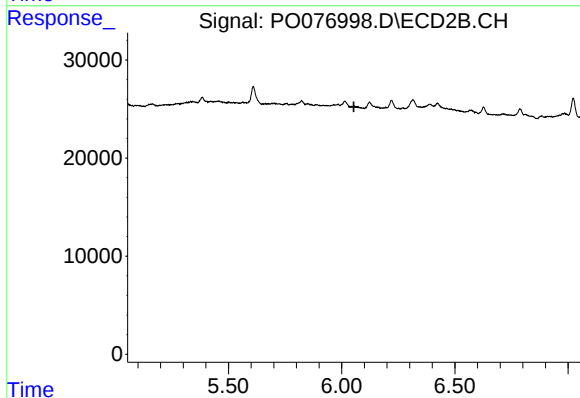


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 6.054 min
Response: 0
Conc: N.D.

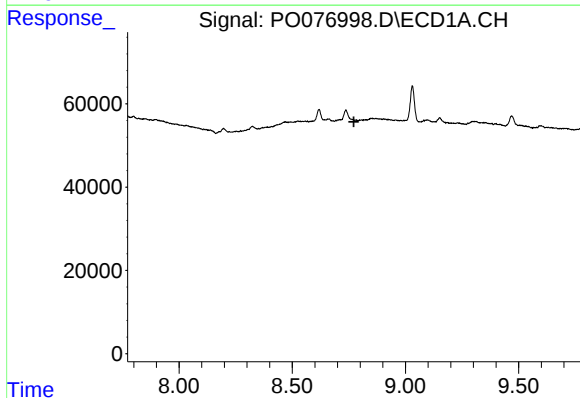


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 8.772 min
Response: 0
Conc: N.D.

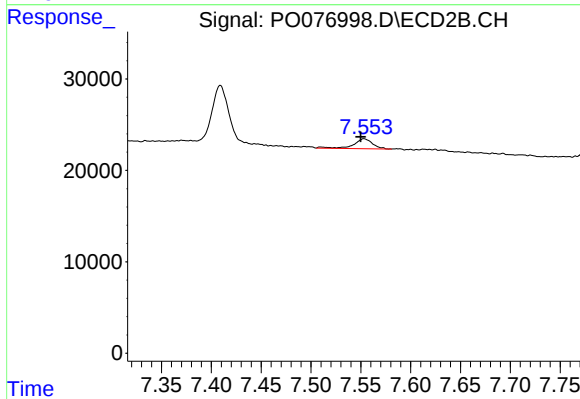

#34 AR-1260-4


R.T.: 7.553 min
Delta R.T.: 0.003 min
Response: 14207
Conc: 5.68 ng/ml

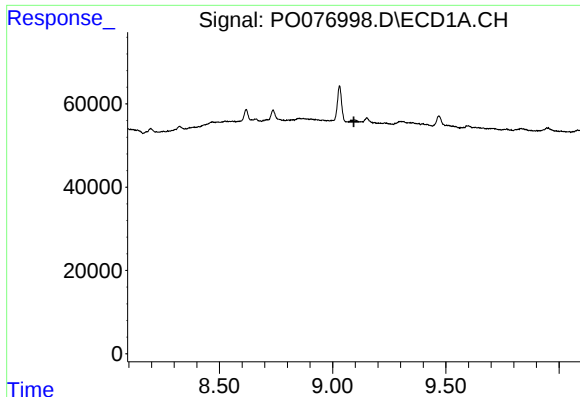

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 9.094 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

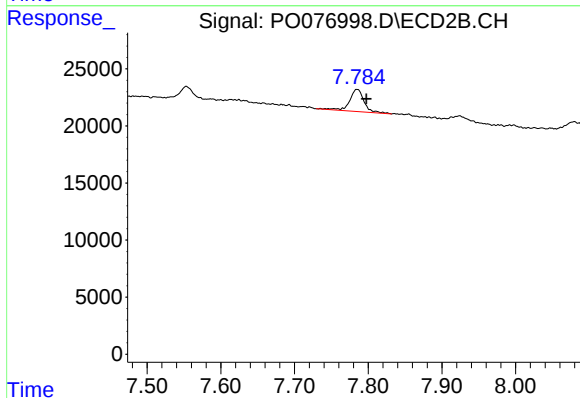


#35 AR-1260-5

R.T.: 7.785 min
Delta R.T.: -0.013 min
Response: 26695
Conc: 4.53 ng/ml

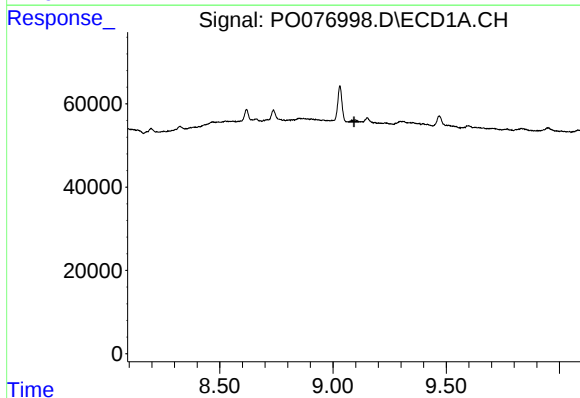


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 9.093 min
Response: 0
Conc: N.D.

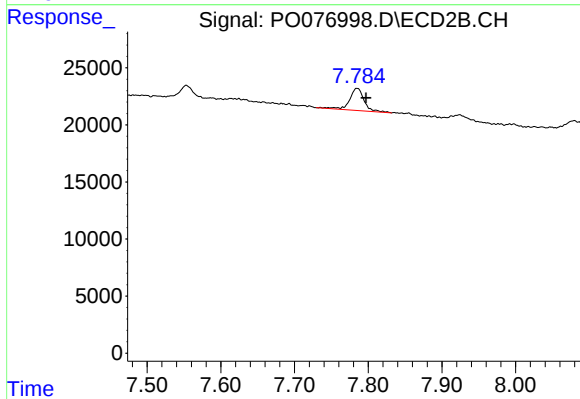

#37 AR-1262-2


R.T.: 7.785 min
Delta R.T.: -0.013 min
Response: 26695
Conc: 4.41 ng/ml

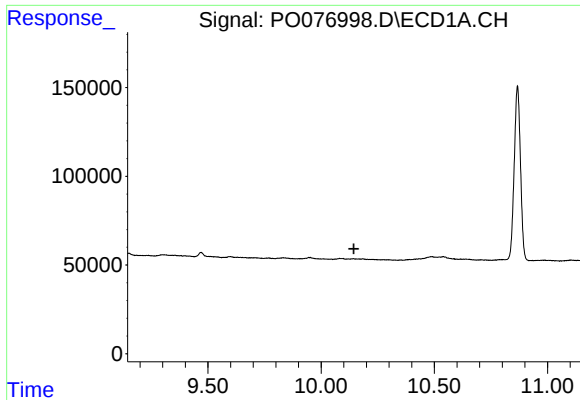

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 10.144 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

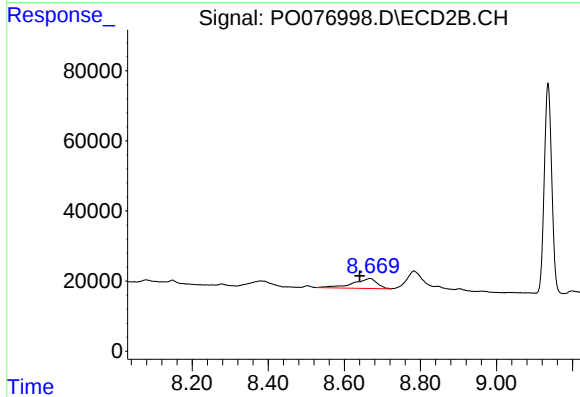


#40 AR-1262-5

R.T.: 8.669 min
Delta R.T.: 0.028 min
Response: 123759
Conc: 62.49 ng/ml

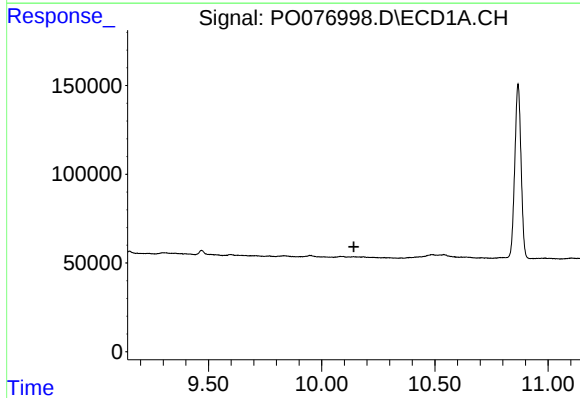

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 10.142 min
Response: 0
Conc: N.D.

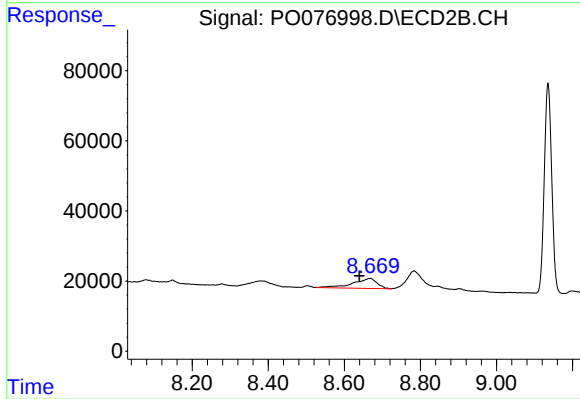

#44 AR-1268-4

R.T.: 8.669 min
Delta R.T.: 0.029 min
Response: 123759
Conc: 56.03 ng/ml