

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041521\
 Data File : P0077006.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Apr 2021 14:56
 Operator : AJ/MA
 Sample : M2048-18
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 15:36:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 02 05:20:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.900	3.896	2291628	1214059	24.638	24.193
2) SA Decachlor...	10.870	9.139	1642176	712256	17.730	14.678
Target Compounds						
8) L2 AR-1221-1	5.153	0.000	245317	0	271.139	N.D. #
9) L2 AR-1221-2	0.000	4.242	0	22515	N.D.	63.844 #
31) L7 AR-1260-1	0.000	6.716	0	13369	N.D.	5.116 #
32) L7 AR-1260-2	0.000	6.910	0	8016	N.D.	2.539 #
40) L8 AR-1262-5	0.000	8.663f	0	73654	N.D.	37.189 #
43) L9 AR-1268-3	0.000	8.377f	0	44024	N.D.	7.600 #
44) L9 AR-1268-4	0.000	8.663f	0	73654	N.D.	33.346 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041521\
Data File : P0077006.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Apr 2021 14:56
Operator : AJ/MA
Sample : M2048-18
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 15:36:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 02 05:20:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

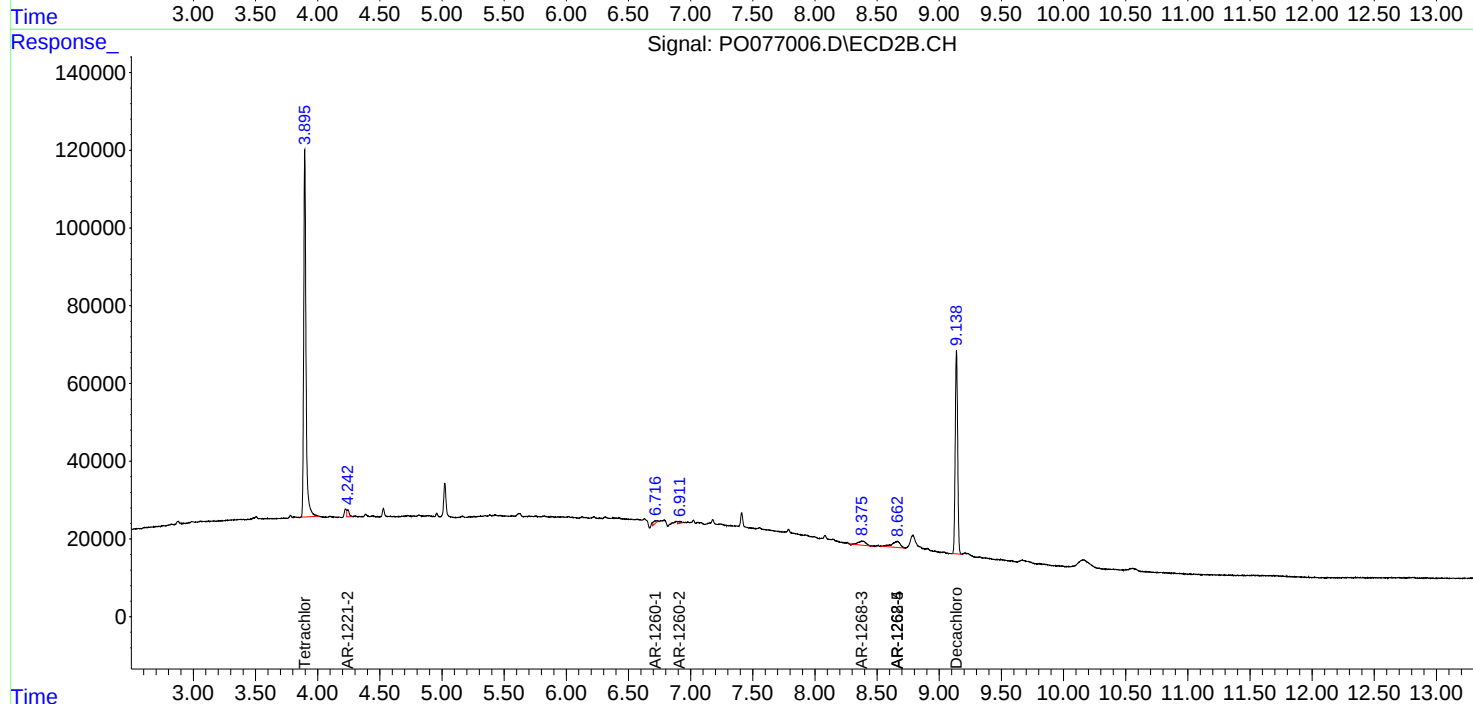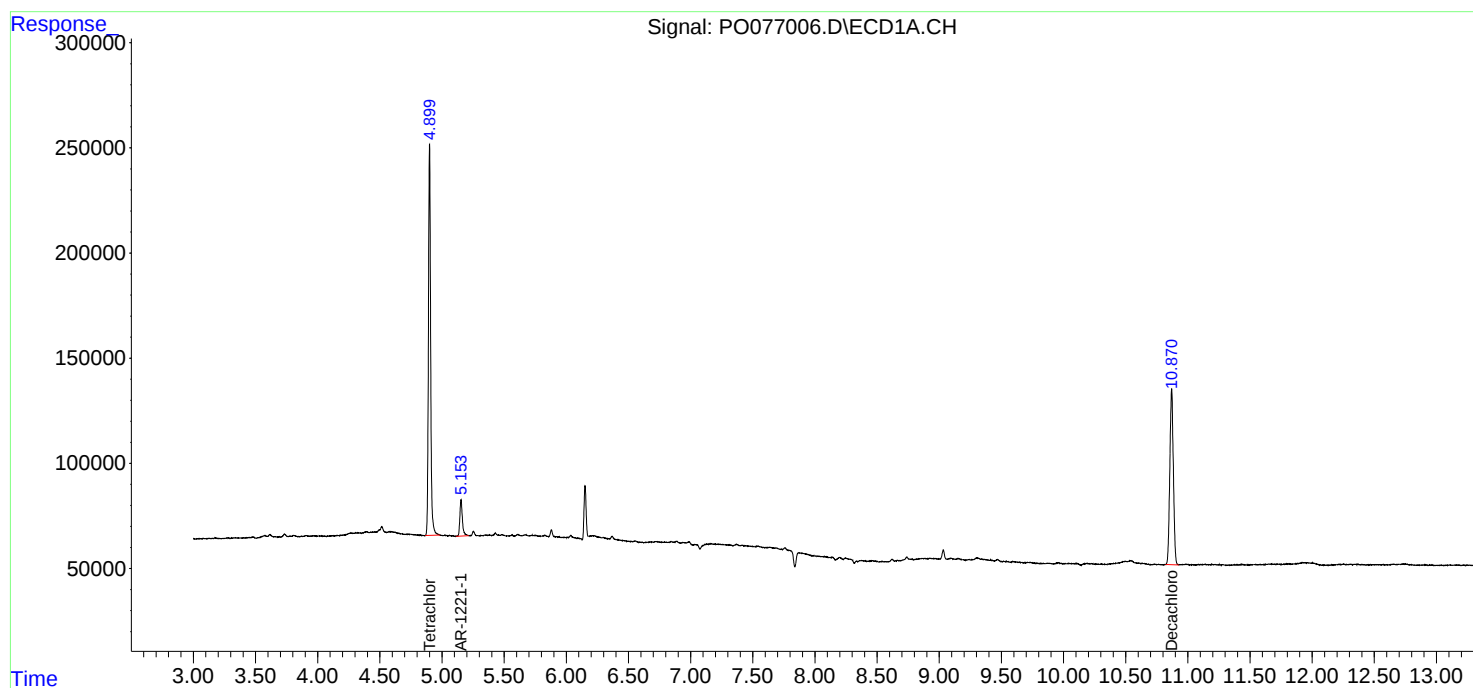


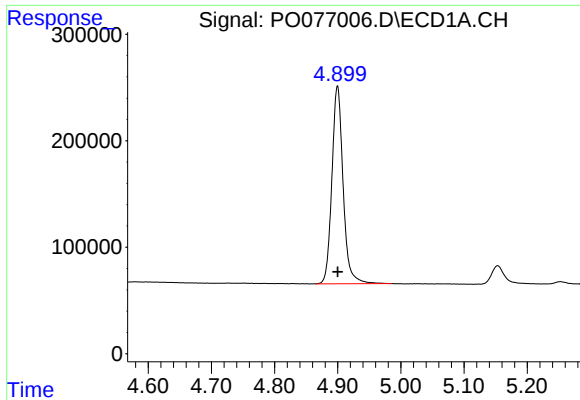

#1 Tetrachloro-m-xylene


R.T.: 4.900 min
Delta R.T.: 0.000 min
Response: 2291628
Conc: 24.64 ng/ml

Instrument :
ECD_O
ClientSampleId :

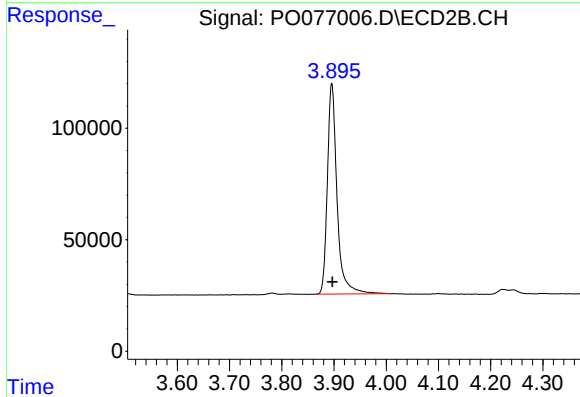


#1 Tetrachloro-m-xylene

R.T.: 3.896 min
Delta R.T.: -0.001 min
Response: 1214059
Conc: 24.19 ng/ml

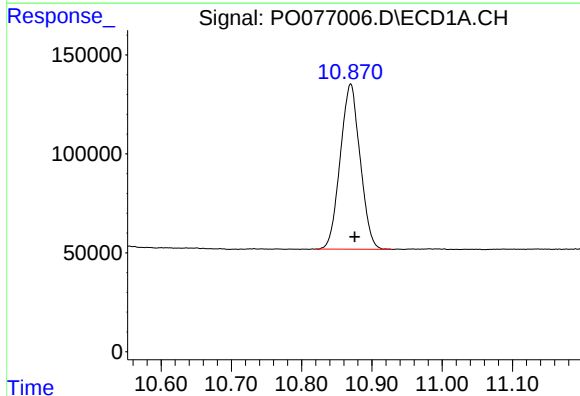


#2 Decachlorobiphenyl

R.T.: 10.870 min
Delta R.T.: -0.006 min
Response: 1642176
Conc: 17.73 ng/ml

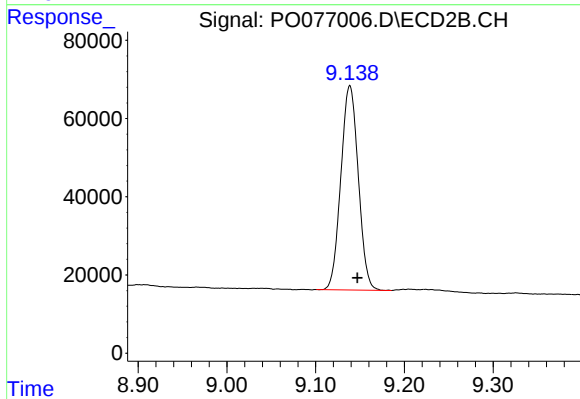

#2 Decachlorobiphenyl


R.T.: 9.139 min
Delta R.T.: -0.009 min
Response: 712256
Conc: 14.68 ng/ml

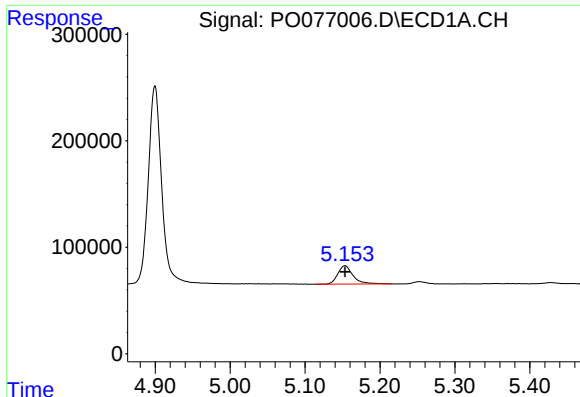

#8 AR-1221-1


R.T.: 5.153 min
Delta R.T.: 0.000 min
Response: 245317
Conc: 271.14 ng/ml

Instrument :
ECD_O
ClientSampleId :

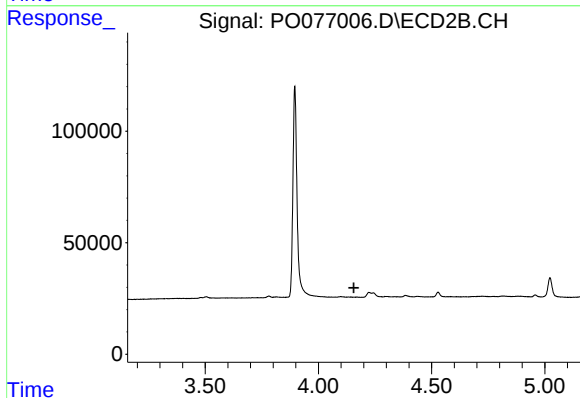


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.157 min
Response: 0
Conc: N.D.

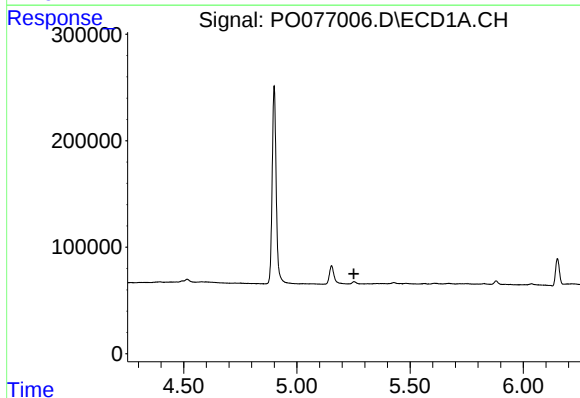


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 5.251 min
Response: 0
Conc: N.D.

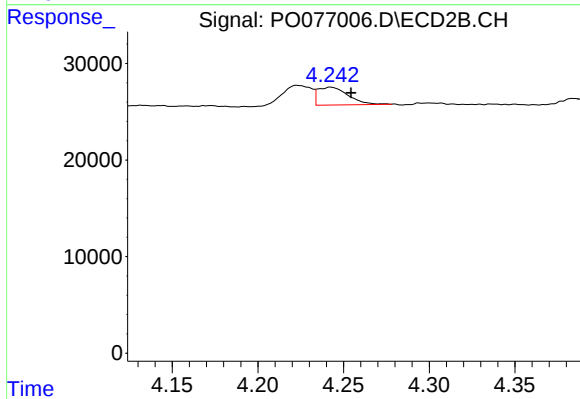

#9 AR-1221-2


R.T.: 4.242 min
Delta R.T.: -0.012 min
Response: 22515
Conc: 63.84 ng/ml

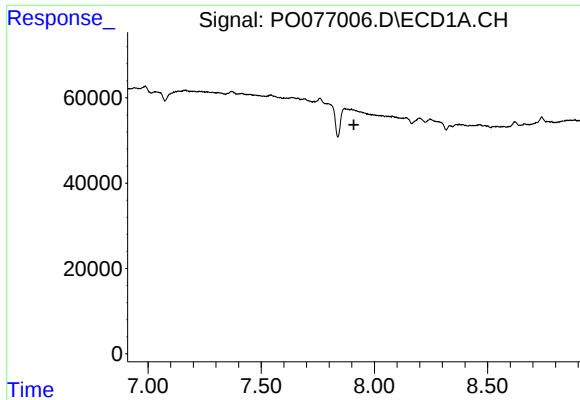

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T. : 7.909 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

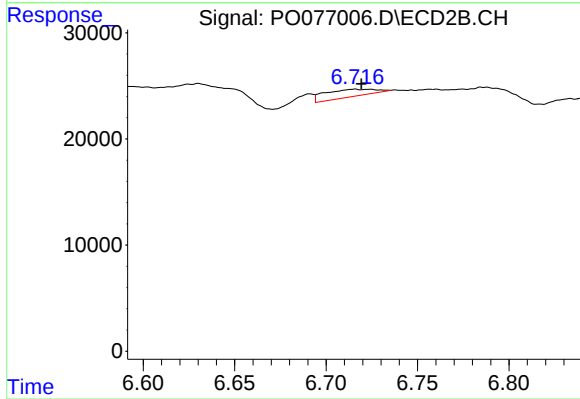


#31 AR-1260-1

R.T.: 6.716 min
Delta R.T.: -0.003 min
Response: 13369
Conc: 5.12 ng/ml

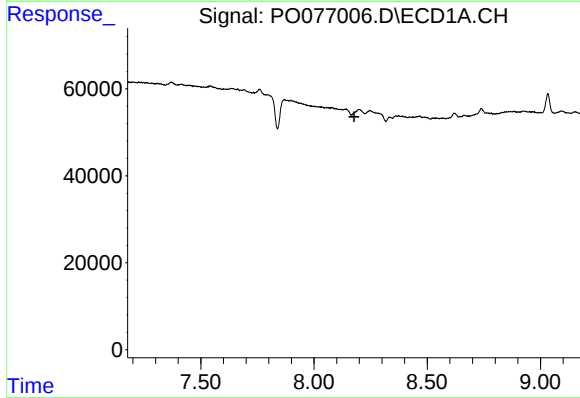


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 8.176 min
Response: 0
Conc: N.D.

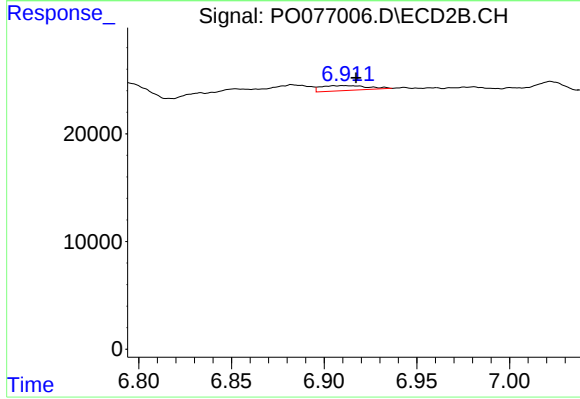

#32 AR-1260-2


R.T.: 6.910 min
Delta R.T.: -0.007 min
Response: 8016
Conc: 2.54 ng/ml

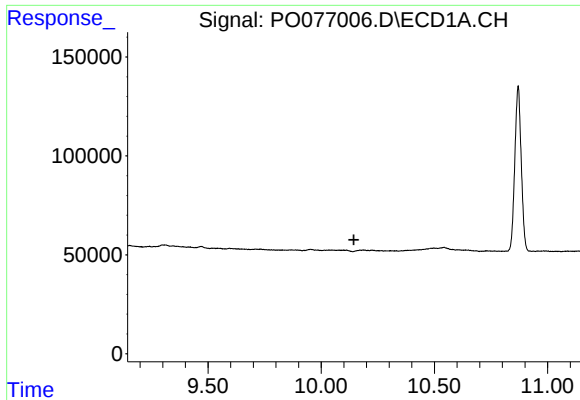

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 10.144 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

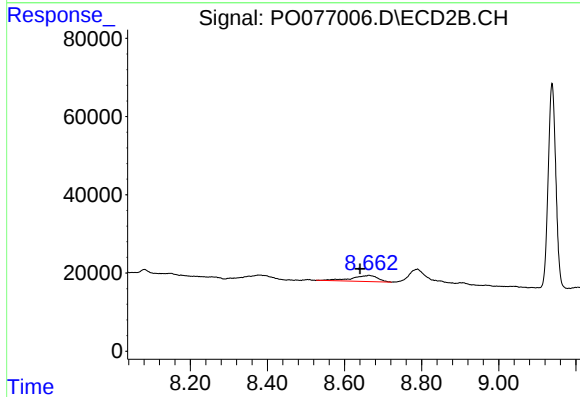


#40 AR-1262-5

R.T.: 8.663 min
Delta R.T.: 0.023 min
Response: 73654
Conc: 37.19 ng/ml

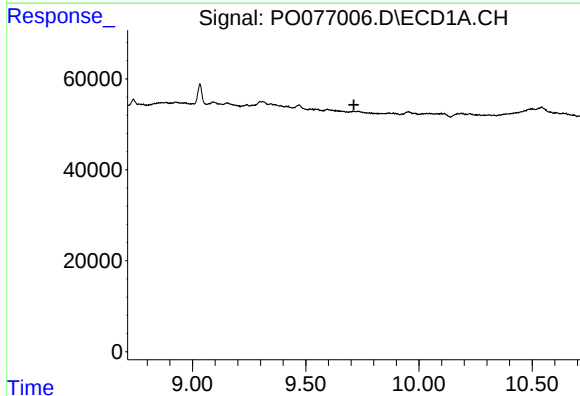


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 9.713 min
Response: 0
Conc: N.D.

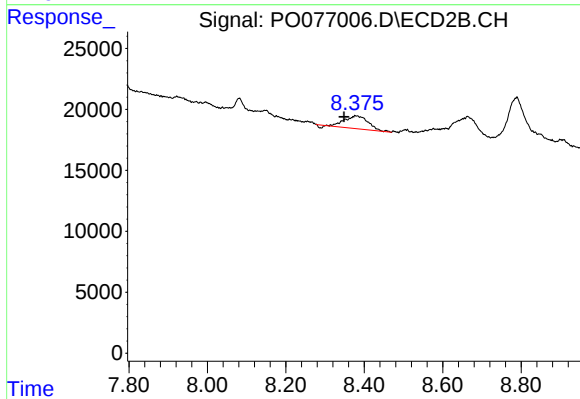

#43 AR-1268-3


R.T.: 8.377 min
Delta R.T.: 0.028 min
Response: 44024
Conc: 7.60 ng/ml

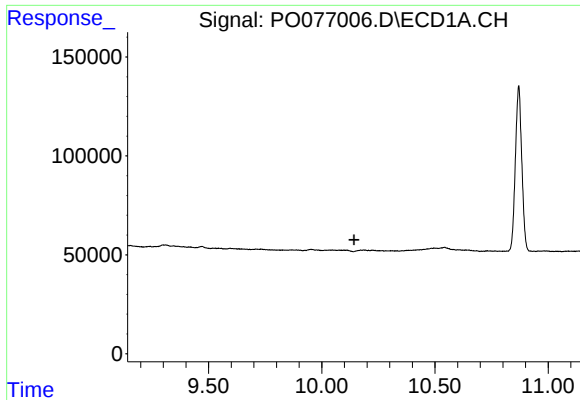

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 10.142 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

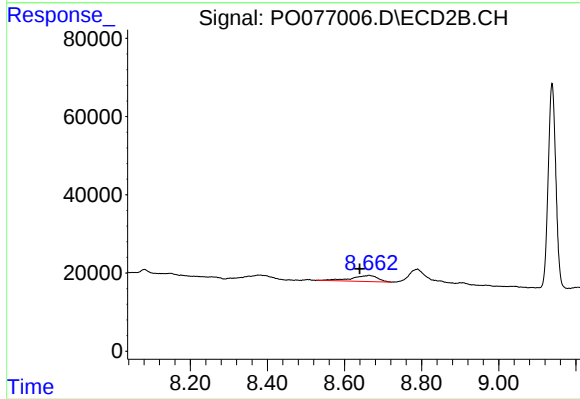

#44 AR-1268-4

R.T.: 8.663 min
Delta R.T.: 0.024 min
Response: 73654
Conc: 33.35 ng/ml