

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0041521\
 Data File : P0076997.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Apr 2021 12:21
 Operator : AJ/MA
 Sample : M2048-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-02-0-2.0

Manual Integrations
 APPROVED

Ankita
 4/16/2021 3:23:57 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 10:58:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0040121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 02 05:20:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.898	3.894	2539264	1329114	27.300	26.486
2) SA Decachlor...	10.868	9.136	2574043	1094005	27.791	22.545
Target Compounds						
31) L7 AR-1260-1	7.900	6.708	153204	224373	38.255m	85.869 #
32) L7 AR-1260-2	8.171	6.915	309521	353468	62.488	111.939 #
33) L7 AR-1260-3	8.536	7.061	296640	103676	76.394	35.486 #
34) L7 AR-1260-4	8.766	7.539	308985	157581	71.743	62.991
35) L7 AR-1260-5	9.089	7.787	293349	361456	34.423	61.278 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041521\
Data File : P0076997.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Apr 2021 12:21
Operator : AJ/MA
Sample : M2048-04
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-02-0-2.0


Manual Integrations
APPROVED

Ankita
4/16/2021 3:23:57 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 10:58:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 02 05:20:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

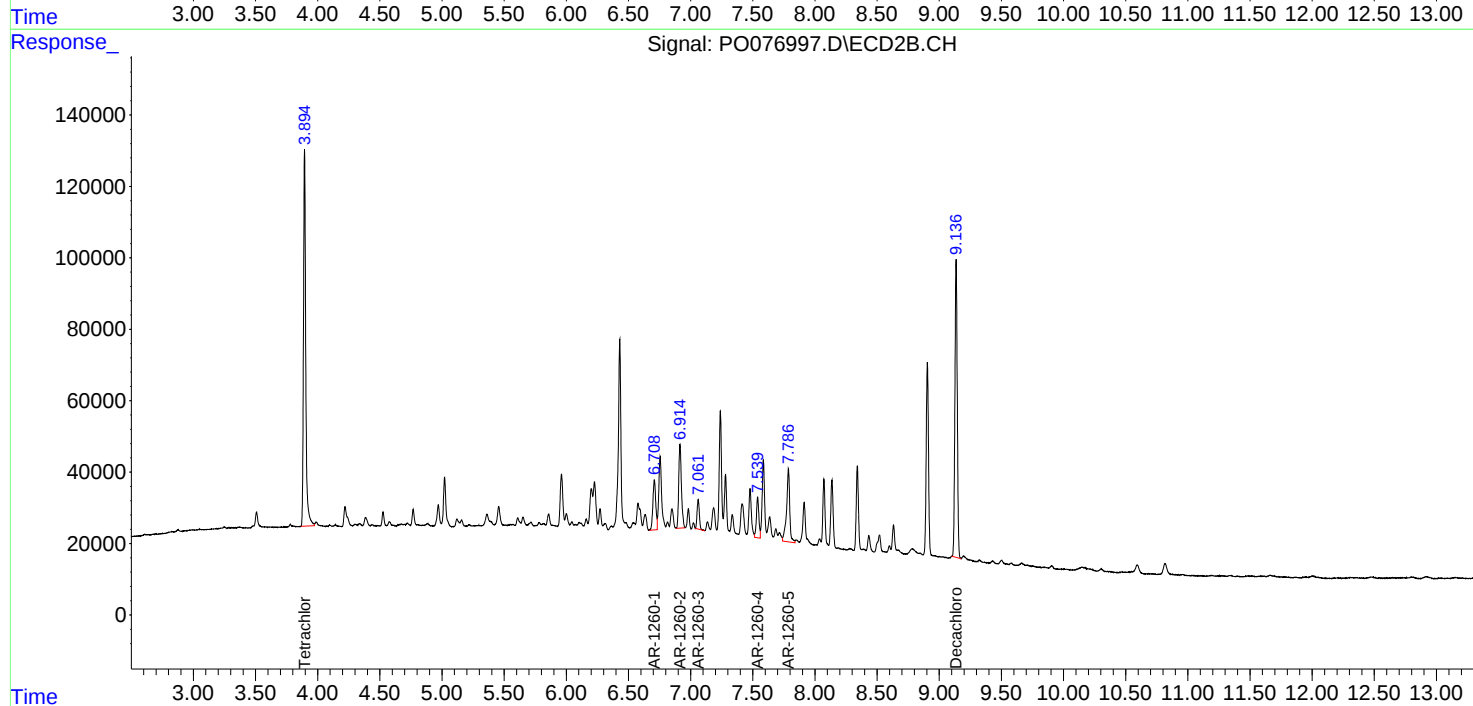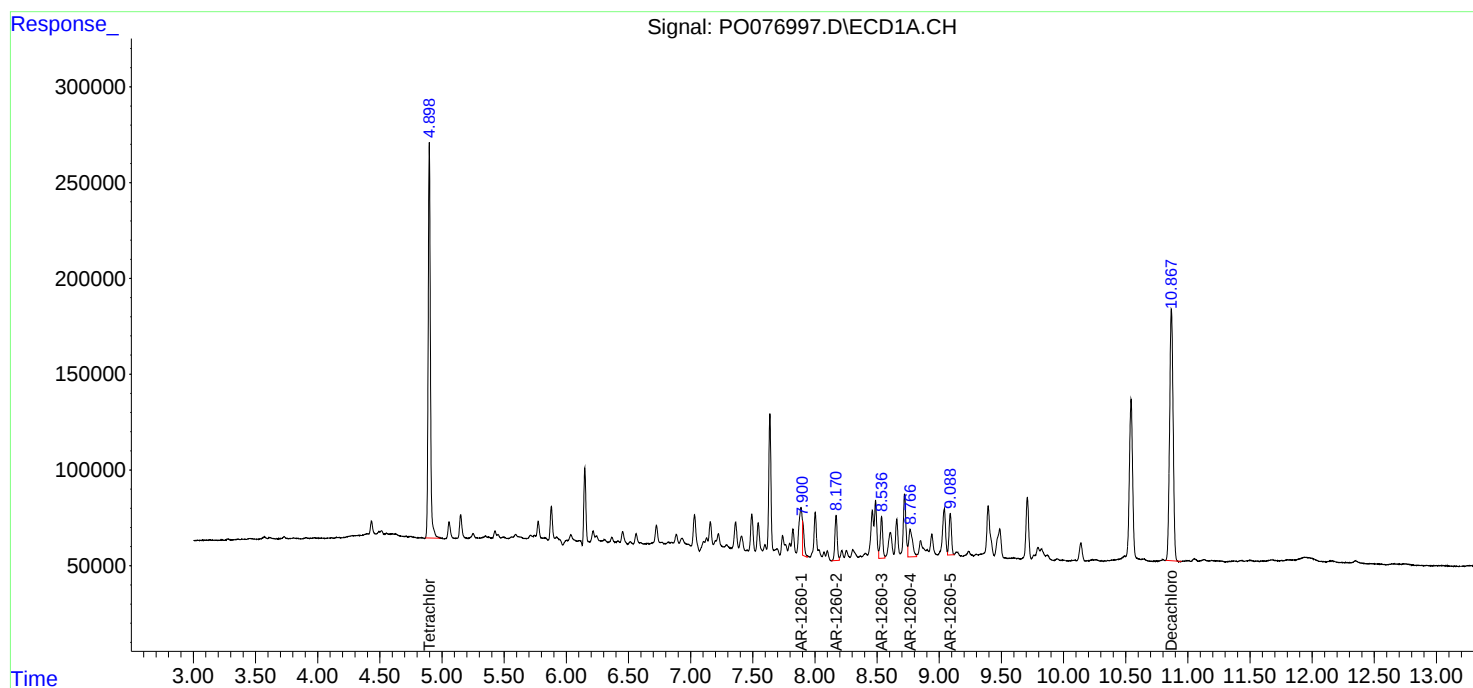

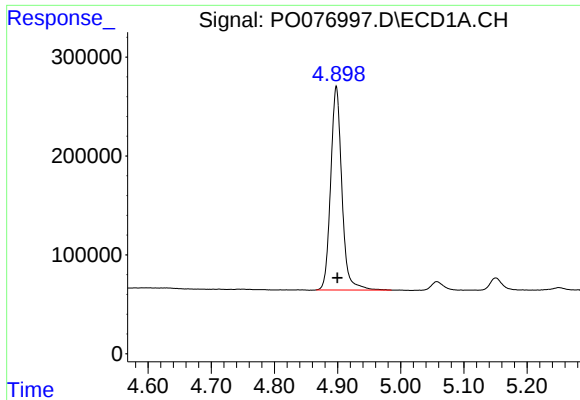


#1 Tetrachloro-m-xylene

R.T.: 4.898 min
Delta R.T.: -0.002 min
Response: 2539264
Conc: 27.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-02-0-2.0


Manual Integrations
APPROVED

Ankita
4/16/2021 3:23:57 PM

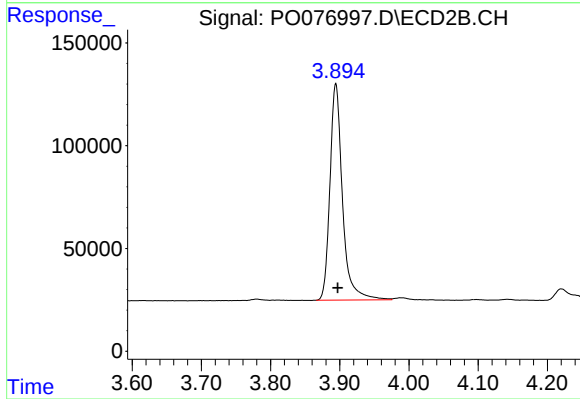


#1 Tetrachloro-m-xylene

R.T.: 3.894 min
Delta R.T.: -0.003 min
Response: 1329114
Conc: 26.49 ng/ml

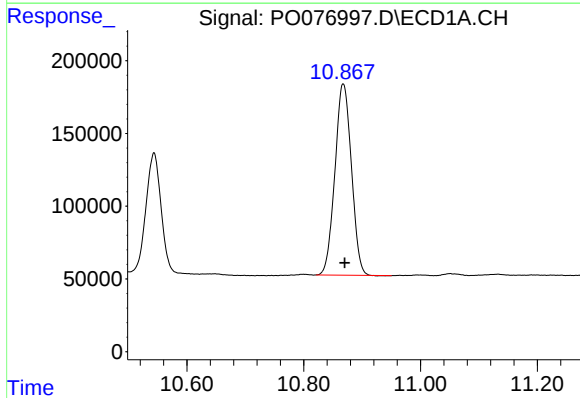


#2 Decachlorobiphenyl

R.T.: 10.868 min
Delta R.T.: -0.002 min
Response: 2574043
Conc: 27.79 ng/ml

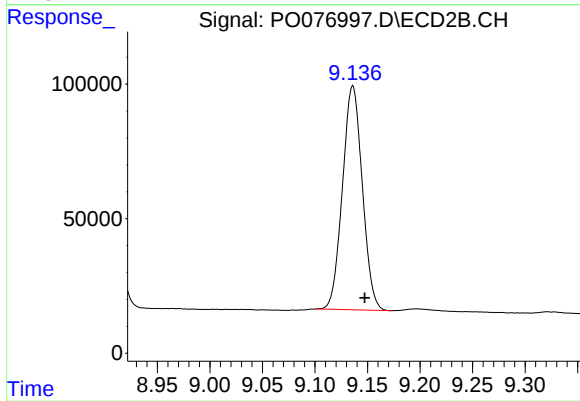

#2 Decachlorobiphenyl

R.T.: 9.136 min
Delta R.T.: -0.011 min
Response: 1094005
Conc: 22.54 ng/ml

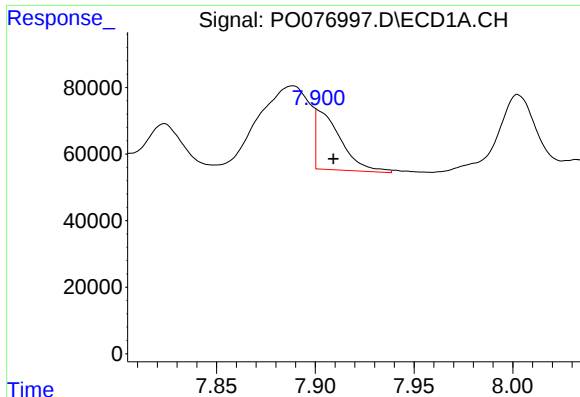


#31 AR-1260-1

R.T.: 7.900 min
Delta R.T.: -0.009 min
Response: 153204
Conc: 38.26 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SB-02-0-2.0


Manual Integrations
APPROVED

Ankita
4/16/2021 3:23:57 PM

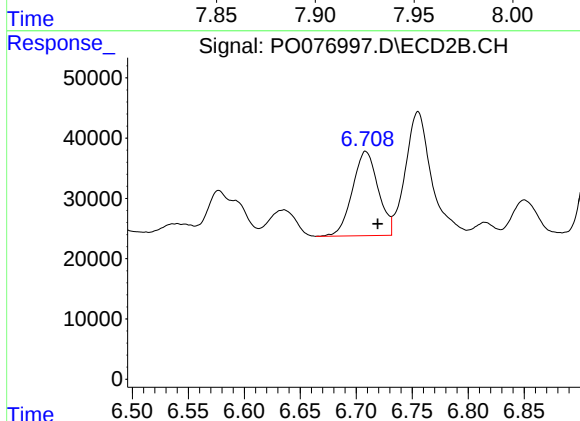


#31 AR-1260-1

R.T.: 6.708 min
Delta R.T.: -0.011 min
Response: 224373
Conc: 85.87 ng/ml

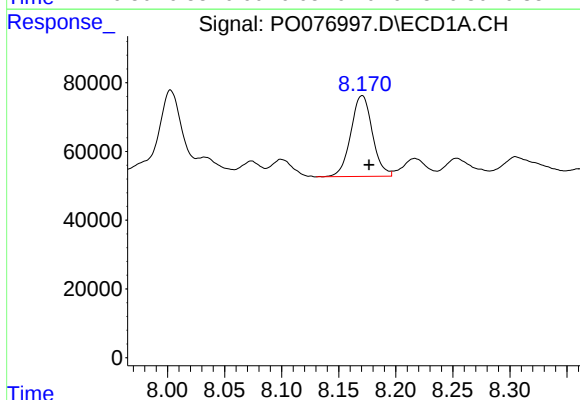


#32 AR-1260-2

R.T.: 8.171 min
Delta R.T.: -0.006 min
Response: 309521
Conc: 62.49 ng/ml

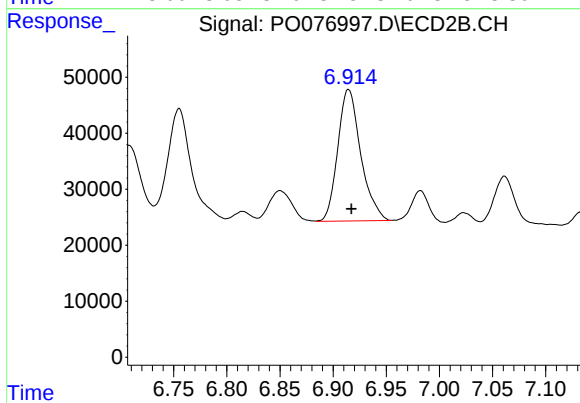

#32 AR-1260-2

R.T.: 6.915 min
Delta R.T.: -0.003 min
Response: 353468
Conc: 111.94 ng/ml

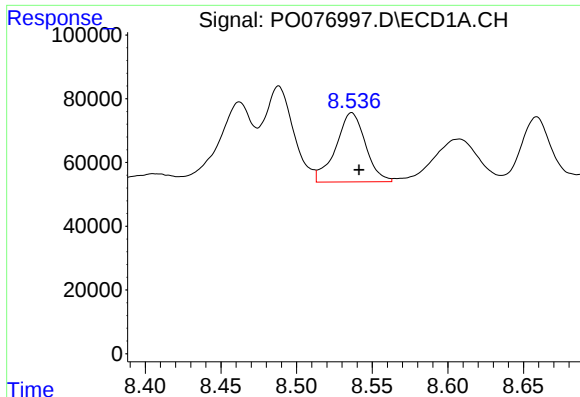


#33 AR-1260-3

R.T.: 8.536 min
Delta R.T.: -0.005 min
Response: 296640
Conc: 76.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-02-0-2.0


Manual Integrations
APPROVED

Ankita
4/16/2021 3:23:57 PM

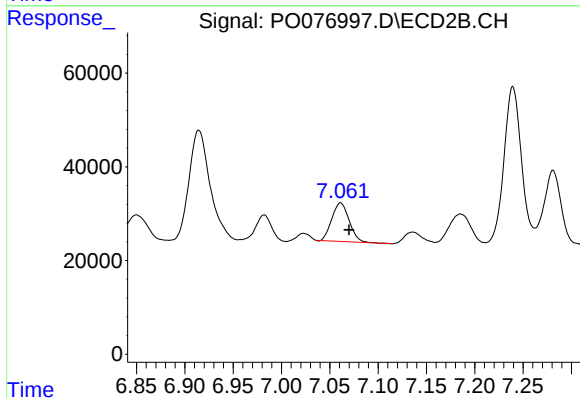


#33 AR-1260-3

R.T.: 7.061 min
Delta R.T.: -0.009 min
Response: 103676
Conc: 35.49 ng/ml

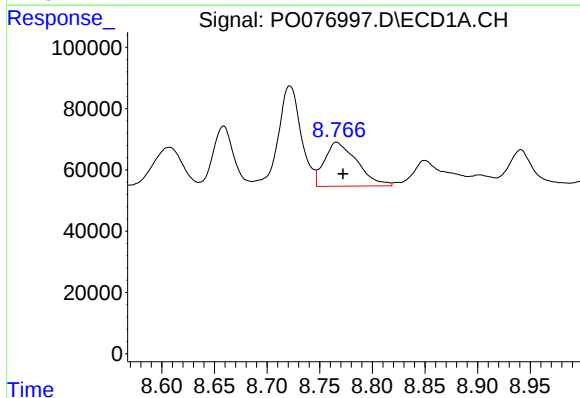


#34 AR-1260-4

R.T.: 8.766 min
Delta R.T.: -0.006 min
Response: 308985
Conc: 71.74 ng/ml

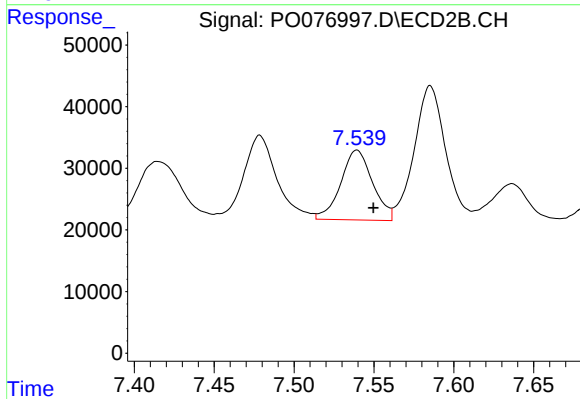

#34 AR-1260-4

R.T.: 7.539 min
Delta R.T.: -0.010 min
Response: 157581
Conc: 62.99 ng/ml

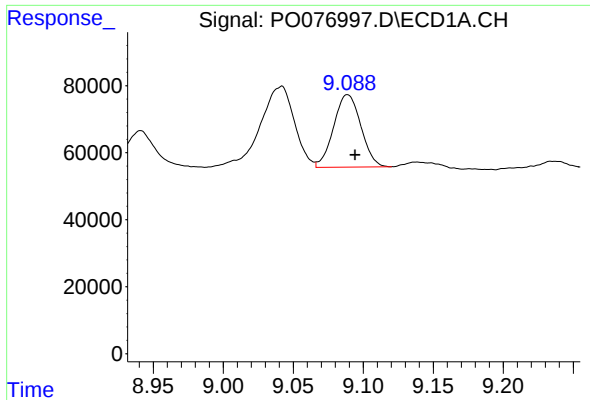


#35 AR-1260-5

R.T.: 9.089 min
Delta R.T.: -0.005 min
Response: 293349
Conc: 34.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-02-0-2.0

Manual Integrations
APPROVED

Ankita
4/16/2021 3:23:57 PM

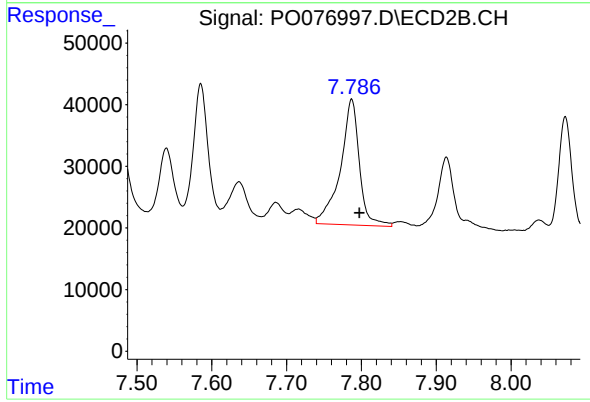

#35 AR-1260-5

R.T.: 7.787 min
Delta R.T.: -0.010 min
Response: 361456
Conc: 61.28 ng/ml