

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041521\
 Data File : P0077001.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Apr 2021 13:30
 Operator : AJ/MA
 Sample : M2048-10
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-04-0-2.0

Manual Integrations
 APPROVED

Ankita
 4/16/2021 3:24:02 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 15:33:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 02 05:20:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.898	3.895	2545025	1330044	27.362	26.504
2) SA Decachlor...	10.865	9.136	2078974	893478	22.446	18.412
Target Compounds						
31) L7 AR-1260-1	7.904	6.711	156302	135300	39.029m	51.781 #
32) L7 AR-1260-2	8.170	6.912	156179	154632	31.530	48.970 #
33) L7 AR-1260-3	8.535	7.060	121356	64909	31.253	22.217 #
34) L7 AR-1260-4	8.765	7.540	150472	80047	34.938	31.998
35) L7 AR-1260-5	9.088	7.788	186167	193180	21.846	32.750 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041521\
Data File : P0077001.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Apr 2021 13:30
Operator : AJ/MA
Sample : M2048-10
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
SB-04-0-2.0


Manual Integrations
APPROVED

Ankita
4/16/2021 3:24:02 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 15:33:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 02 05:20:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

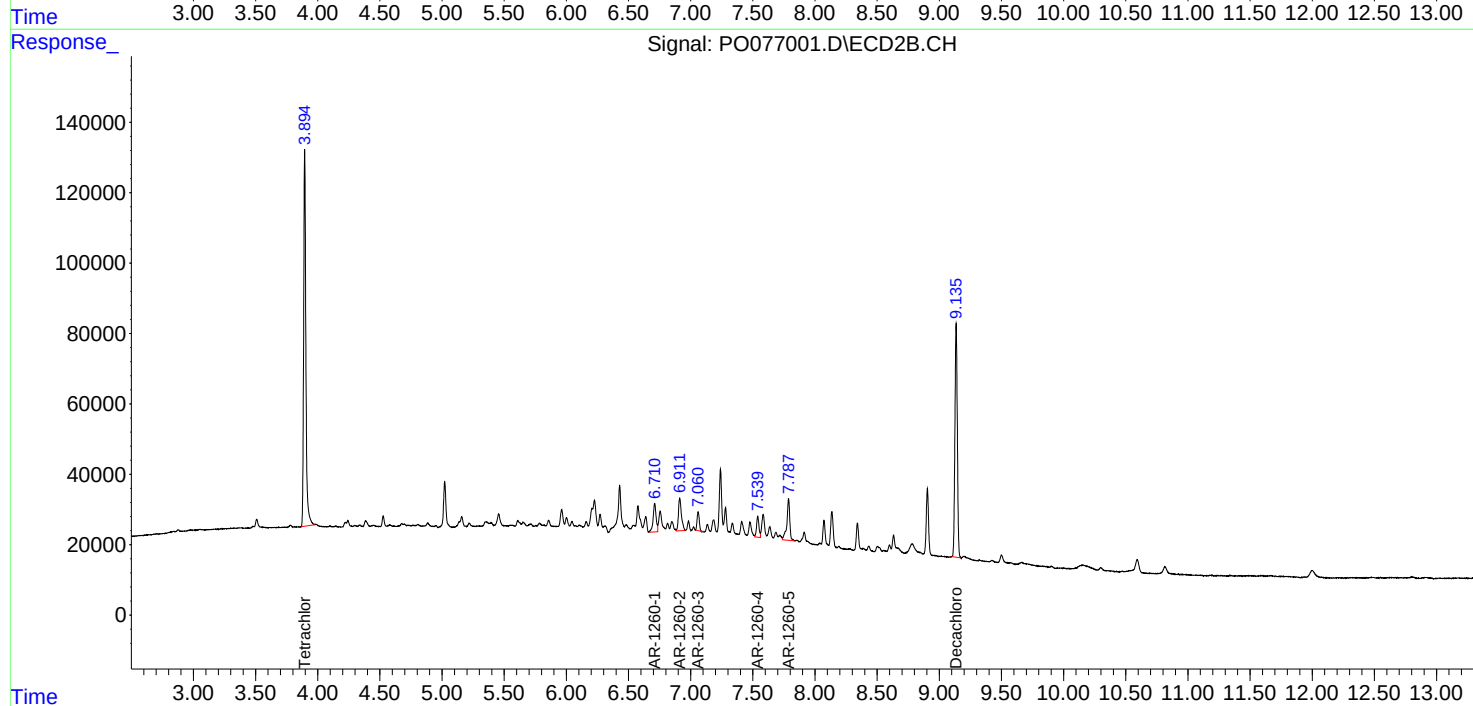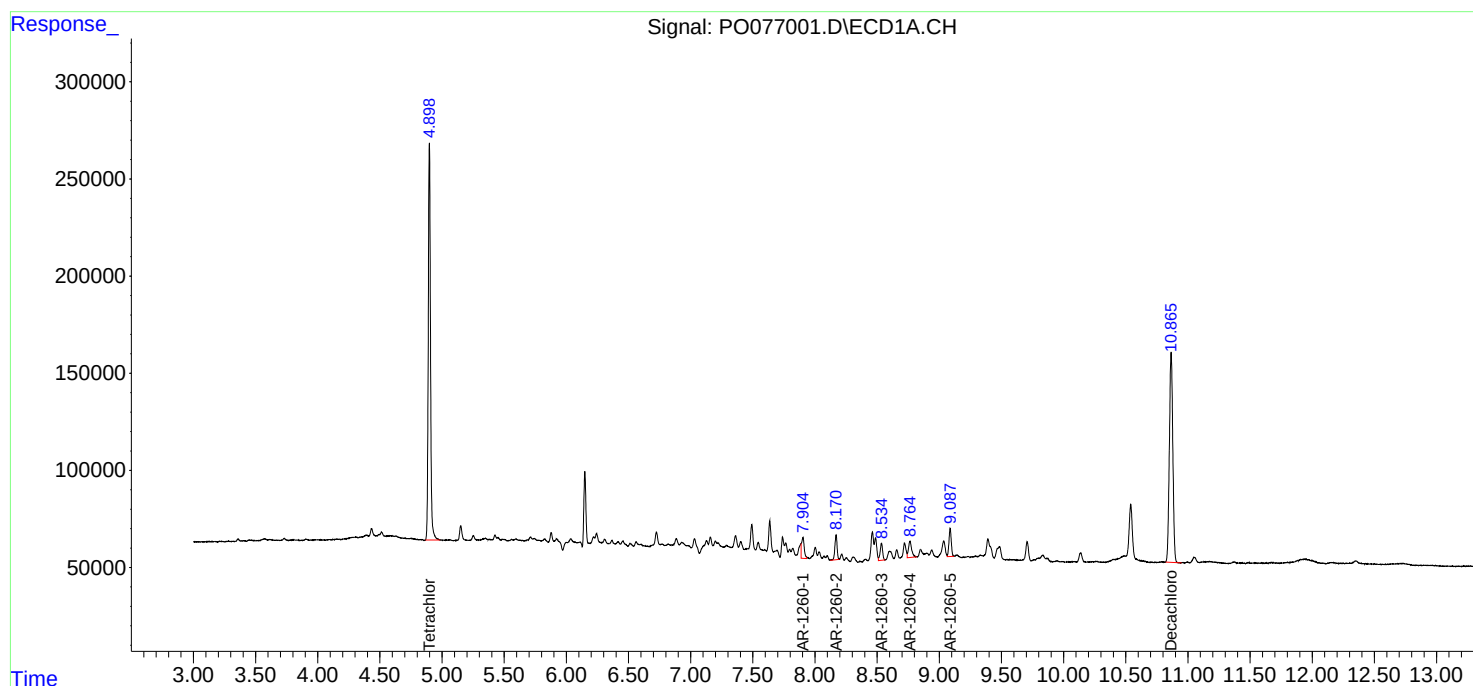

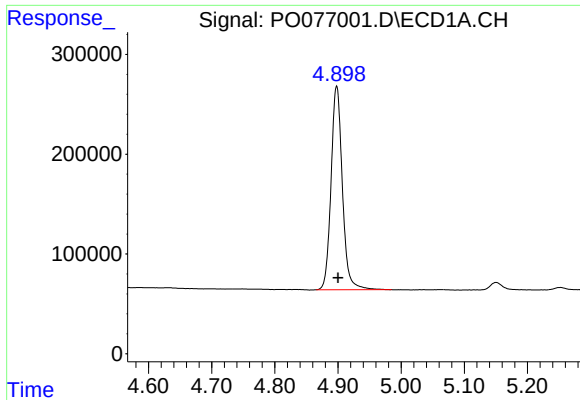


#1 Tetrachloro-m-xylene

R.T.: 4.898 min
Delta R.T.: -0.002 min
Response: 2545025
Conc: 27.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-04-0-2.0


Manual Integrations
APPROVED

Ankita
4/16/2021 3:24:02 PM

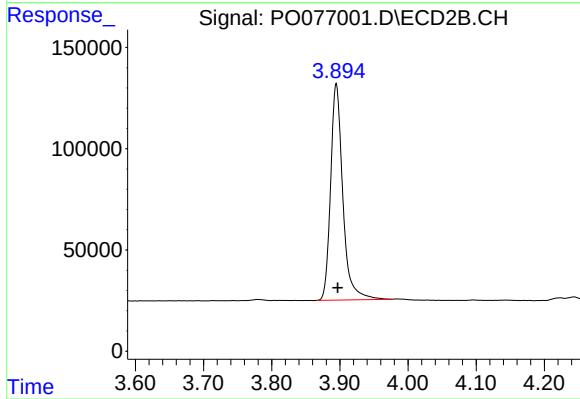


#1 Tetrachloro-m-xylene

R.T.: 3.895 min
Delta R.T.: -0.002 min
Response: 1330044
Conc: 26.50 ng/ml

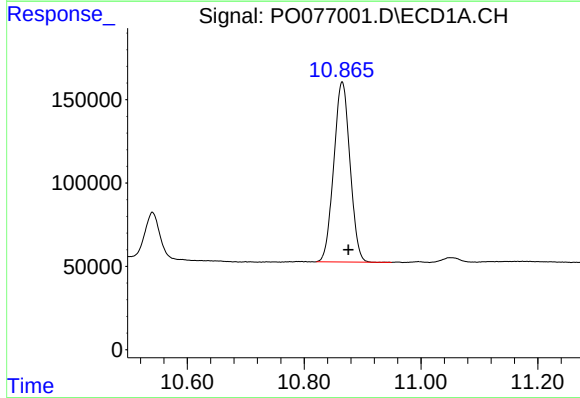


#2 Decachlorobiphenyl

R.T.: 10.865 min
Delta R.T.: -0.011 min
Response: 2078974
Conc: 22.45 ng/ml

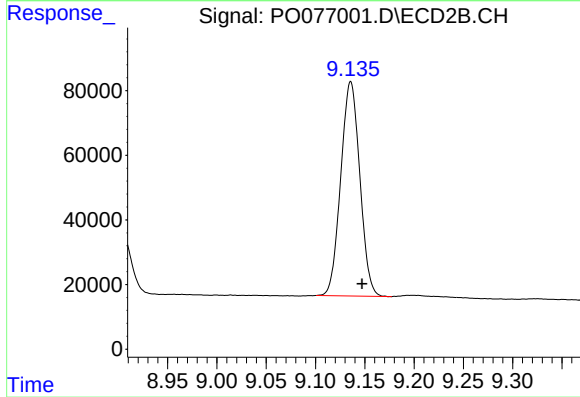

#2 Decachlorobiphenyl

R.T.: 9.136 min
Delta R.T.: -0.012 min
Response: 893478
Conc: 18.41 ng/ml

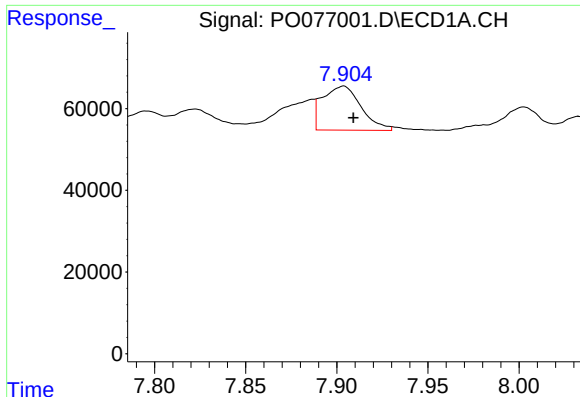


#31 AR-1260-1

R.T.: 7.904 min
Delta R.T.: -0.006 min
Response: 156302
Conc: 39.03 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SB-04-0-2.0


Manual Integrations
APPROVED

Ankita
4/16/2021 3:24:02 PM

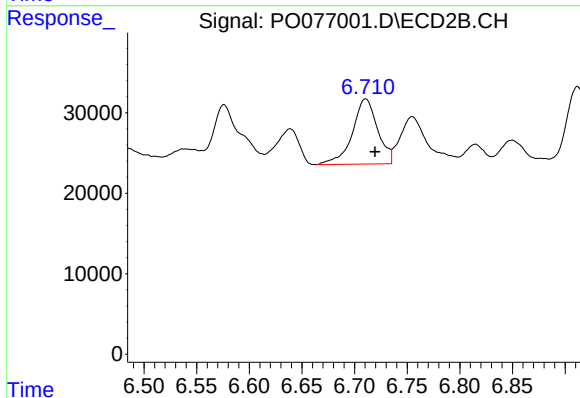


#31 AR-1260-1

R.T.: 6.711 min
Delta R.T.: -0.009 min
Response: 135300
Conc: 51.78 ng/ml

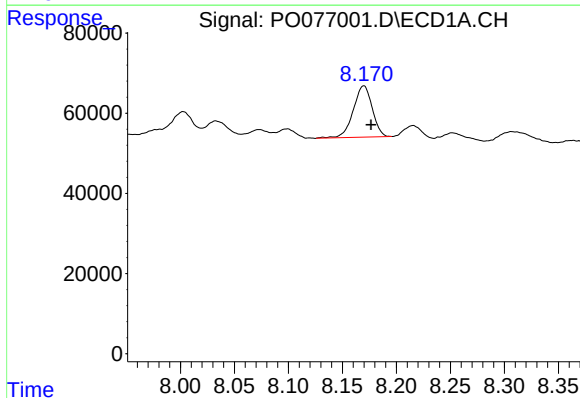


#32 AR-1260-2

R.T.: 8.170 min
Delta R.T.: -0.007 min
Response: 156179
Conc: 31.53 ng/ml

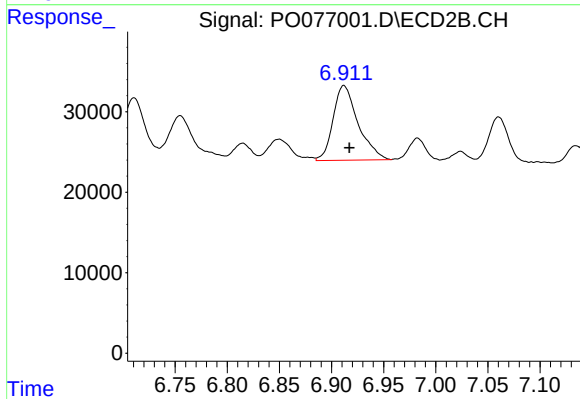

#32 AR-1260-2

R.T.: 6.912 min
Delta R.T.: -0.005 min
Response: 154632
Conc: 48.97 ng/ml

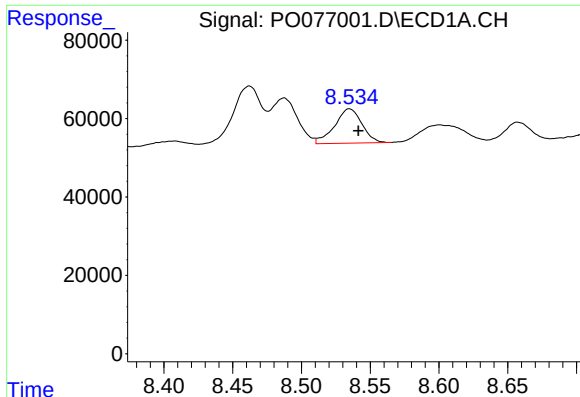


#33 AR-1260-3

R.T.: 8.535 min
Delta R.T.: -0.006 min
Response: 121356
Conc: 31.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-04-0-2.0


Manual Integrations
APPROVED

Ankita
4/16/2021 3:24:02 PM

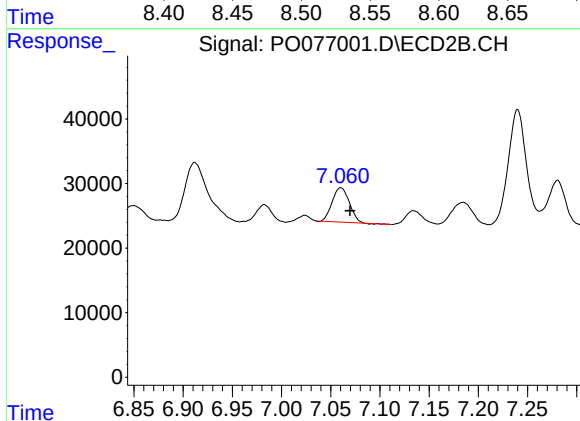


#33 AR-1260-3

R.T.: 7.060 min
Delta R.T.: -0.009 min
Response: 64909
Conc: 22.22 ng/ml

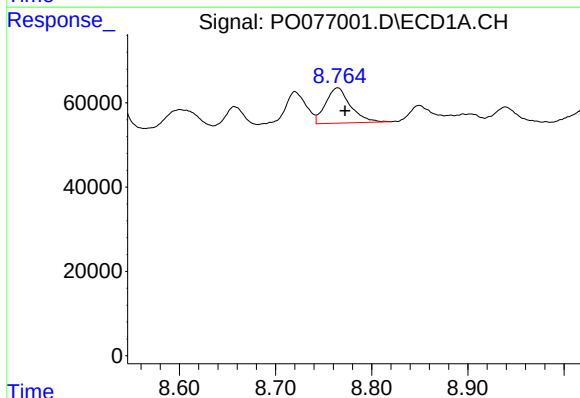


#34 AR-1260-4

R.T.: 8.765 min
Delta R.T.: -0.008 min
Response: 150472
Conc: 34.94 ng/ml

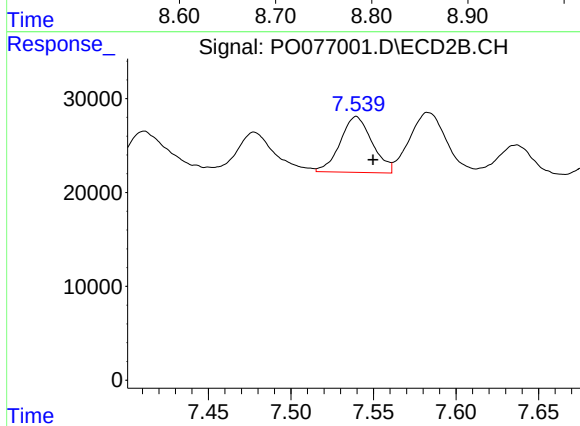

#34 AR-1260-4

R.T.: 7.540 min
Delta R.T.: -0.010 min
Response: 80047
Conc: 32.00 ng/ml

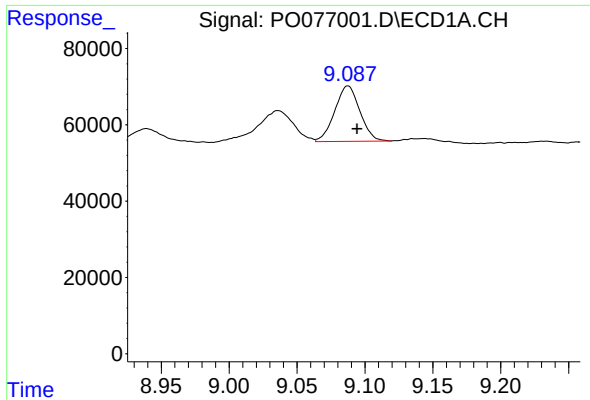


#35 AR-1260-5

R.T.: 9.088 min
Delta R.T.: -0.007 min
Response: 186167
Conc: 21.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-04-0-2.0

Manual Integrations
APPROVED

Ankita
4/16/2021 3:24:02 PM

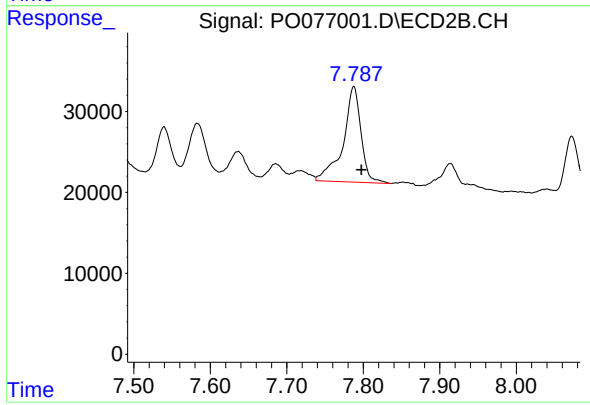

#35 AR-1260-5

R.T.: 7.788 min
Delta R.T.: -0.010 min
Response: 193180
Conc: 32.75 ng/ml