

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041521\
 Data File : P0077013.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Apr 2021 17:48
 Operator : AJ/MA
 Sample : M2032-02
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HOLDING-TANK-260

Manual Integrations
 APPROVED

Ankita
 4/16/2021 3:24:06 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 07:07:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 02 05:20:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.881f	3.896	828220	451383	8.904m	8.995
2) SA Decachlor...	10.874	9.136	521296	4058518	5.628m	83.636 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041521\
Data File : P0077013.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Apr 2021 17:48
Operator : AJ/MA
Sample : M2032-02
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HOLDING-TANK-260


Manual Integrations
APPROVED

Ankita
4/16/2021 3:24:06 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 07:07:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 02 05:20:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

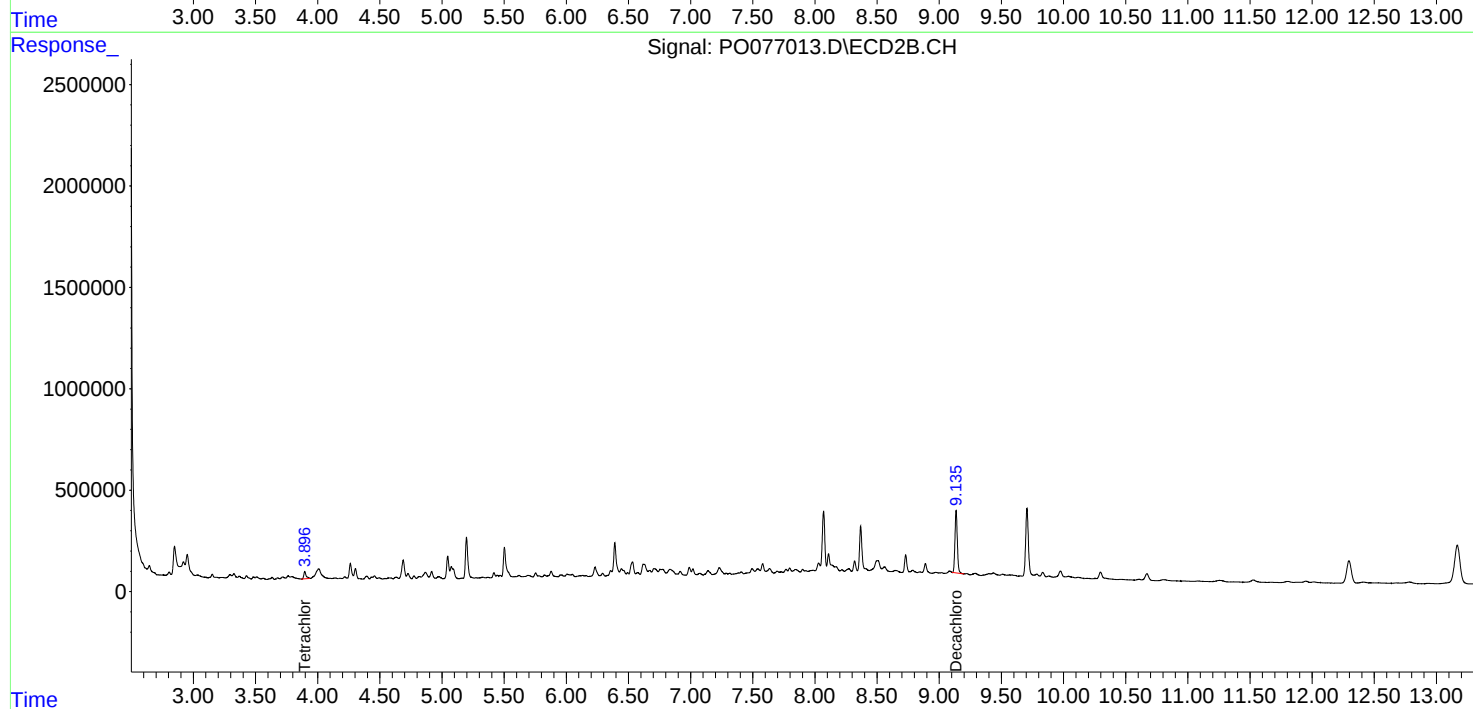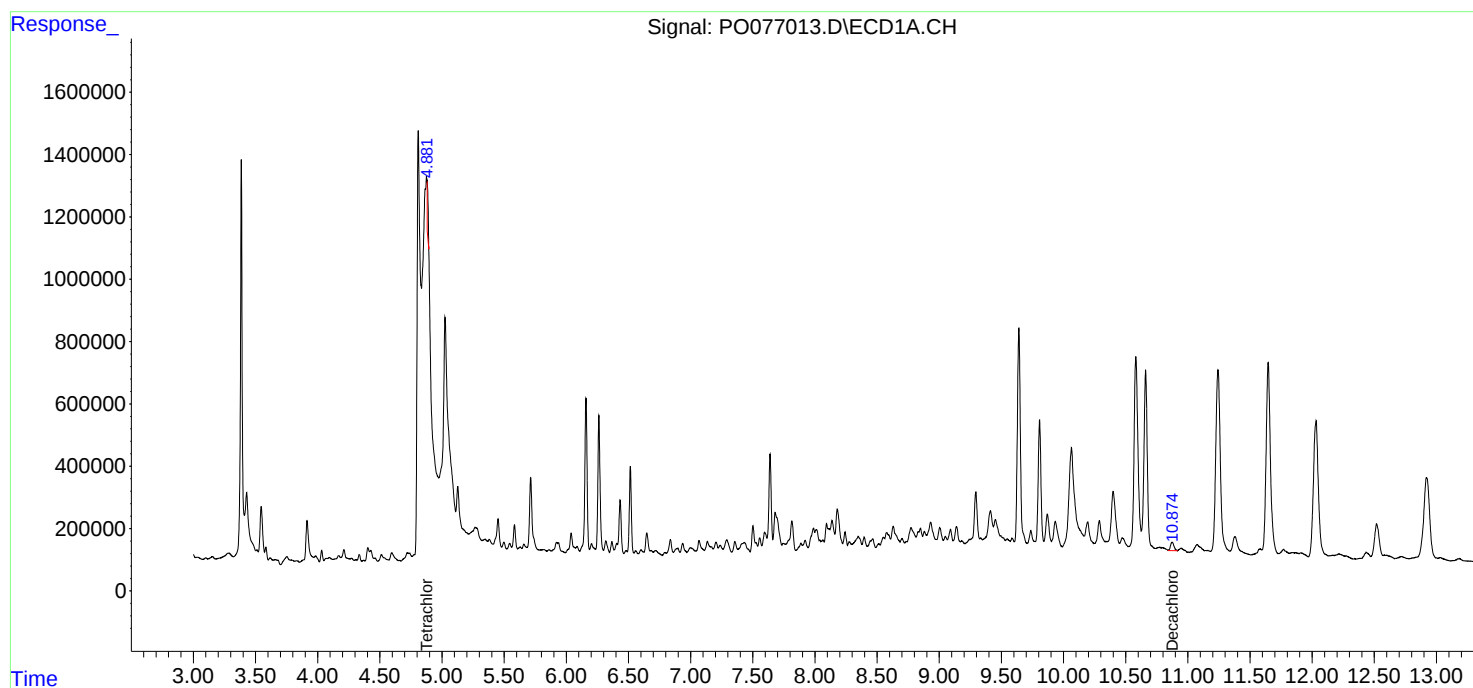

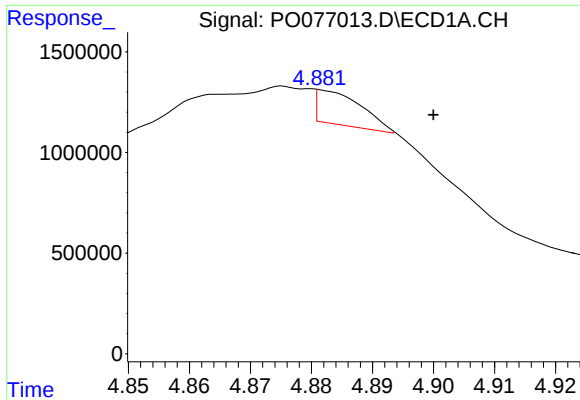


#1 Tetrachloro-m-xylene

R.T.: 4.881 min
Delta R.T.: -0.019 min
Response: 828220
Conc: 8.90 ng/ml m

Instrument :
ECD_O
ClientSampleId :
HOLDING-TANK-260


Manual Integrations
APPROVED

Ankita
4/16/2021 3:24:06 PM

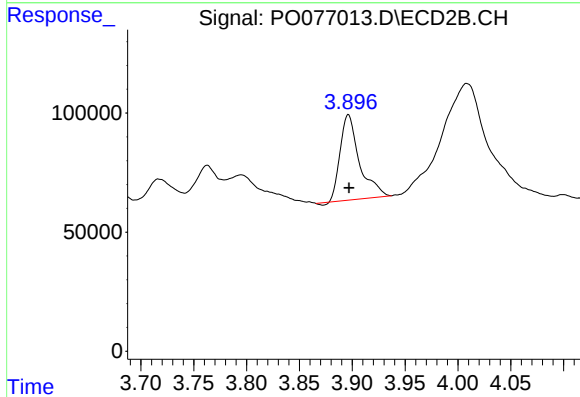


#1 Tetrachloro-m-xylene

R.T.: 3.896 min
Delta R.T.: 0.000 min
Response: 451383
Conc: 8.99 ng/ml

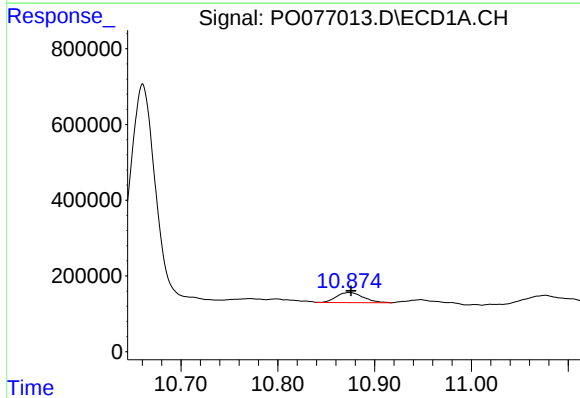

#2 Decachlorobiphenyl

R.T.: 10.874 min
Delta R.T.: -0.002 min
Response: 521296
Conc: 5.63 ng/ml m

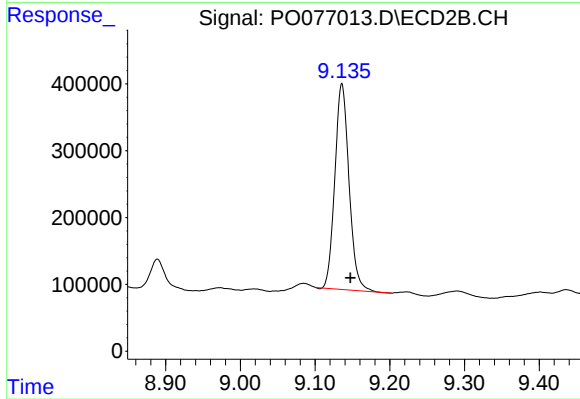

#2 Decachlorobiphenyl

R.T.: 9.136 min
Delta R.T.: -0.011 min
Response: 4058518
Conc: 83.64 ng/ml