

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0041624\
 Data File : P0102880.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Apr 2024 17:21
 Operator : YP/AJ
 Sample : P2127-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 SP-2-BACK

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/17/2024
 Supervised By :Ankita Jodhani 04/17/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 17 02:48:31 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0041524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 16 04:30:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.259	3.376	105.5E6	58235892	16.915m	14.942m
2) SA Decachlor...	9.784	8.231	89394823	57719248	25.430	25.364m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO041624\
Data File : PO102880.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Apr 2024 17:21
Operator : YP/AJ
Sample : P2127-04
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SP-2-BACK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/17/2024
Supervised By :Ankita Jodhani 04/17/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 17 02:48:31 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO041524.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 16 04:30:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

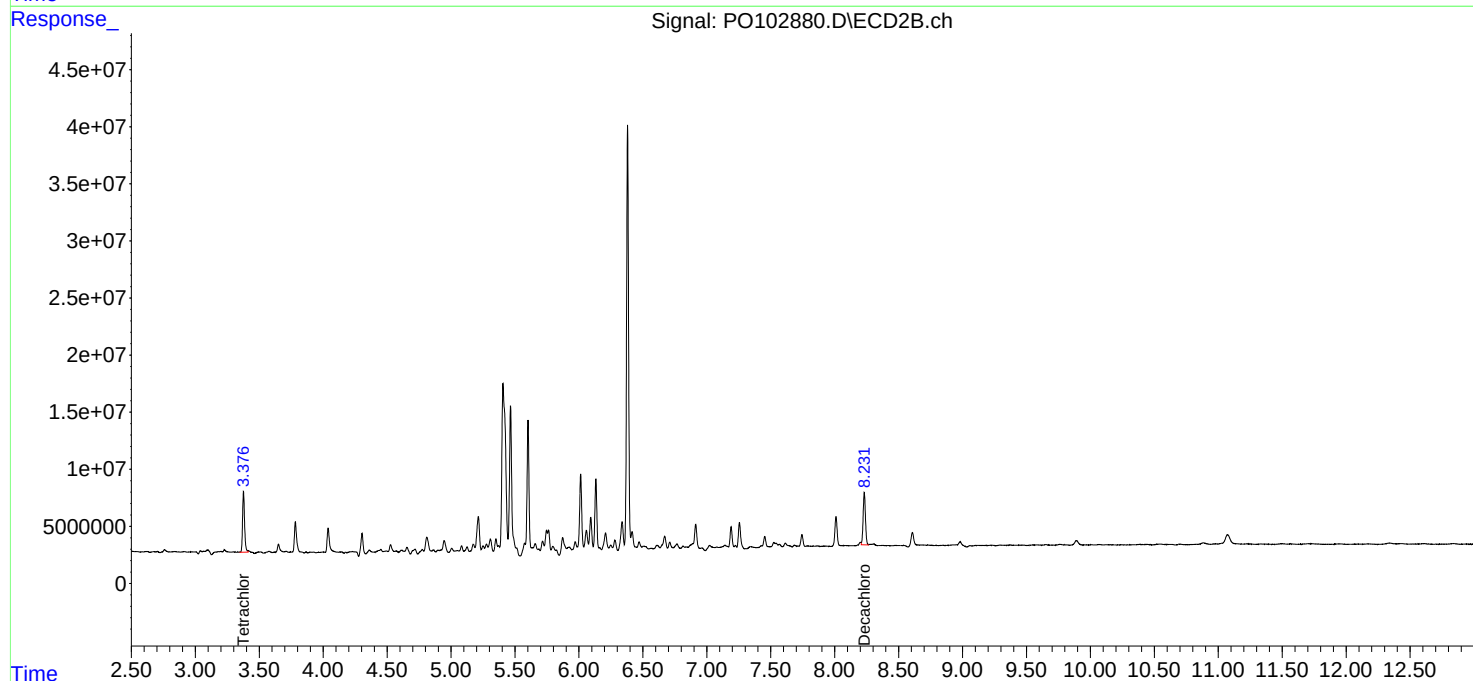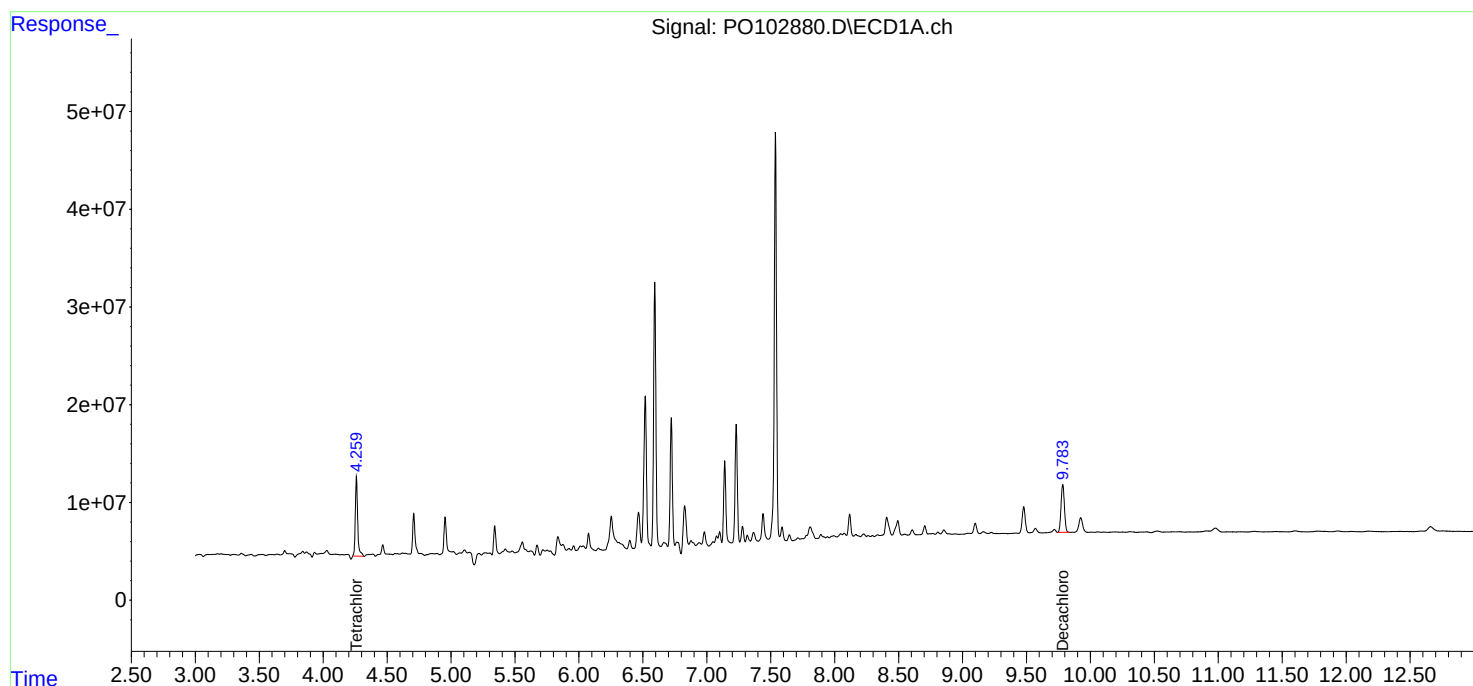

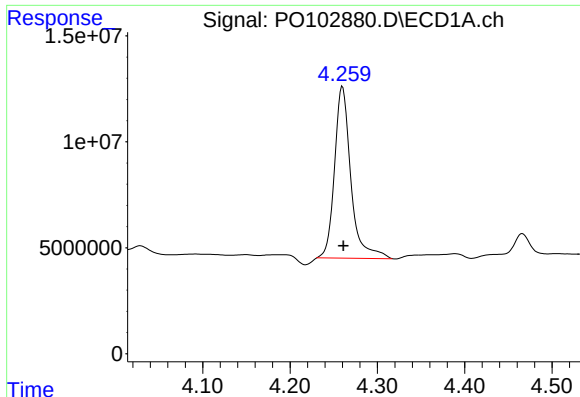

#1 Tetrachloro-m-xylene

R.T.: 4.259 min
Delta R.T.: -0.002 min
Response: 105477363
Conc: 16.92 ng/ml

Instrument :

ECD_O


ClientSampleId :

SP-2-BACK

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 04/17/2024
Supervised By :Ankita Jodhani 04/17/2024

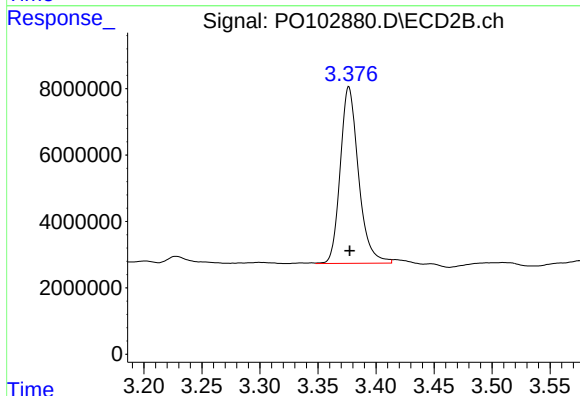


#1 Tetrachloro-m-xylene

R.T.: 3.376 min
Delta R.T.: -0.001 min
Response: 58235892
Conc: 14.94 ng/ml m

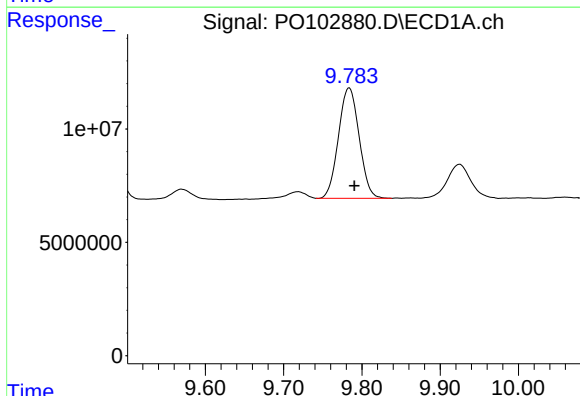

#2 Decachlorobiphenyl

R.T.: 9.784 min
Delta R.T.: -0.007 min
Response: 89394823
Conc: 25.43 ng/ml

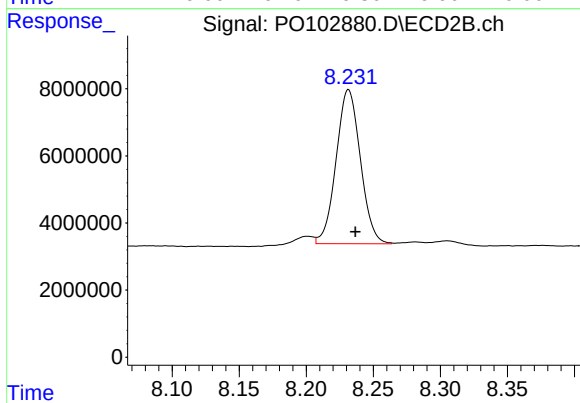

#2 Decachlorobiphenyl

R.T.: 8.231 min
Delta R.T.: -0.005 min
Response: 57719248
Conc: 25.36 ng/ml m