

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041725\
 Data File : P0110489.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Apr 2025 19:27
 Operator : YP/AJ
 Sample : Q1817-09 10X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 03-0371-2-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/18/2025
 Supervised By :mohammad ahmed 04/21/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 18 01:21:35 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0041025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 11 02:12:41 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.685	3.683	13137272	6908471	1.502m	1.385m
2) SA Decachlor...	8.730	8.683	10390158	2386971	1.316	1.240

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041725\
Data File : P0110489.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Apr 2025 19:27
Operator : YP/AJ
Sample : Q1817-09 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
03-0371-2-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/18/2025
Supervised By :mohammad ahmed 04/21/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 18 01:21:35 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0041025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 11 02:12:41 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

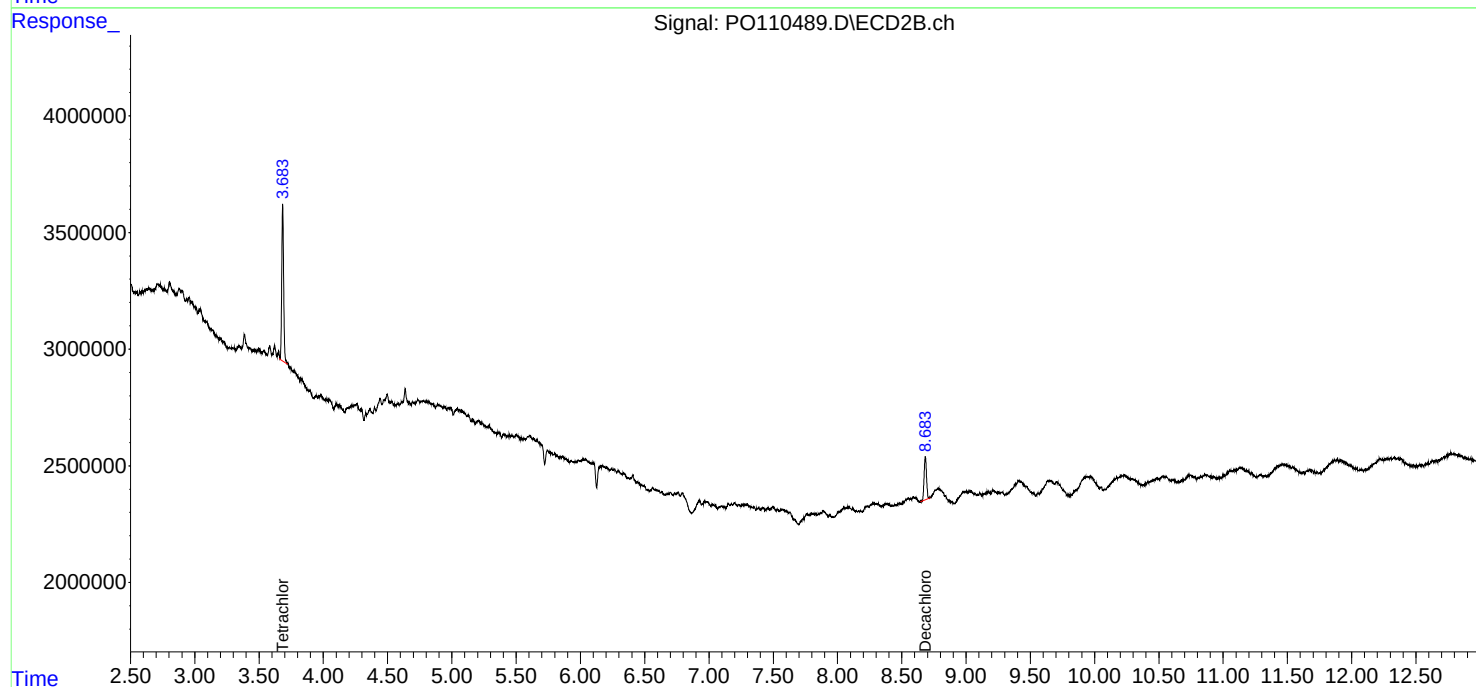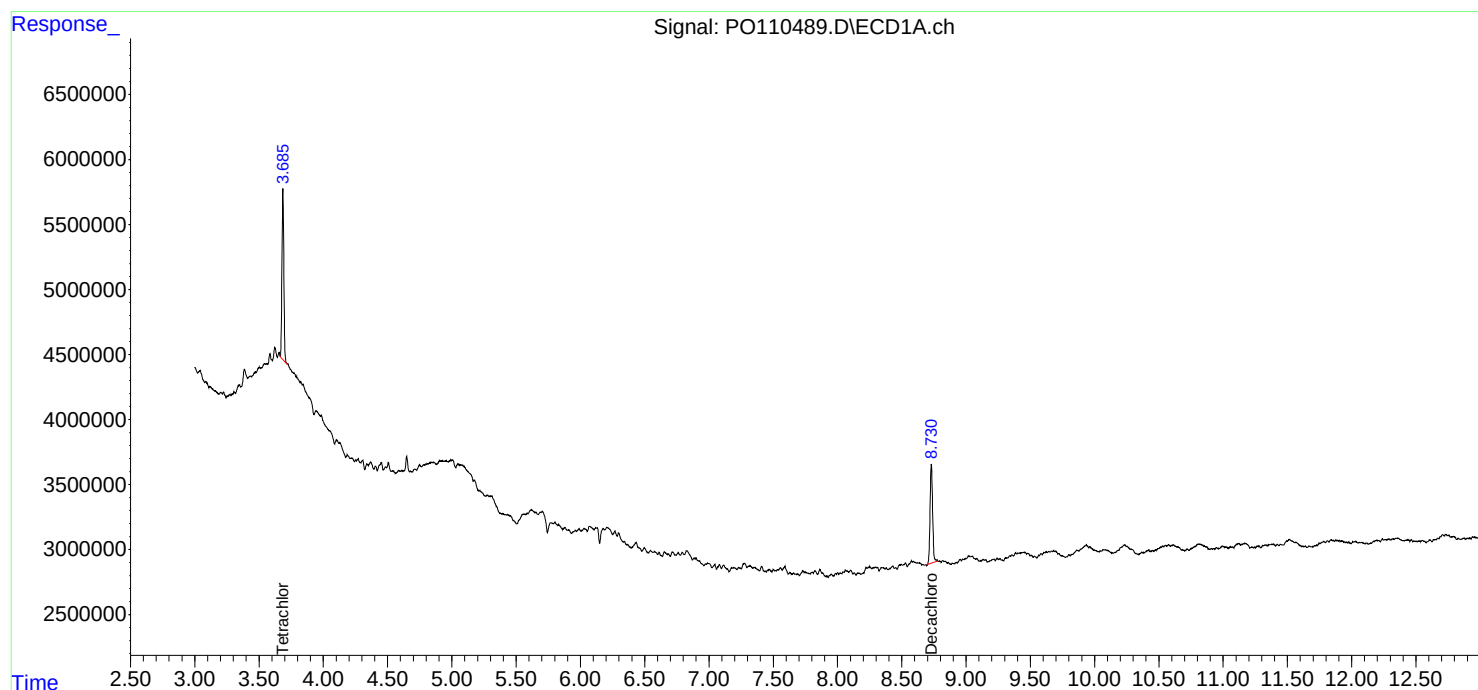

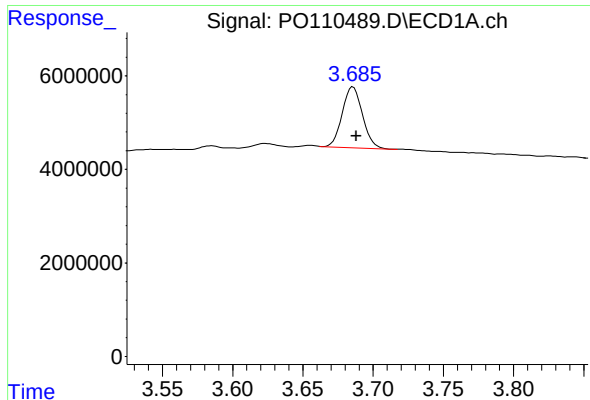


#1 Tetrachloro-m-xylene

R.T.: 3.685 min
Delta R.T.: -0.003 min
Response: 13137272
Conc: 1.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
03-0371-2-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/18/2025
Supervised By :mohammad ahmed 04/21/2025

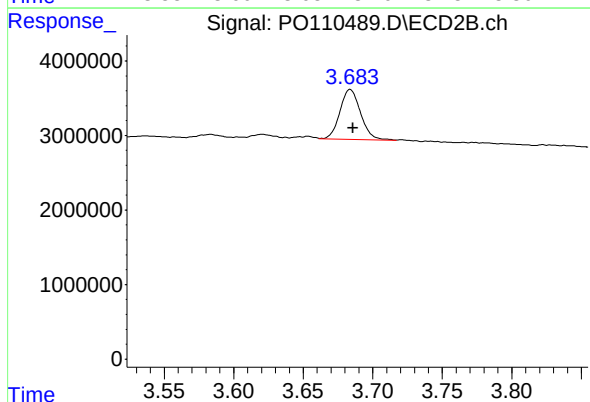


#1 Tetrachloro-m-xylene

R.T.: 3.683 min
Delta R.T.: -0.002 min
Response: 6908471
Conc: 1.38 ng/ml m

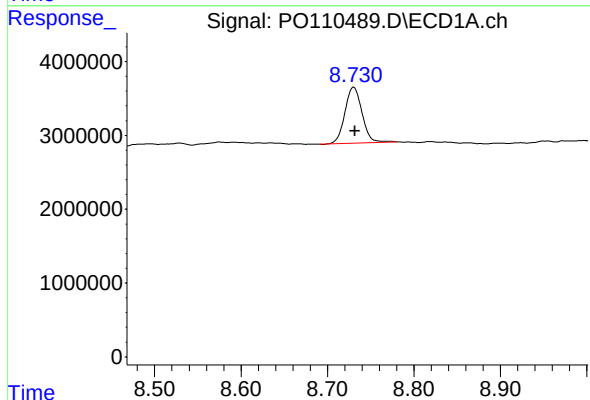

#2 Decachlorobiphenyl

R.T.: 8.730 min
Delta R.T.: -0.001 min
Response: 10390158
Conc: 1.32 ng/ml

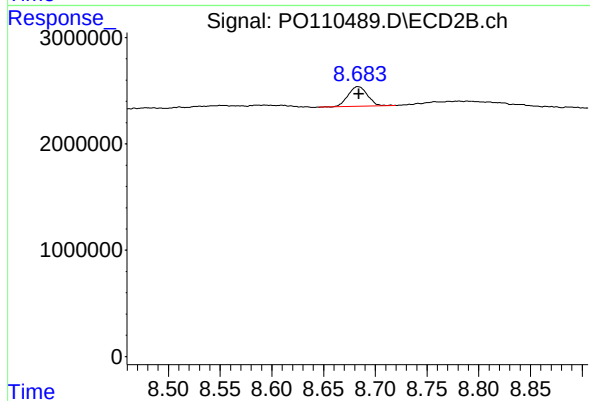

#2 Decachlorobiphenyl

R.T.: 8.683 min
Delta R.T.: 0.000 min
Response: 2386971
Conc: 1.24 ng/ml