

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041823\
 Data File : P0094335.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Apr 2023 14:32
 Operator : YP/AJ
 Sample : 02371-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :

ECD_O

ClientSampleId :

SB-23-COMP

Manual Integrations**APPROVED**

Reviewed By :Yogesh Patel 04/19/2023

Supervised By :Ankita Jodhani 04/19/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 19 06:10:09 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 04 06:20:55 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.417	3.619	71825917	26730648	19.214	20.991
2) SA Decachlor...	10.263	8.640	61409500	26351243	27.453	26.357
Target Compounds						
31) L7 AR-1260-1	7.219	6.188	18523893	10115584	126.905	155.120
32) L7 AR-1260-2	7.475	6.378	27902097	10262535	174.329	141.311
33) L7 AR-1260-3	7.842	6.530	13629291	8952800	102.647	123.362
34) L7 AR-1260-4	8.069	7.003	17623530	6314330	127.945	113.705
35) L7 AR-1260-5	8.399	7.248	28341363	14481550	130.132	139.549

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO041823\
Data File : PO094335.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Apr 2023 14:32
Operator : YP/AJ
Sample : 02371-04
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-23-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/19/2023
Supervised By :Ankita Jodhani 04/19/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 19 06:10:09 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO040323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 04 06:20:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

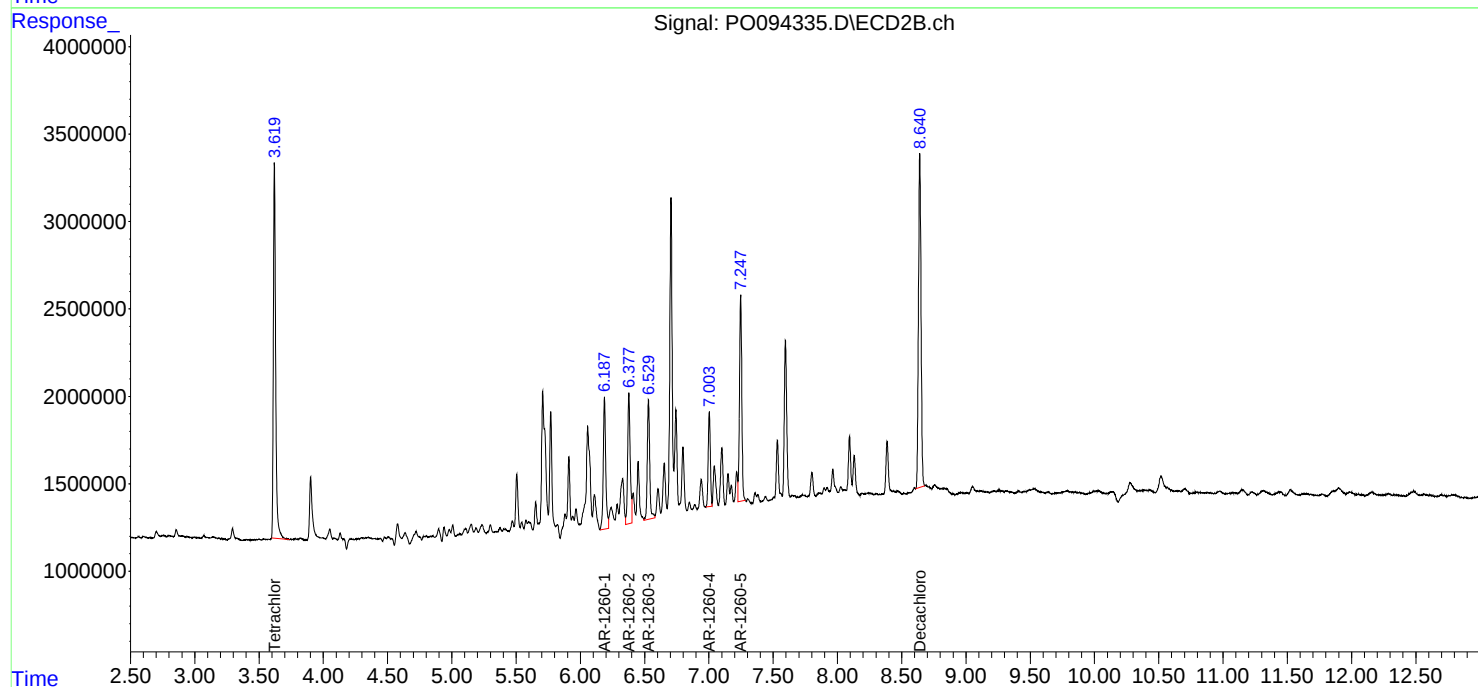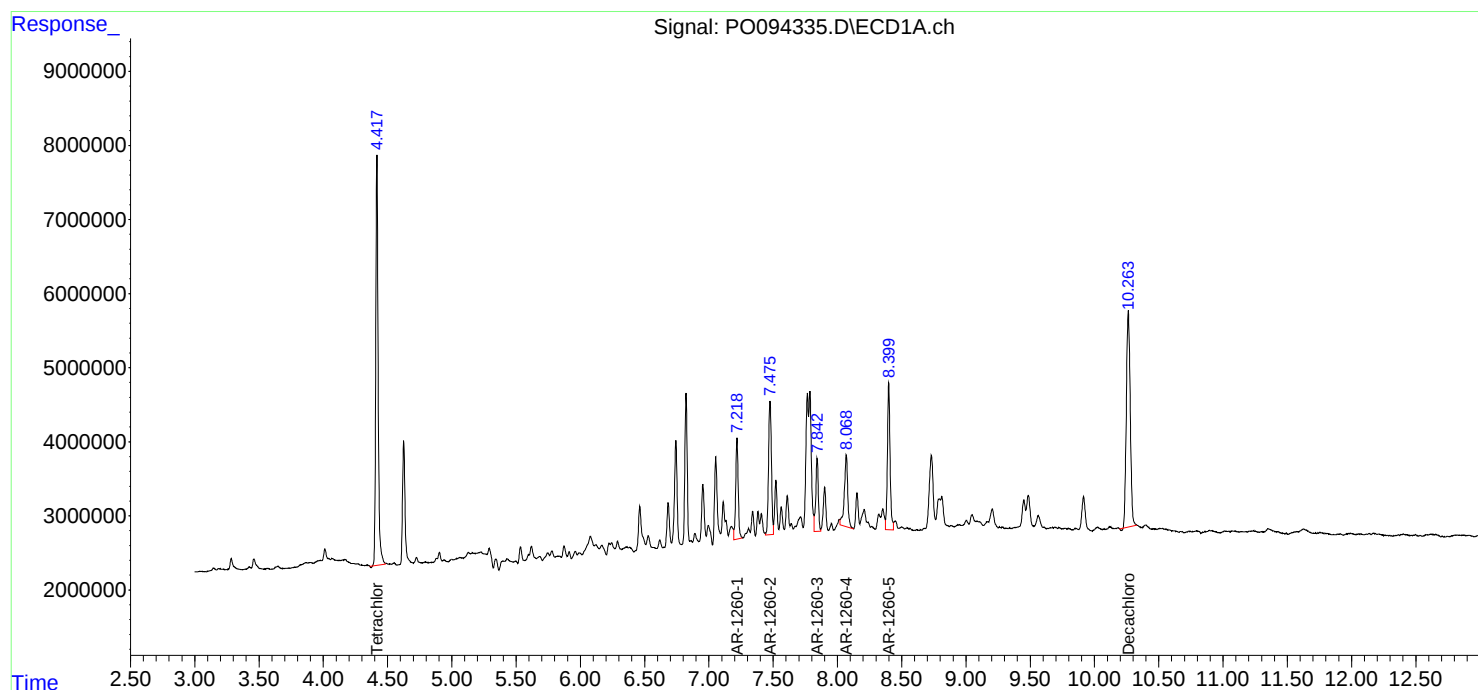

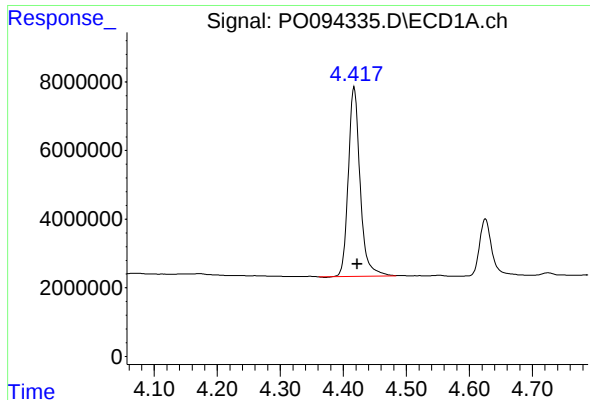

#1 Tetrachloro-m-xylene

R.T.: 4.417 min
Delta R.T.: -0.005 min
Response: 71825917
Conc: 19.21 ng/ml


Instrument :

ECD_O

ClientSampleId :
SB-23-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/19/2023
Supervised By :Ankita Jodhani 04/19/2023

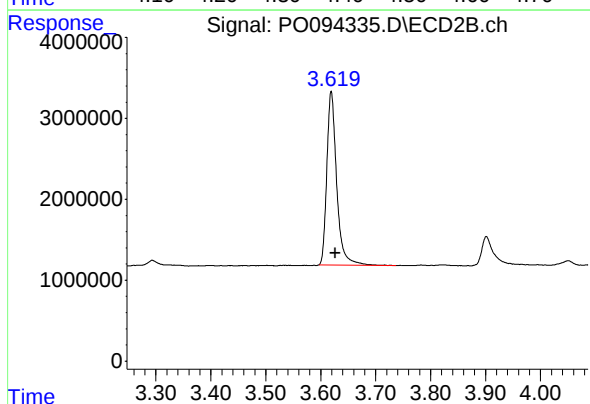


#1 Tetrachloro-m-xylene

R.T.: 3.619 min
Delta R.T.: -0.008 min
Response: 26730648
Conc: 20.99 ng/ml

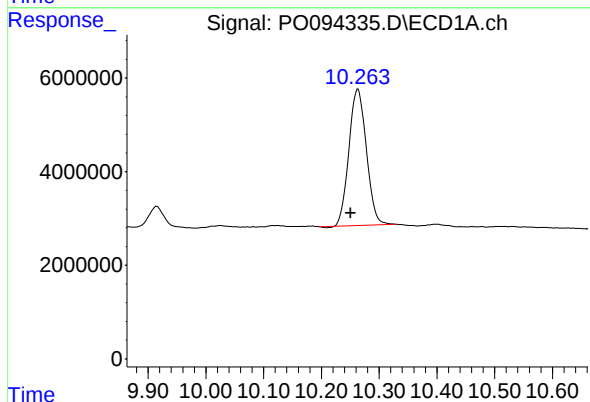


#2 Decachlorobiphenyl

R.T.: 10.263 min
Delta R.T.: 0.012 min
Response: 61409500
Conc: 27.45 ng/ml

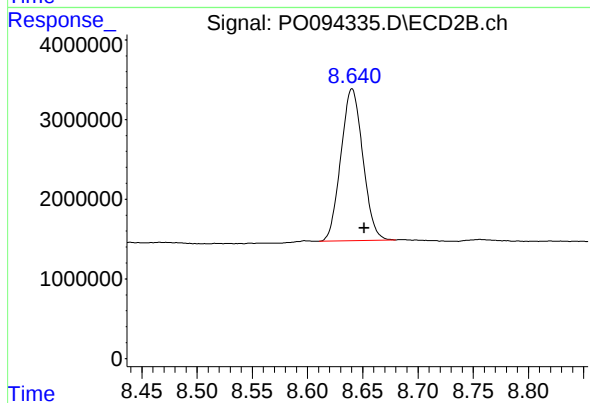

#2 Decachlorobiphenyl

R.T.: 8.640 min
Delta R.T.: -0.011 min
Response: 26351243
Conc: 26.36 ng/ml

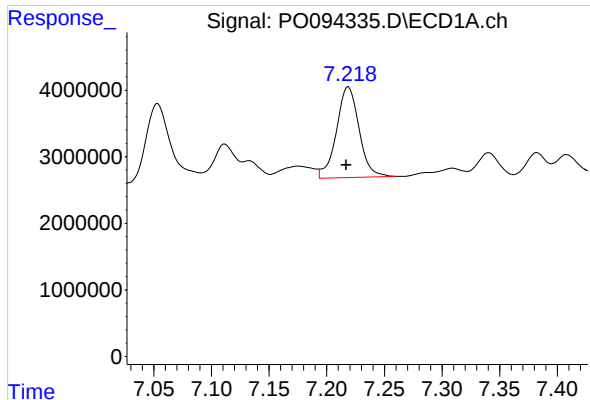


#31 AR-1260-1

R.T.: 7.219 min
Delta R.T.: 0.002 min
Response: 18523893
Conc: 126.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-23-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/19/2023
Supervised By :Ankita Jodhani 04/19/2023

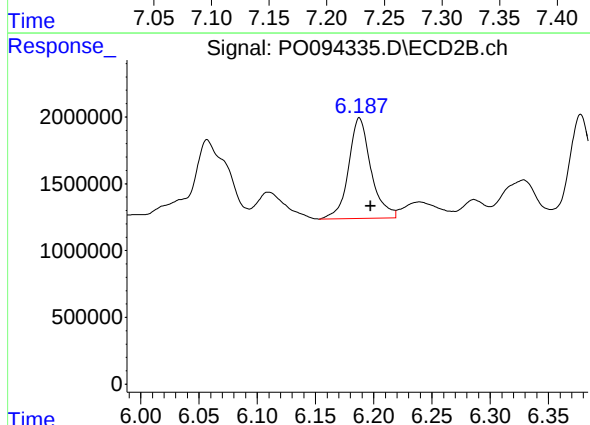


#31 AR-1260-1

R.T.: 6.188 min
Delta R.T.: -0.009 min
Response: 10115584
Conc: 155.12 ng/ml

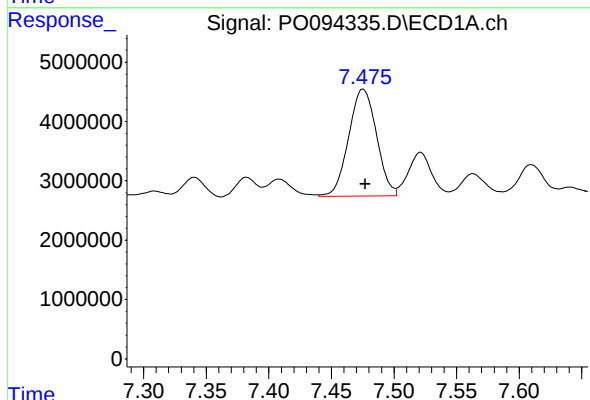


#32 AR-1260-2

R.T.: 7.475 min
Delta R.T.: -0.002 min
Response: 27902097
Conc: 174.33 ng/ml

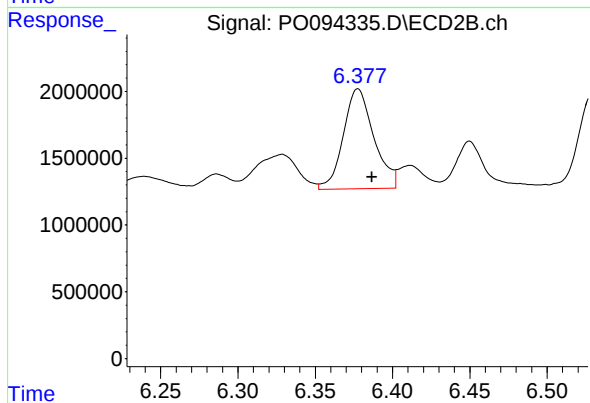

#32 AR-1260-2

R.T.: 6.378 min
Delta R.T.: -0.009 min
Response: 10262535
Conc: 141.31 ng/ml

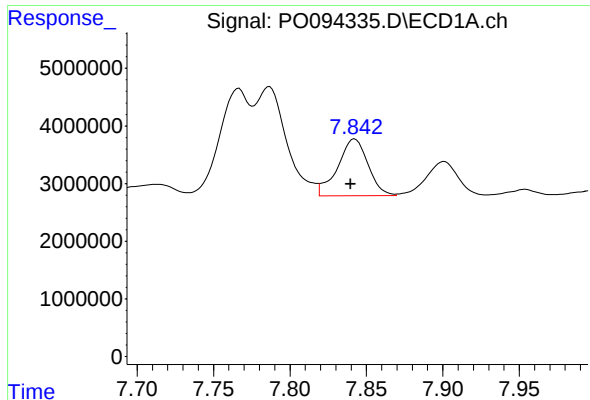


#33 AR-1260-3

R.T.: 7.842 min
Delta R.T.: 0.002 min
Response: 13629291
Conc: 102.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-23-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/19/2023
Supervised By :Ankita Jodhani 04/19/2023

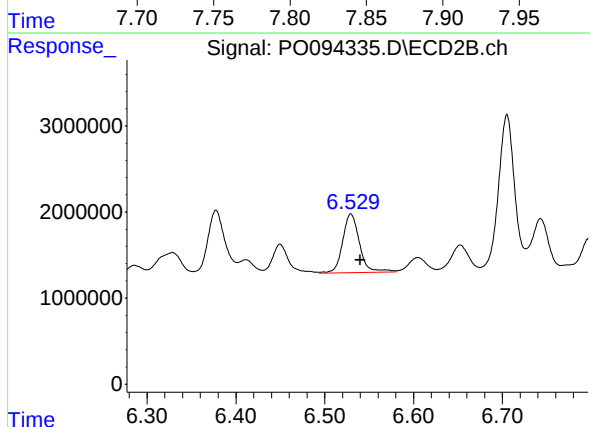


#33 AR-1260-3

R.T.: 6.530 min
Delta R.T.: -0.011 min
Response: 8952800
Conc: 123.36 ng/ml

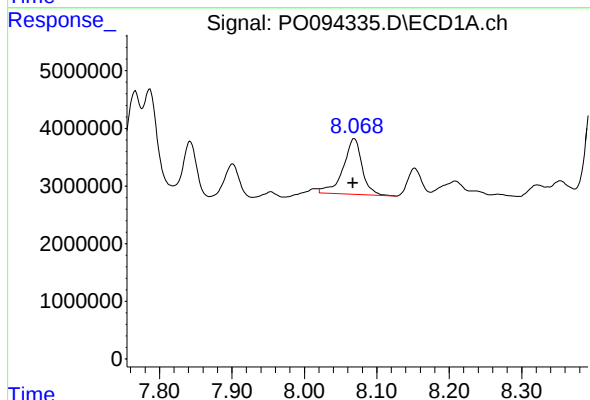


#34 AR-1260-4

R.T.: 8.069 min
Delta R.T.: 0.002 min
Response: 17623530
Conc: 127.94 ng/ml

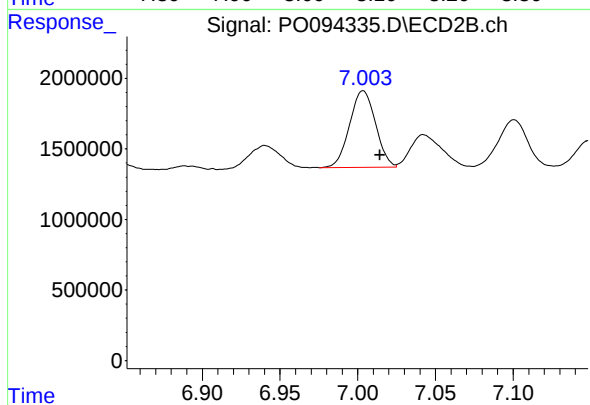

#34 AR-1260-4

R.T.: 7.003 min
Delta R.T.: -0.011 min
Response: 6314330
Conc: 113.70 ng/ml

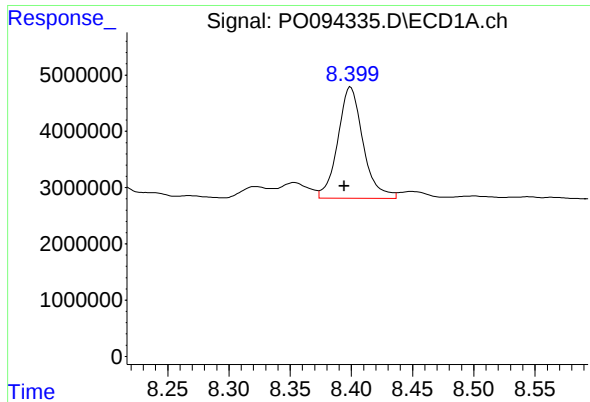


#35 AR-1260-5

R.T.: 8.399 min
Delta R.T.: 0.005 min
Response: 28341363
Conc: 130.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-23-COMP

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/19/2023
Supervised By :Ankita Jodhani 04/19/2023

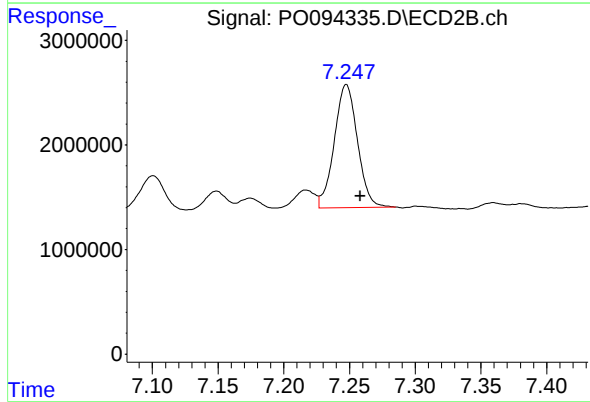

#35 AR-1260-5

R.T.: 7.248 min
Delta R.T.: -0.011 min
Response: 14481550
Conc: 139.55 ng/ml