

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041823\
 Data File : P0094338.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Apr 2023 15:23
 Operator : YP/AJ
 Sample : 02371-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-20-COMP

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/19/2023
 Supervised By :Ankita Jodhani 04/19/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 19 06:12:54 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 04 06:20:55 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.417	3.620	68531843	26580100	18.333	20.873
2) SA Decachlor...	10.262	8.641	49273684	21751411	22.027	21.756
Target Compounds						
31) L7 AR-1260-1	7.218	6.188	10338088	5772792	70.825	88.524
32) L7 AR-1260-2	7.477	6.377	16300684	6491703	101.845	89.388
33) L7 AR-1260-3	7.841	6.530	5337072	5625988	40.195	77.521 #
34) L7 AR-1260-4	8.060	7.004	10586863	2091960	76.859	37.671 #
35) L7 AR-1260-5	8.397	7.249	10274165	5308489	47.175m	51.154

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO041823\
Data File : PO094338.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Apr 2023 15:23
Operator : YP/AJ
Sample : 02371-10
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-20-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/19/2023
Supervised By :Ankita Jodhani 04/19/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 19 06:12:54 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO040323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 04 06:20:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

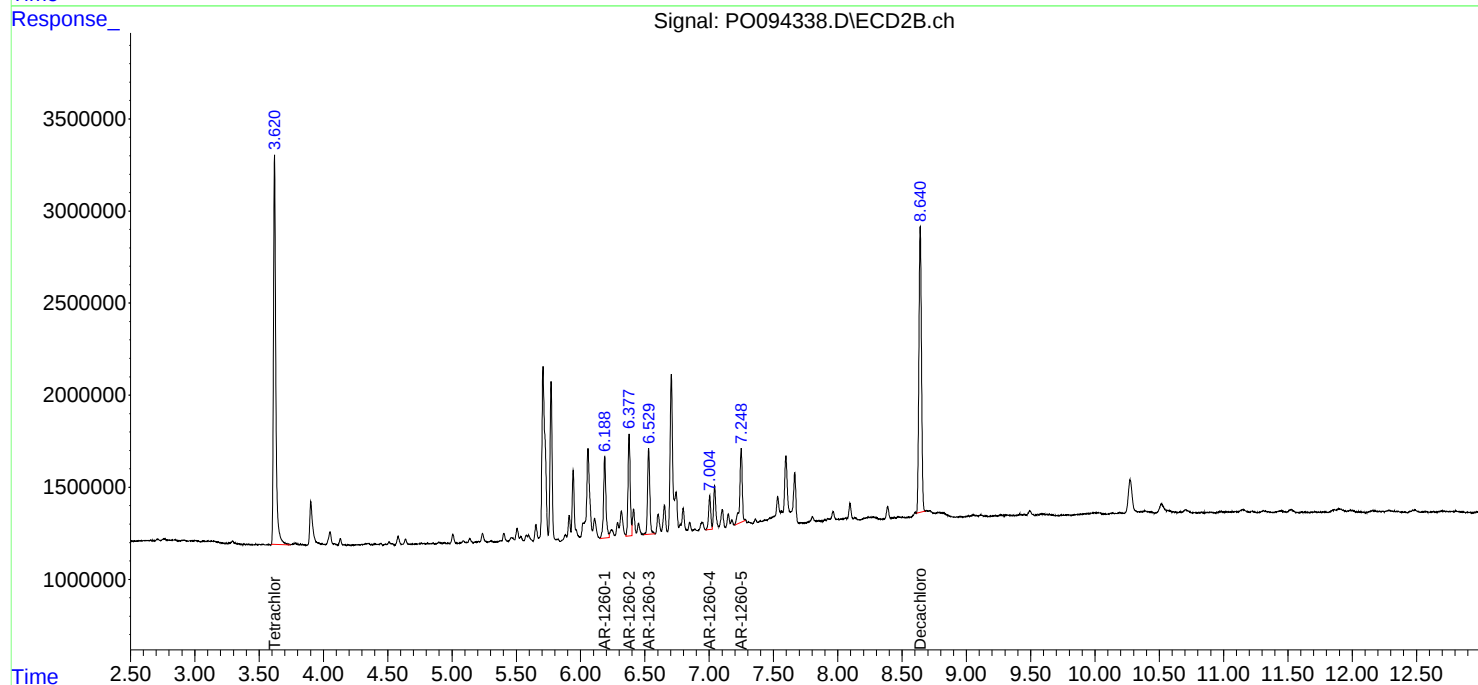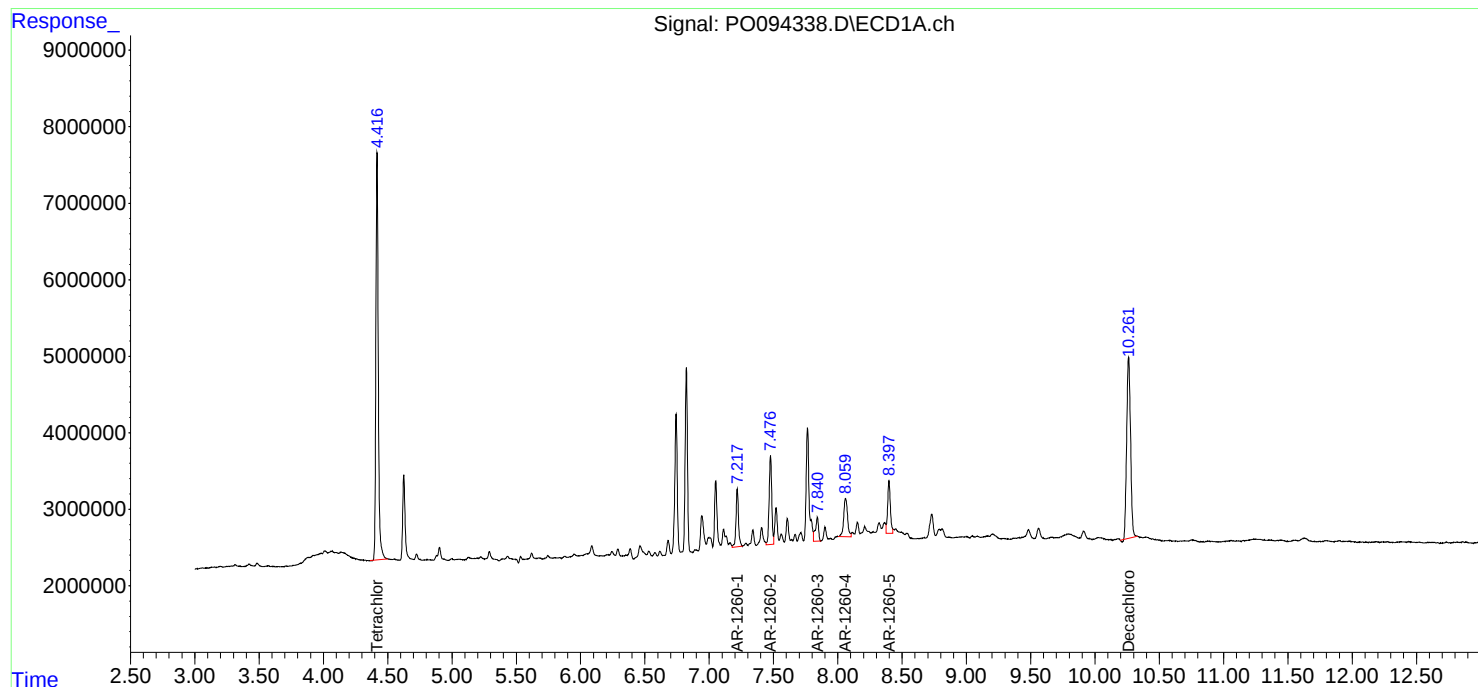

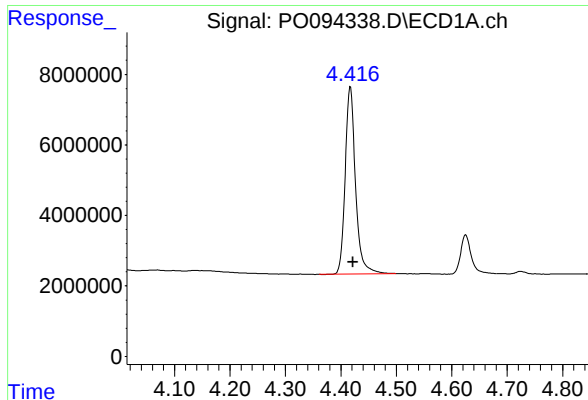


#1 Tetrachloro-m-xylene

R.T.: 4.417 min
Delta R.T.: -0.005 min
Response: 68531843
Conc: 18.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-20-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/19/2023
Supervised By :Ankita Jodhani 04/19/2023

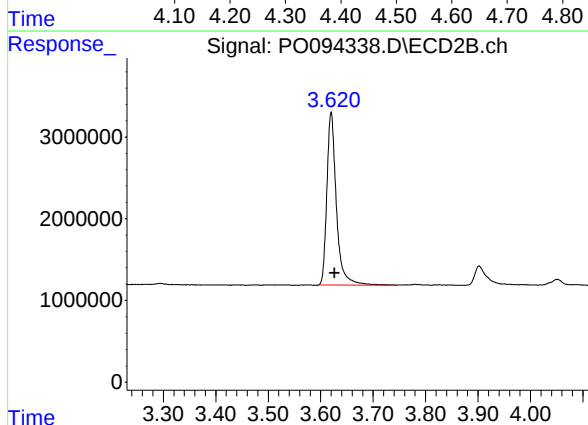


#1 Tetrachloro-m-xylene

R.T.: 3.620 min
Delta R.T.: -0.007 min
Response: 26580100
Conc: 20.87 ng/ml

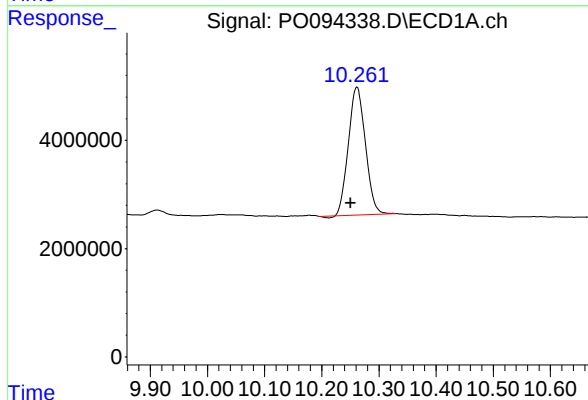


#2 Decachlorobiphenyl

R.T.: 10.262 min
Delta R.T.: 0.011 min
Response: 49273684
Conc: 22.03 ng/ml

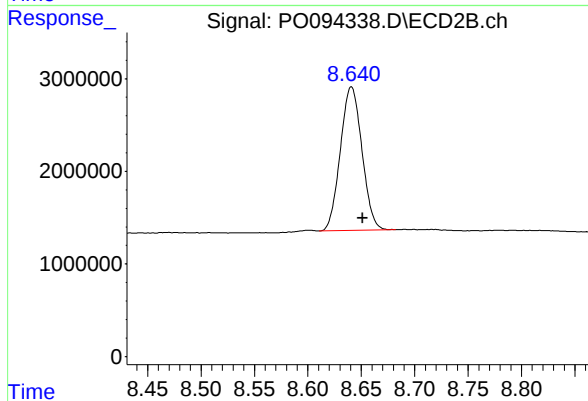

#2 Decachlorobiphenyl

R.T.: 8.641 min
Delta R.T.: -0.011 min
Response: 21751411
Conc: 21.76 ng/ml

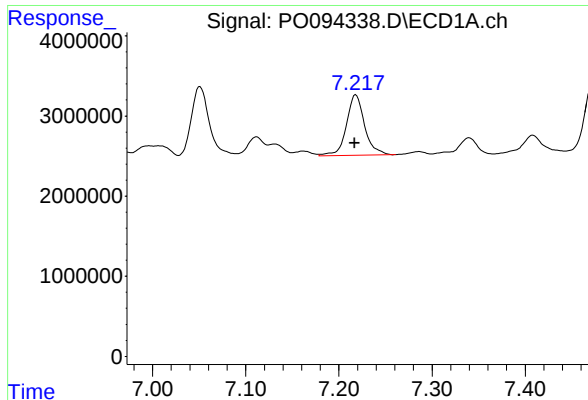


#31 AR-1260-1

R.T.: 7.218 min
Delta R.T.: 0.001 min
Response: 10338088
Conc: 70.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-20-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/19/2023
Supervised By :Ankita Jodhani 04/19/2023

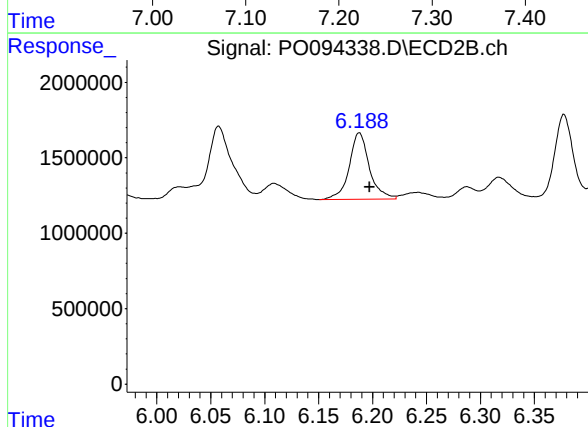


#31 AR-1260-1

R.T.: 6.188 min
Delta R.T.: -0.010 min
Response: 5772792
Conc: 88.52 ng/ml

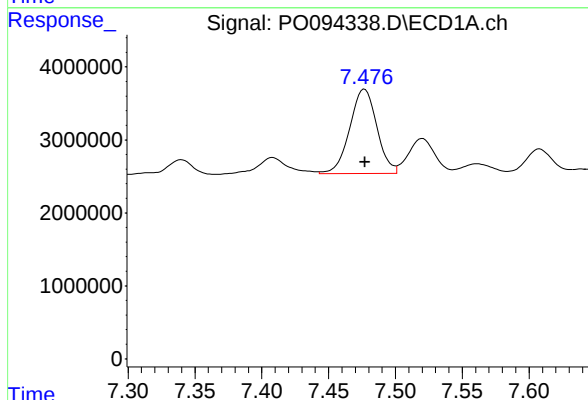


#32 AR-1260-2

R.T.: 7.477 min
Delta R.T.: 0.000 min
Response: 16300684
Conc: 101.84 ng/ml

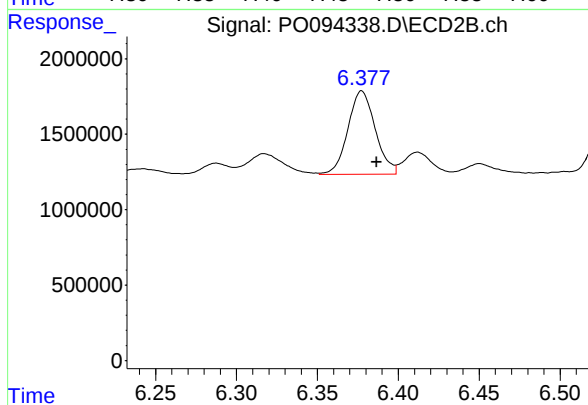

#32 AR-1260-2

R.T.: 6.377 min
Delta R.T.: -0.009 min
Response: 6491703
Conc: 89.39 ng/ml

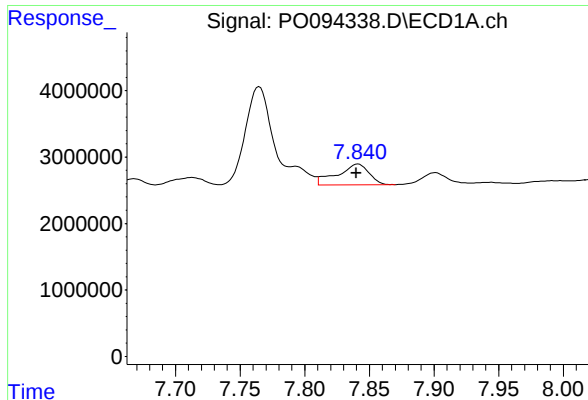


#33 AR-1260-3

R.T.: 7.841 min
Delta R.T.: 0.001 min
Response: 5337072
Conc: 40.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-20-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/19/2023
Supervised By :Ankita Jodhani 04/19/2023

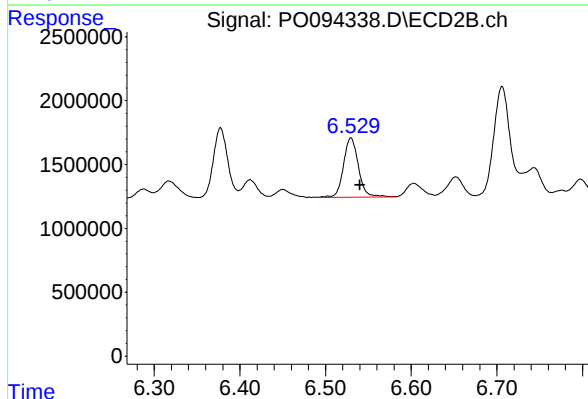


#33 AR-1260-3

R.T.: 6.530 min
Delta R.T.: -0.011 min
Response: 5625988
Conc: 77.52 ng/ml

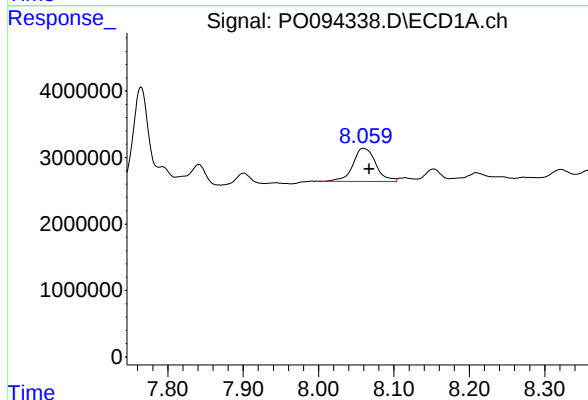


#34 AR-1260-4

R.T.: 8.060 min
Delta R.T.: -0.008 min
Response: 10586863
Conc: 76.86 ng/ml

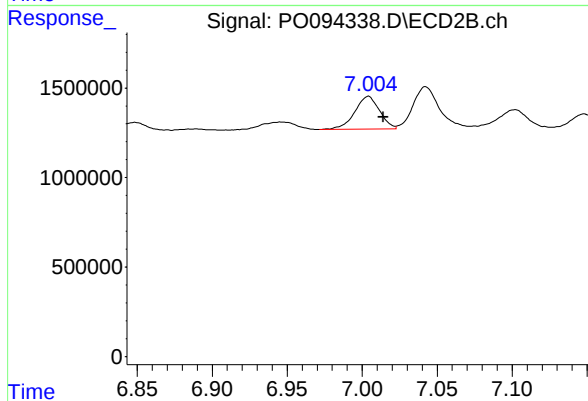

#34 AR-1260-4

R.T.: 7.004 min
Delta R.T.: -0.010 min
Response: 2091960
Conc: 37.67 ng/ml

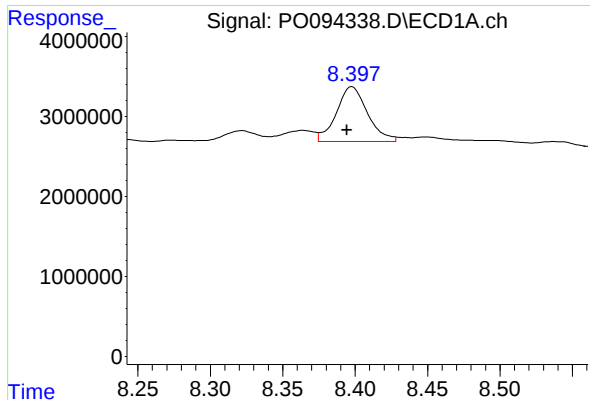


#35 AR-1260-5

R.T.: 8.397 min
Delta R.T.: 0.003 min
Response: 10274165
Conc: 47.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-20-COMP

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/19/2023
Supervised By :Ankita Jodhani 04/19/2023

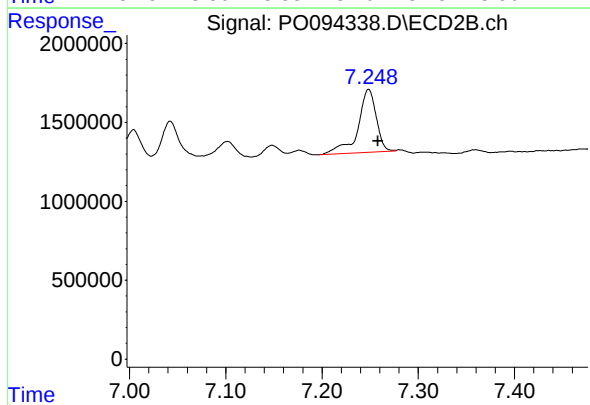

#35 AR-1260-5

R.T.: 7.249 min
Delta R.T.: -0.010 min
Response: 5308489
Conc: 51.15 ng/ml