

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041923\
 Data File : P0094399.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2023 00:59
 Operator : YP/AJ
 Sample : AR1268ICC050
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/20/2023
 Supervised By :Ankita Jodhani 04/20/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 20 04:53:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0041923.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 20 04:42:56 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.414	3.616	16512546	6404640	4.851	4.833
2) SA Decachlor...	10.250	8.631	19443880	10040572	4.954m	5.480
Target Compounds						
41) L9 AR-1268-1	8.710	7.526	16098203	8754321	50.760	52.960m
42) L9 AR-1268-2	8.807	7.591	14032481	7819793	49.741	50.794
43) L9 AR-1268-3	9.041	7.797	13017332	7213886	49.385	52.562
44) L9 AR-1268-4	9.477	8.088	3757617	2226090	44.544	49.118
45) L9 AR-1268-5	9.902	8.379	39994689	19208531	50.205m	51.495

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO041923\
Data File : PO094399.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2023 00:59
Operator : YP/AJ
Sample : AR1268ICC050
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/20/2023
Supervised By :Ankita Jodhani 04/20/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 04:53:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO041923.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 20 04:42:56 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

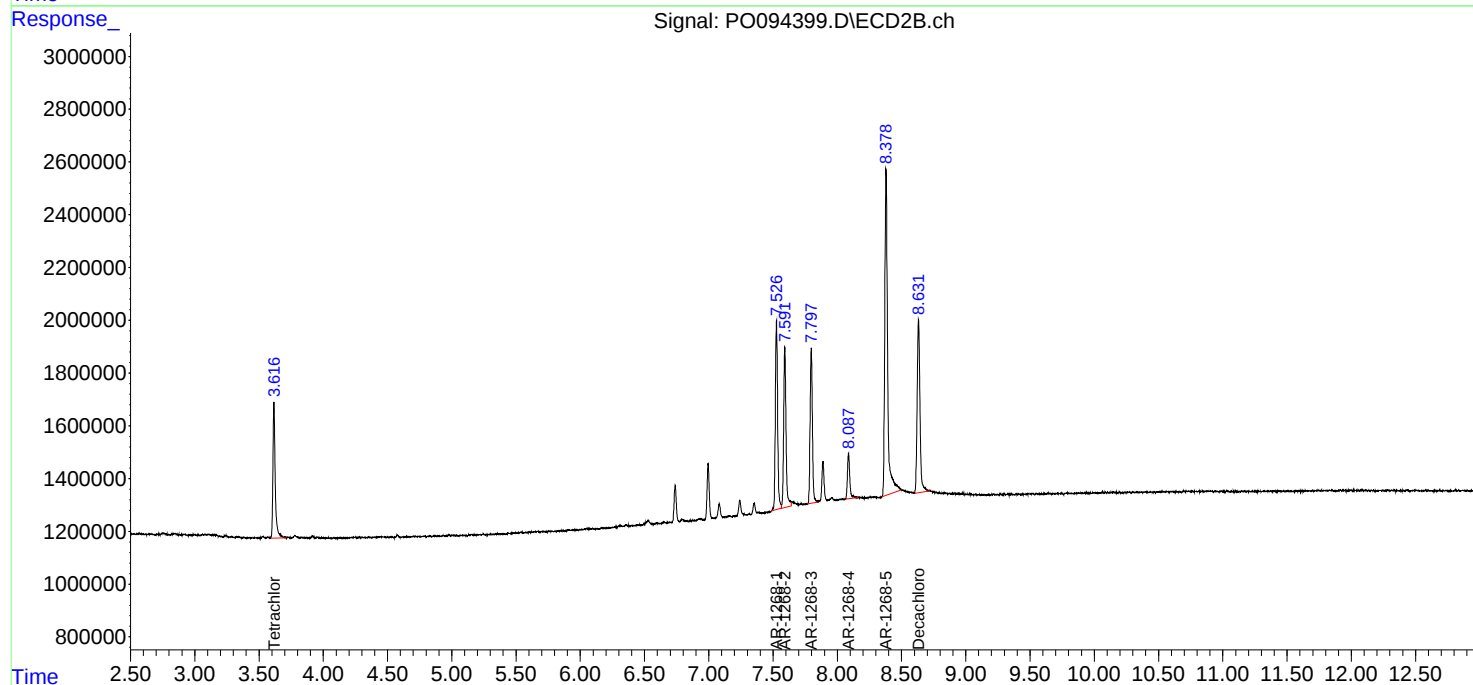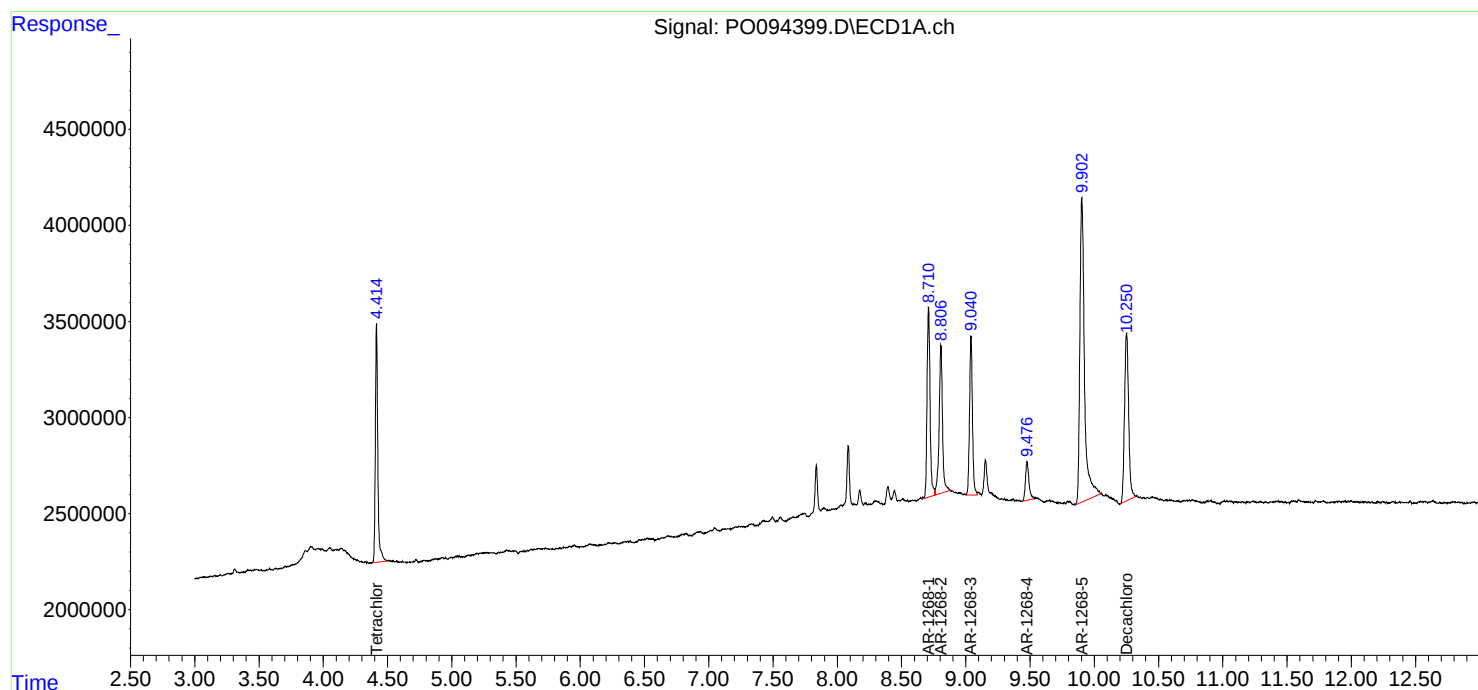

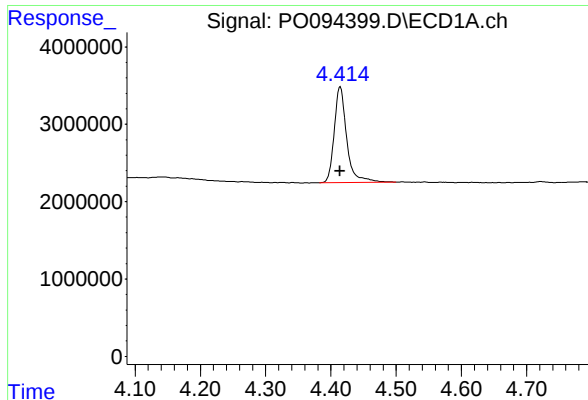


#1 Tetrachloro-m-xylene

R.T.: 4.414 min
Delta R.T.: 0.000 min
Response: 16512546
Conc: 4.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/20/2023
Supervised By :Ankita Jodhani 04/20/2023

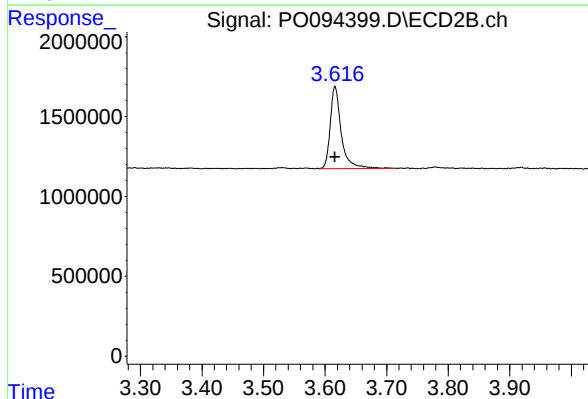


#1 Tetrachloro-m-xylene

R.T.: 3.616 min
Delta R.T.: 0.000 min
Response: 6404640
Conc: 4.83 ng/ml

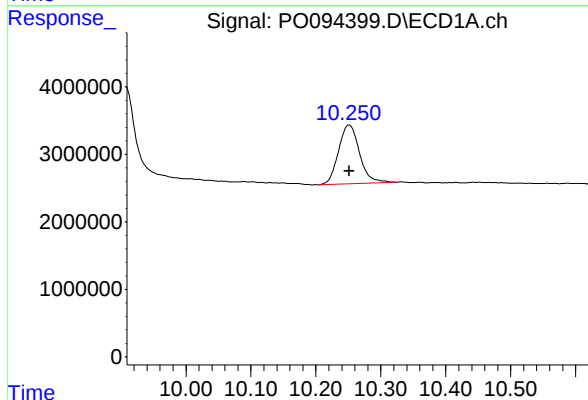


#2 Decachlorobiphenyl

R.T.: 10.250 min
Delta R.T.: 0.000 min
Response: 19443880
Conc: 4.95 ng/ml m

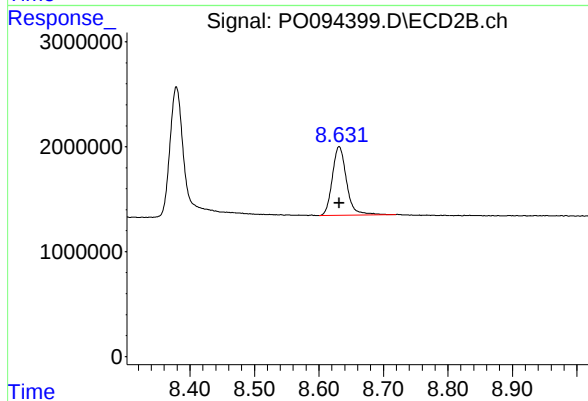

#2 Decachlorobiphenyl

R.T.: 8.631 min
Delta R.T.: 0.000 min
Response: 10040572
Conc: 5.48 ng/ml

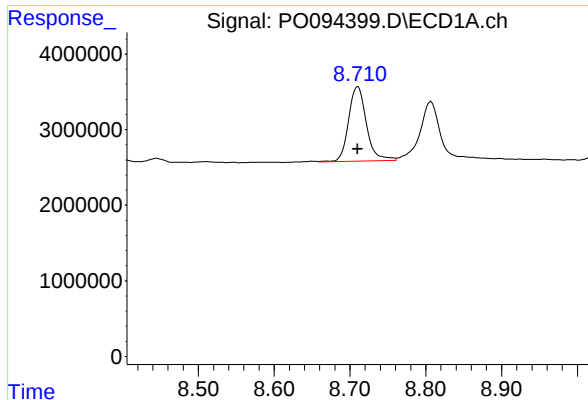


#41 AR-1268-1

R.T.: 8.710 min
Delta R.T.: 0.000 min
Response: 16098203
Conc: 50.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/20/2023
Supervised By :Ankita Jodhani 04/20/2023

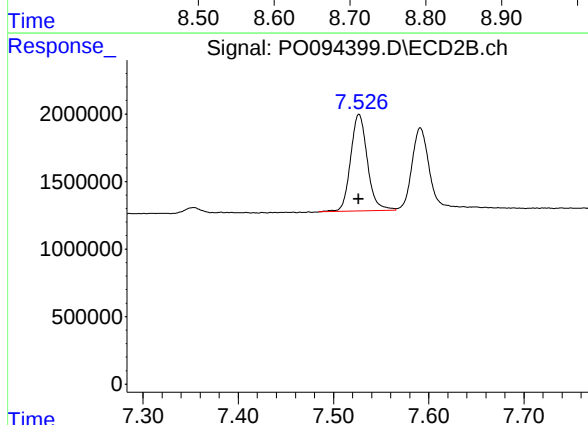


#41 AR-1268-1

R.T.: 7.526 min
Delta R.T.: 0.000 min
Response: 8754321
Conc: 52.96 ng/ml

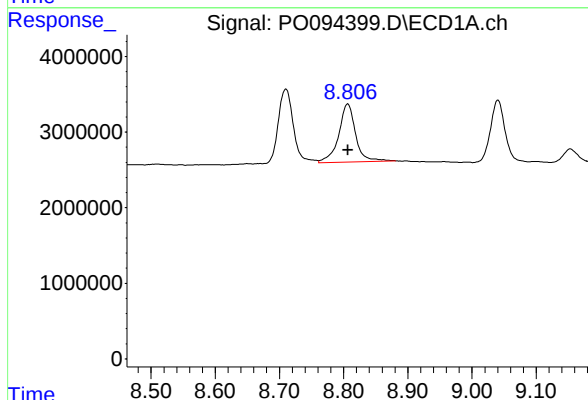


#42 AR-1268-2

R.T.: 8.807 min
Delta R.T.: 0.000 min
Response: 14032481
Conc: 49.74 ng/ml

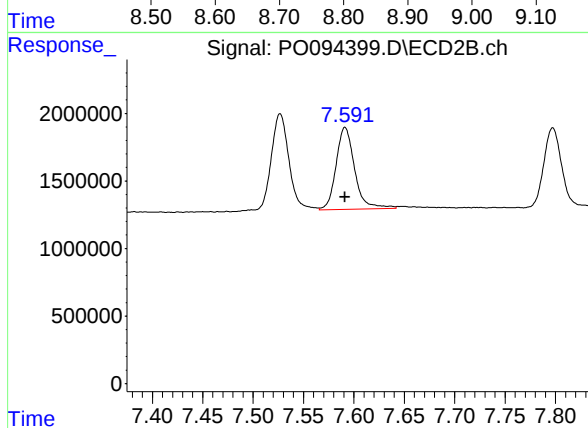

#42 AR-1268-2

R.T.: 7.591 min
Delta R.T.: 0.000 min
Response: 7819793
Conc: 50.79 ng/ml

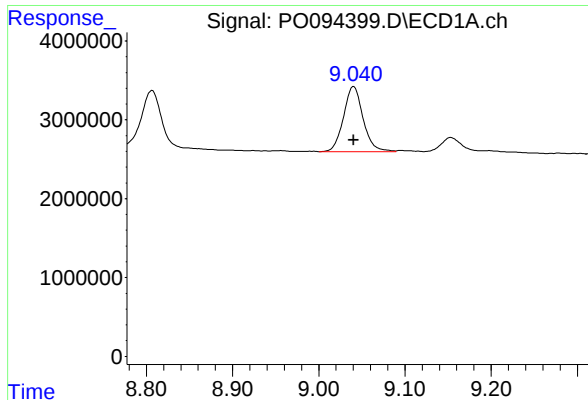


#43 AR-1268-3

R.T.: 9.041 min
Delta R.T.: 0.000 min
Response: 13017332
Conc: 49.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/20/2023
Supervised By :Ankita Jodhani 04/20/2023

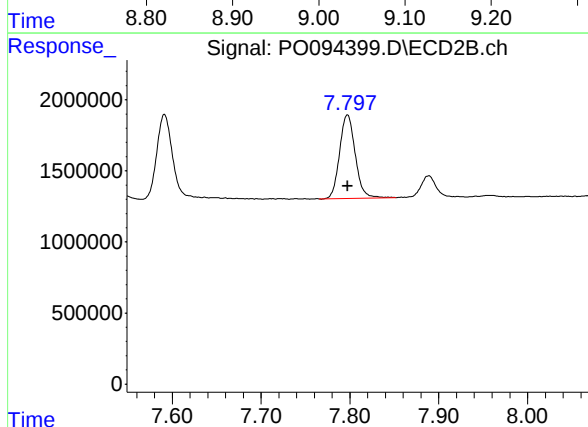


#43 AR-1268-3

R.T.: 7.797 min
Delta R.T.: 0.000 min
Response: 7213886
Conc: 52.56 ng/ml

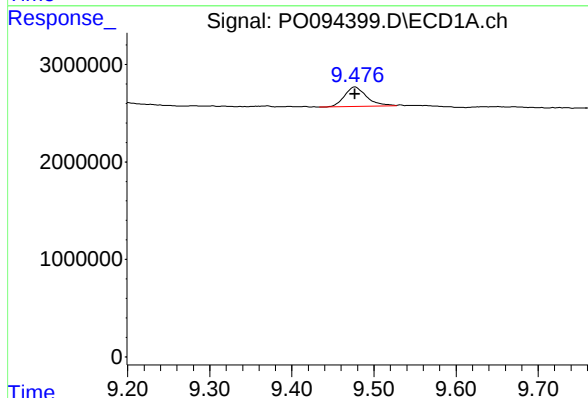


#44 AR-1268-4

R.T.: 9.477 min
Delta R.T.: 0.000 min
Response: 3757617
Conc: 44.54 ng/ml

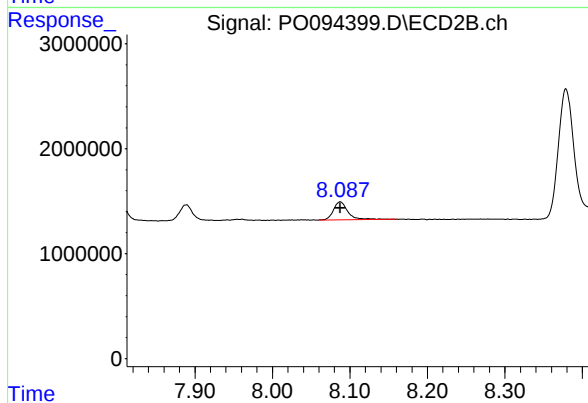

#44 AR-1268-4

R.T.: 8.088 min
Delta R.T.: 0.000 min
Response: 2226090
Conc: 49.12 ng/ml

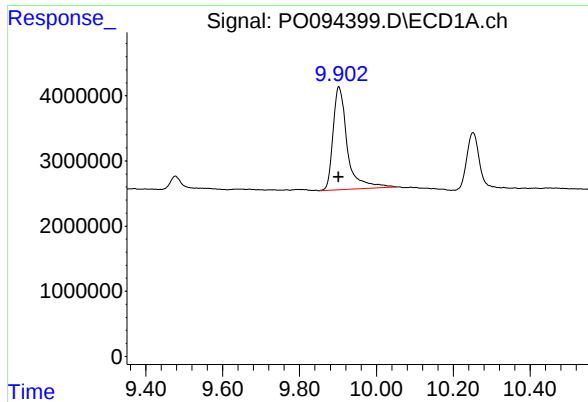


#45 AR-1268-5

R.T.: 9.902 min
Delta R.T.: 0.000 min
Response: 39994689
Conc: 50.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1268ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/20/2023
Supervised By :Ankita Jodhani 04/20/2023

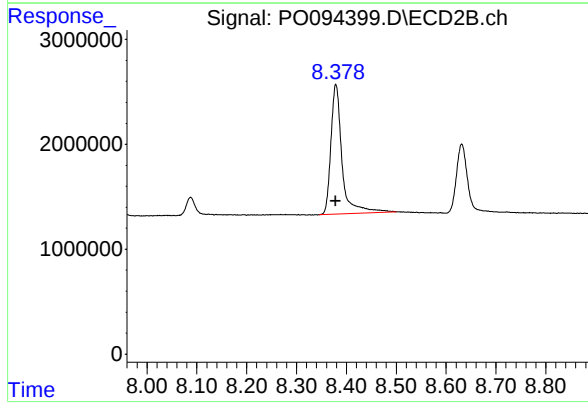

#45 AR-1268-5

R.T.: 8.379 min
Delta R.T.: 0.000 min
Response: 19208531
Conc: 51.49 ng/ml