

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041924\
 Data File : P0102959.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Apr 2024 23:03
 Operator : YP/AJ
 Sample : P2185-03
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TOTE-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/22/2024
 Supervised By :Ankita Jodhani 04/22/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 20 00:42:24 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0041524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 16 04:30:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.254	3.370	101.4E6	56291117	16.267	14.443m
2) SA Decachlor...	9.784	8.236	50731165	28511719	14.431m	12.529

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO041924\
Data File : PO102959.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Apr 2024 23:03
Operator : YP/AJ
Sample : P2185-03
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TOTE-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/22/2024
Supervised By :Ankita Jodhani 04/22/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 00:42:24 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO041524.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 16 04:30:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

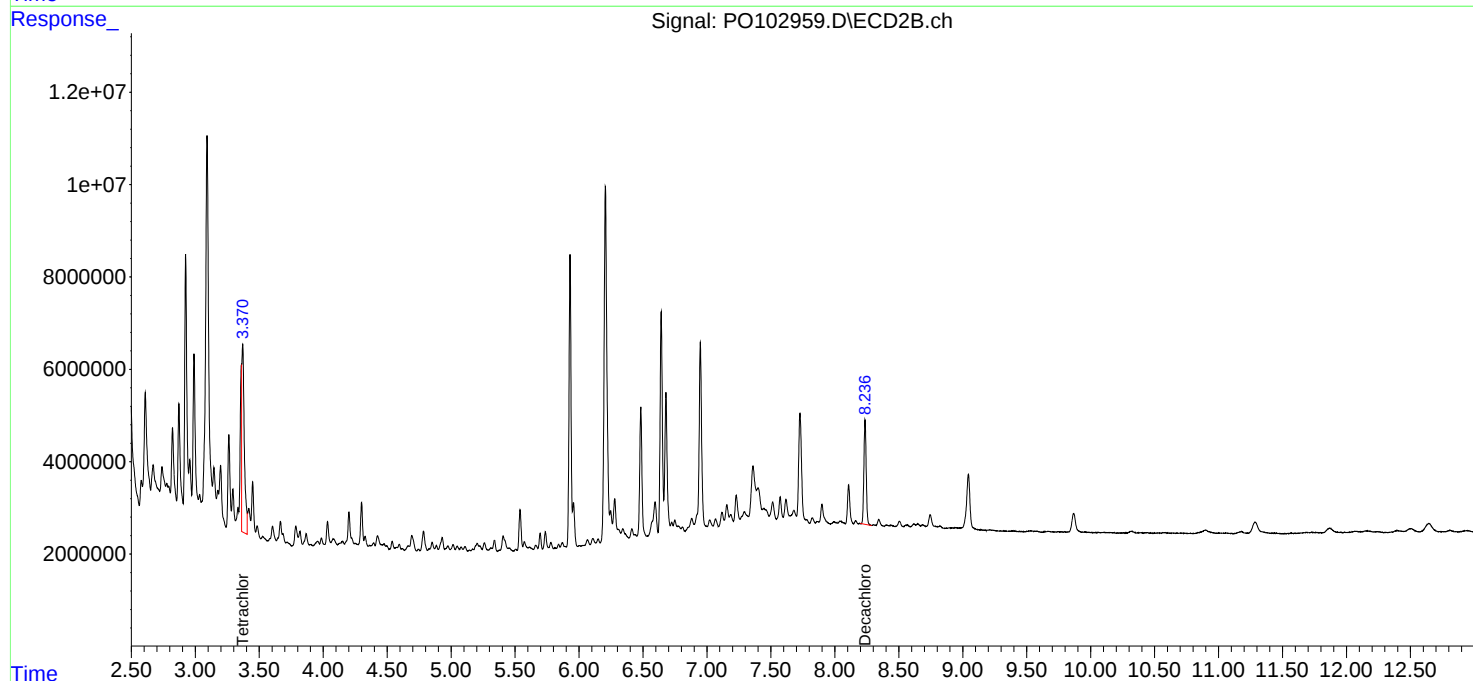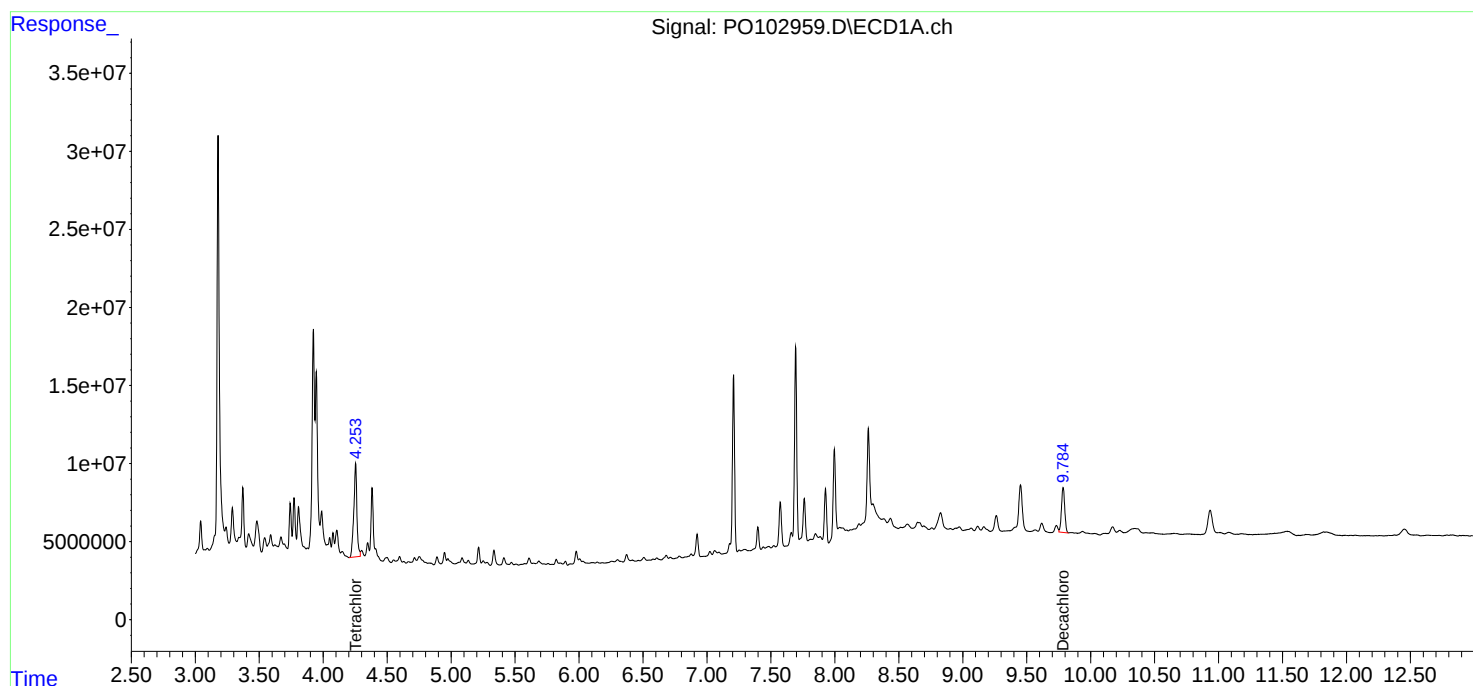

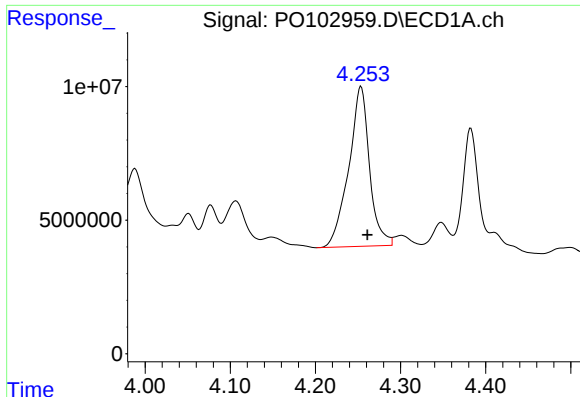


#1 Tetrachloro-m-xylene

R.T.: 4.254 min
Delta R.T.: -0.007 min
Response: 101436022
Conc: 16.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
TOTE-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/22/2024
Supervised By :Ankita Jodhani 04/22/2024

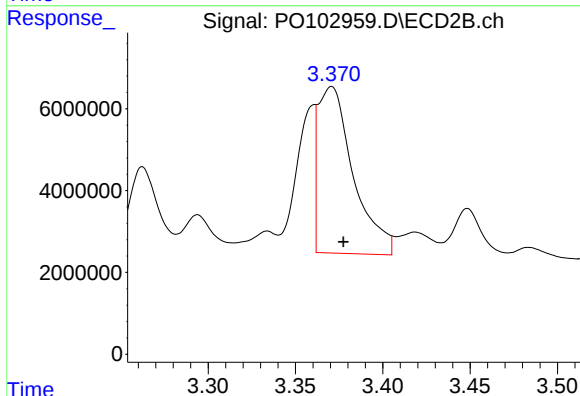


#1 Tetrachloro-m-xylene

R.T.: 3.370 min
Delta R.T.: -0.007 min
Response: 56291117
Conc: 14.44 ng/ml m

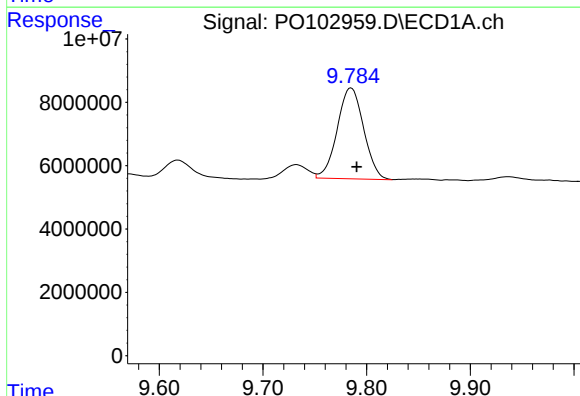

#2 Decachlorobiphenyl

R.T.: 9.784 min
Delta R.T.: -0.006 min
Response: 50731165
Conc: 14.43 ng/ml m

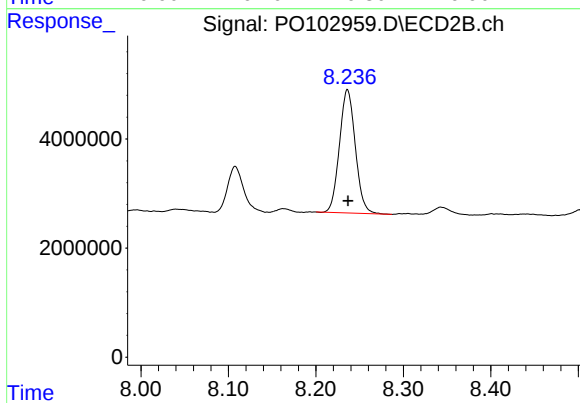

#2 Decachlorobiphenyl

R.T.: 8.236 min
Delta R.T.: 0.000 min
Response: 28511719
Conc: 12.53 ng/ml