

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041924\
 Data File : P0102978.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2024 04:58
 Operator : YP/AJ
 Sample : P2183-06 10X
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ANTIFREEZE-DRUM-1103

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/22/2024
 Supervised By :Ankita Jodhani 04/22/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 20 05:28:34 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0041524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 16 04:30:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.253	3.372	8482671	5363139	1.360m	1.376m
2) SA Decachlor...	9.772	8.228	2866044	1430730	0.815	0.629

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO041924\
Data File : PO102978.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2024 04:58
Operator : YP/AJ
Sample : P2183-06 10X
Misc :
ALS Vial : 42 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
ANTIFREEZE-DRUM-1103


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/22/2024
Supervised By :Ankita Jodhani 04/22/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 05:28:34 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO041524.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 16 04:30:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

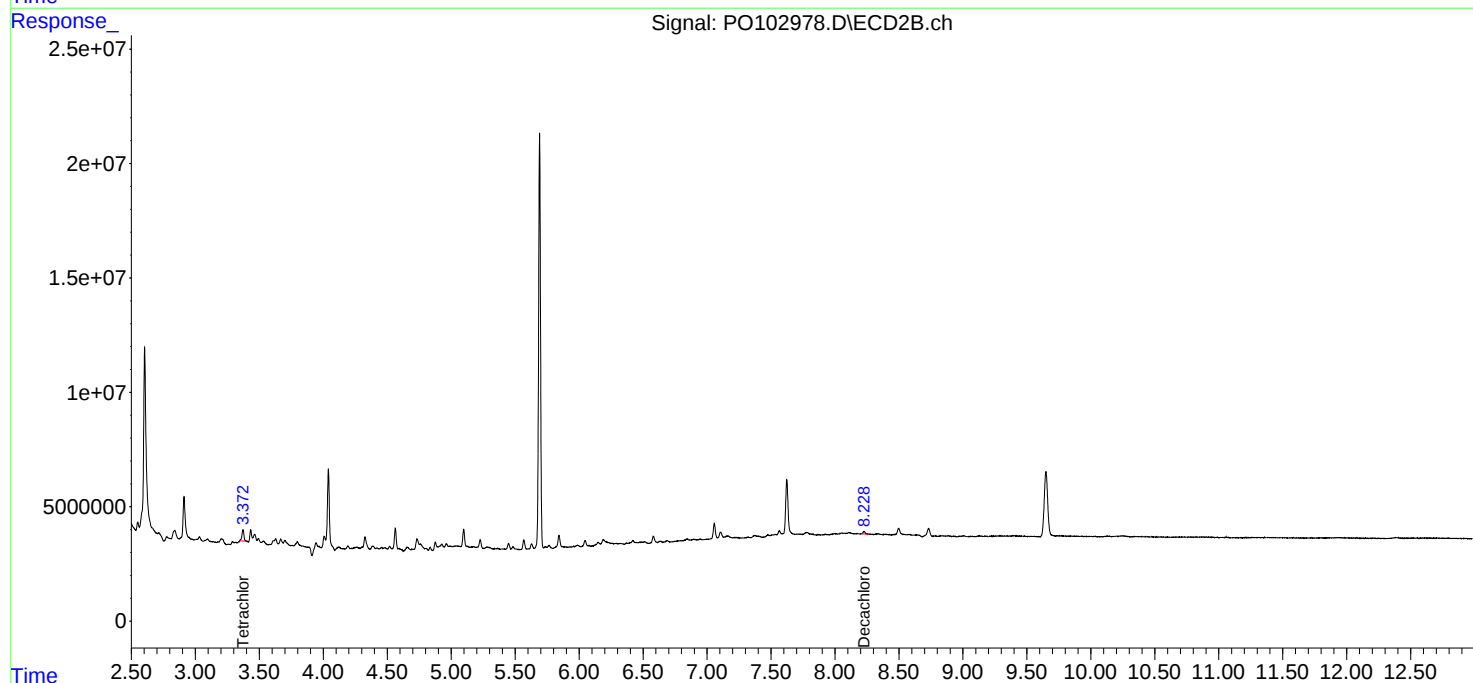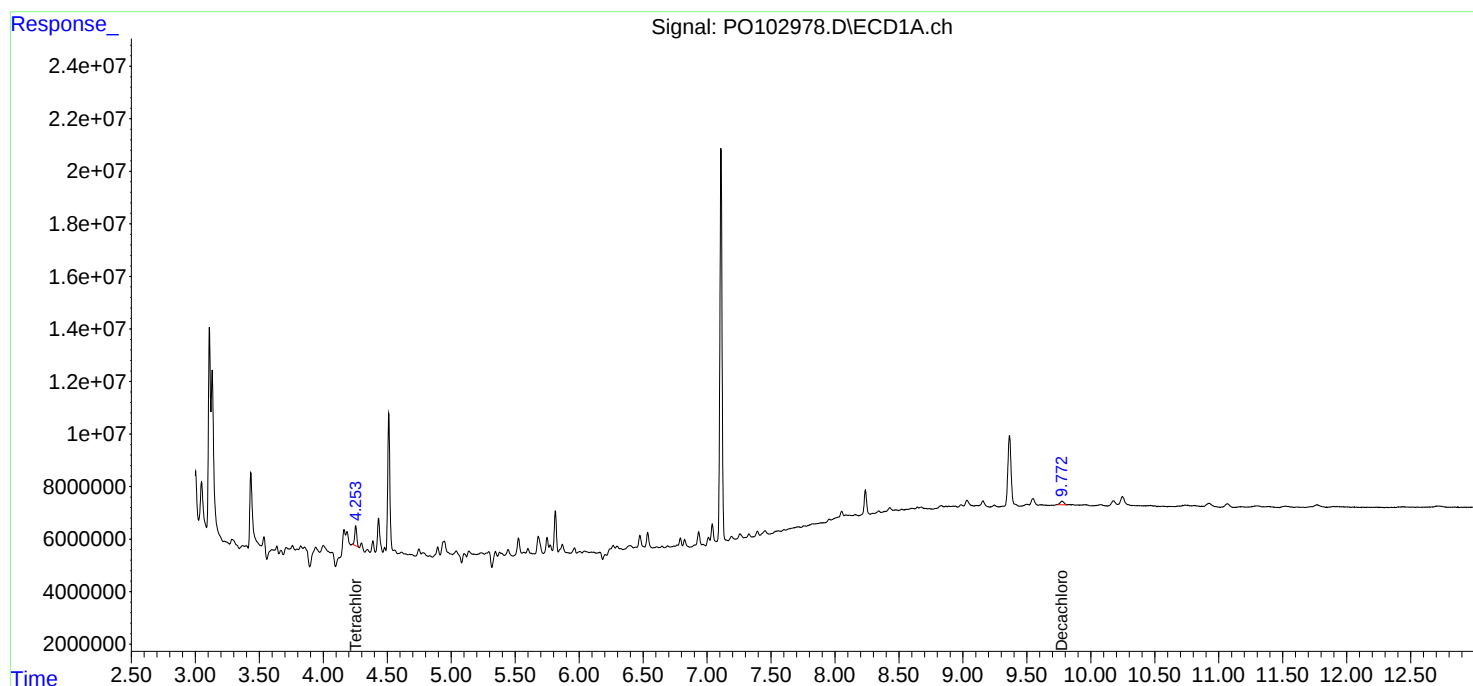

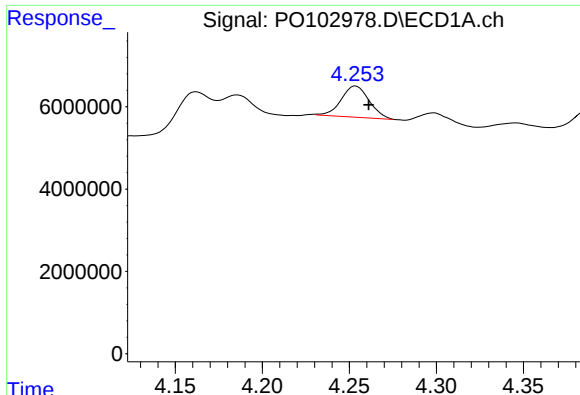


#1 Tetrachloro-m-xylene

R.T.: 4.253 min
Delta R.T.: -0.008 min
Response: 8482671
Conc: 1.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
ANTIFREEZE-DRUM-1103


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/22/2024
Supervised By :Ankita Jodhani 04/22/2024

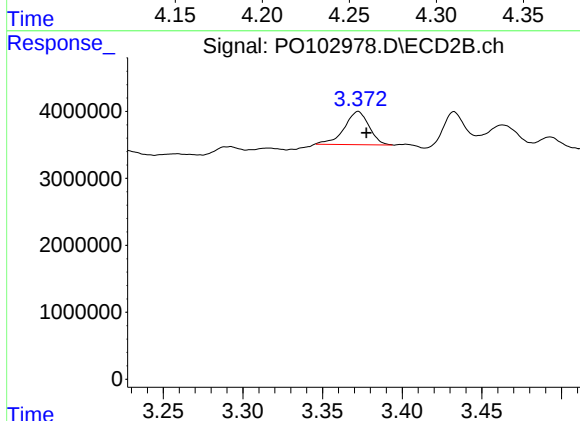


#1 Tetrachloro-m-xylene

R.T.: 3.372 min
Delta R.T.: -0.005 min
Response: 5363139
Conc: 1.38 ng/ml m

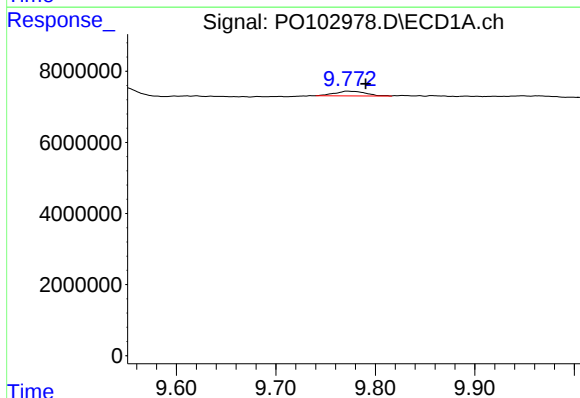

#2 Decachlorobiphenyl

R.T.: 9.772 min
Delta R.T.: -0.018 min
Response: 2866044
Conc: 0.82 ng/ml

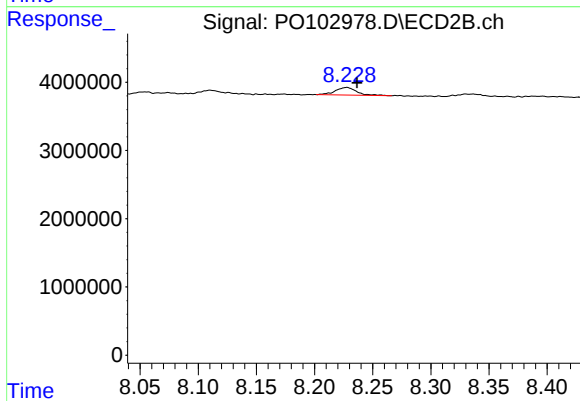

#2 Decachlorobiphenyl

R.T.: 8.228 min
Delta R.T.: -0.009 min
Response: 1430730
Conc: 0.63 ng/ml