

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041924\
 Data File : P0102988.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2024 08:17
 Operator : YP/AJ
 Sample : P2124-01
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 B-131-SB01

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/22/2024
 Supervised By :Ankita Jodhani 04/22/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 20 09:40:00 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0041524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 16 04:30:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.254	3.372	72491276	54453353	11.625m	13.972m
2) SA Decachlor...	9.776	8.227	46182346	27791898	13.137	12.213

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO041924\
Data File : PO102988.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2024 08:17
Operator : YP/AJ
Sample : P2124-01
Misc :
ALS Vial : 47 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
B-131-SB01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/22/2024
Supervised By :Ankita Jodhani 04/22/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 09:40:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO041524.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 16 04:30:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

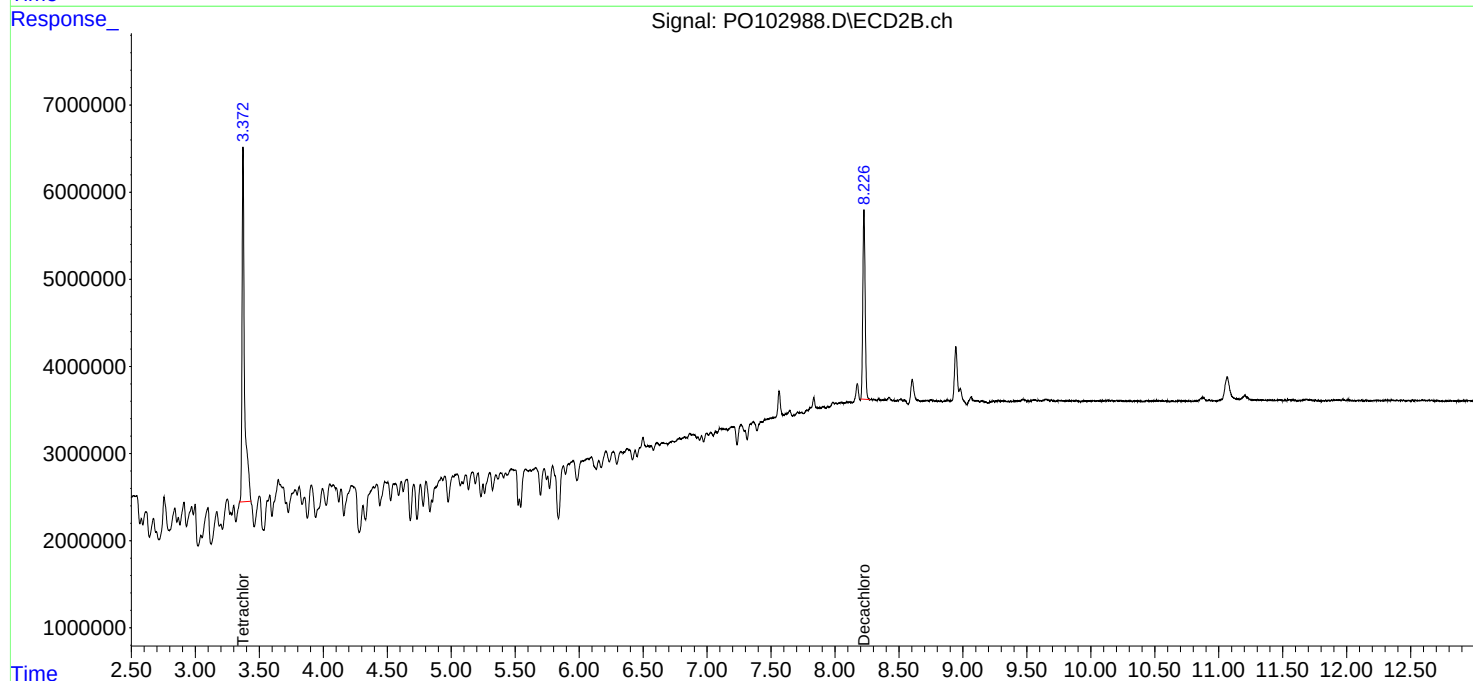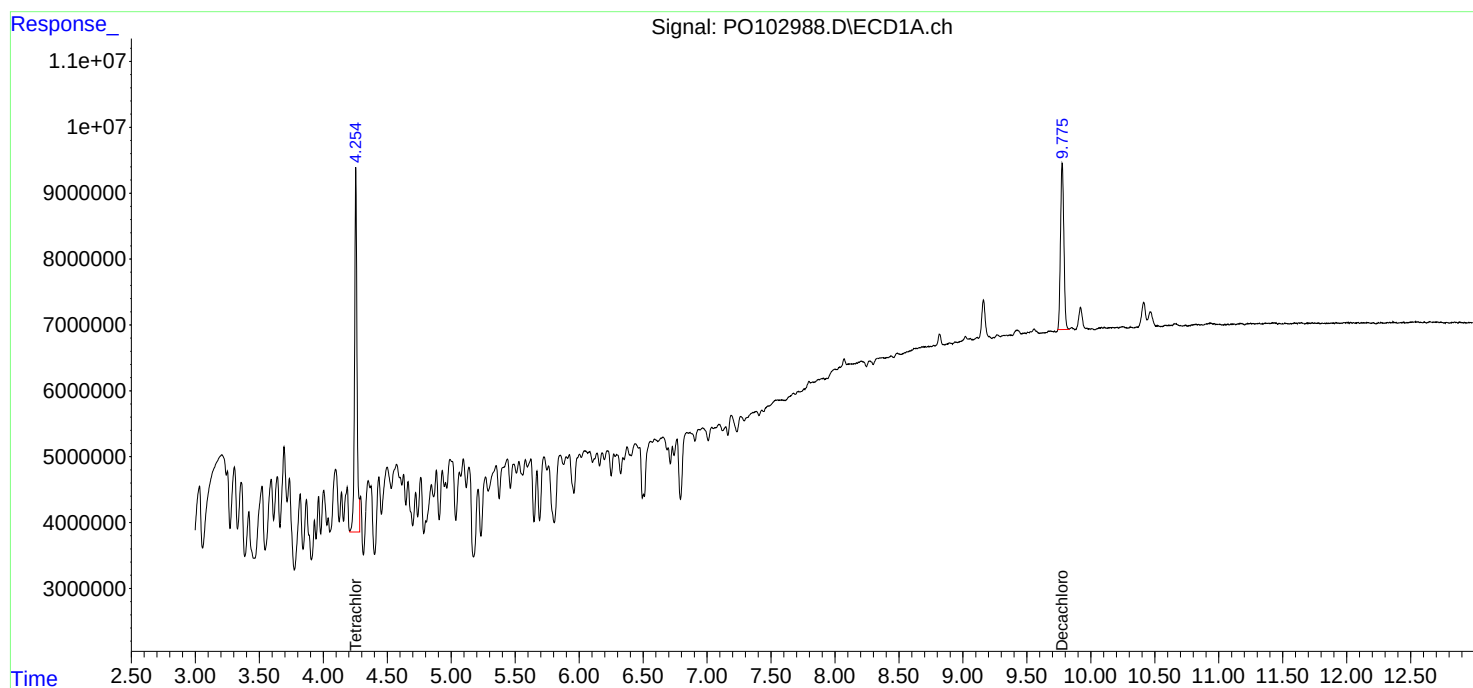

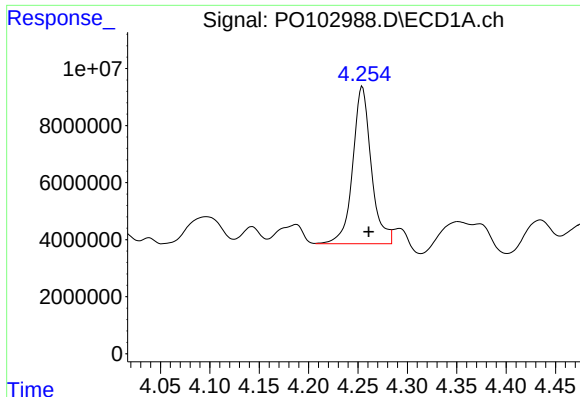


#1 Tetrachloro-m-xylene

R.T.: 4.254 min
Delta R.T.: -0.007 min
Response: 72491276
Conc: 11.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
B-131-SB01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/22/2024
Supervised By :Ankita Jodhani 04/22/2024

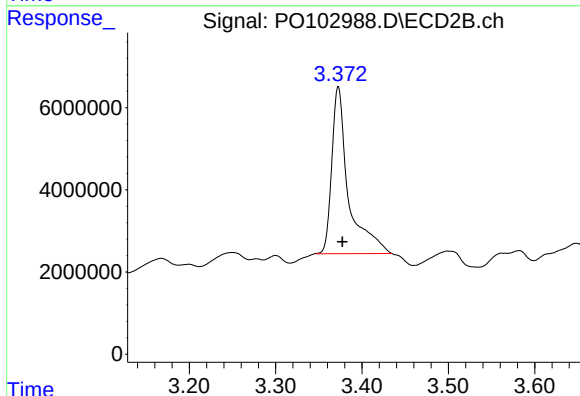


#1 Tetrachloro-m-xylene

R.T.: 3.372 min
Delta R.T.: -0.005 min
Response: 54453353
Conc: 13.97 ng/ml m

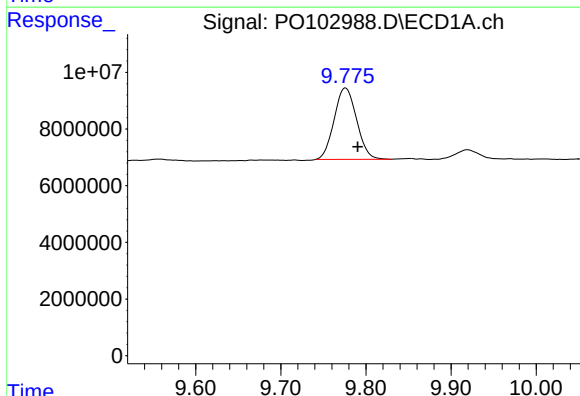

#2 Decachlorobiphenyl

R.T.: 9.776 min
Delta R.T.: -0.014 min
Response: 46182346
Conc: 13.14 ng/ml

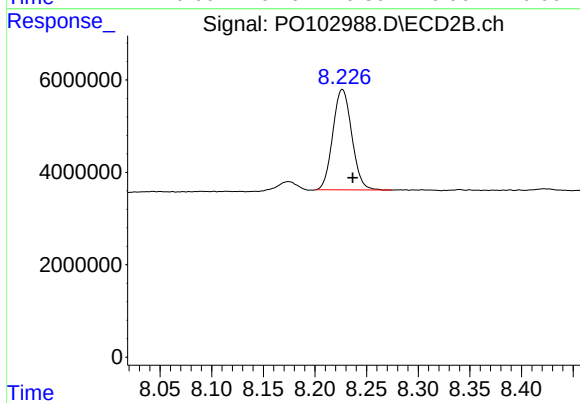

#2 Decachlorobiphenyl

R.T.: 8.227 min
Delta R.T.: -0.010 min
Response: 27791898
Conc: 12.21 ng/ml