

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042023\
 Data File : P0094430.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2023 16:06
 Operator : YP/AJ
 Sample : 02406-04
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-13-COMP

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/21/2023
 Supervised By :Ankita Jodhani 04/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 20 21:53:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0041923.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 20 05:15:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.417	3.620	67684327	26452396	21.039	20.479
2) SA Decachlor...	10.258	8.636	37820302	17828800	17.694	17.900
Target Compounds						
31) L7 AR-1260-1	7.216	6.186	3657787	1931180	27.366	28.768
32) L7 AR-1260-2	7.474	6.376	6196577	1897932	44.266	25.532 #
33) L7 AR-1260-3	7.838	6.528	2416331	1682269	21.189	23.555
34) L7 AR-1260-4	8.059	7.000	3000084	816393	25.066	13.883 #
35) L7 AR-1260-5	8.394	7.246	3230570	1688400	15.666m	14.854

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO042023\
Data File : PO094430.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2023 16:06
Operator : YP/AJ
Sample : 02406-04
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-13-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/21/2023
Supervised By :Ankita Jodhani 04/21/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 21:53:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO041923.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 20 05:15:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

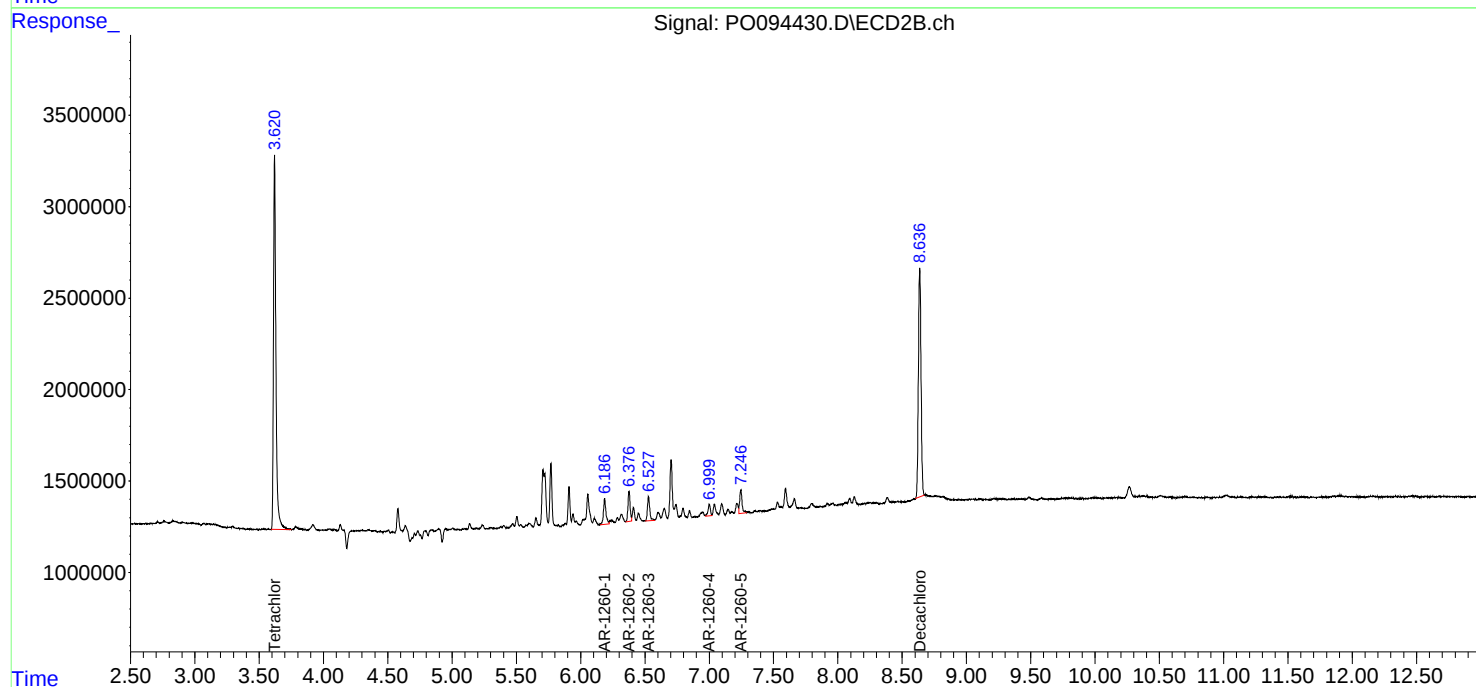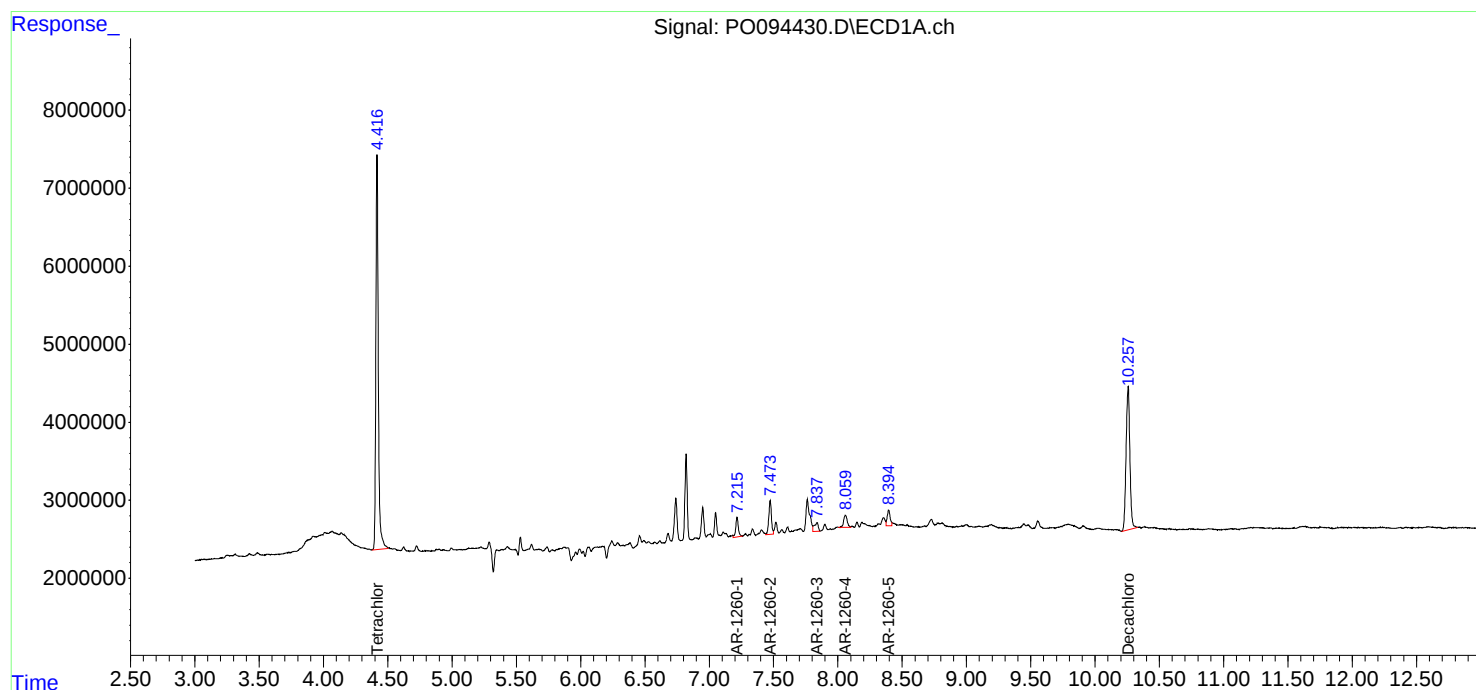

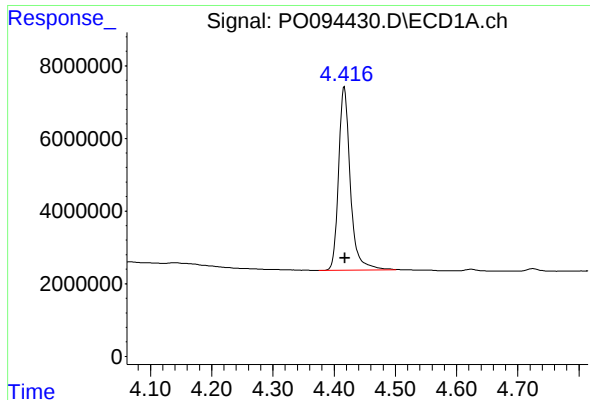


#1 Tetrachloro-m-xylene

R.T.: 4.417 min
Delta R.T.: -0.001 min
Response: 67684327
Conc: 21.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-13-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/21/2023
Supervised By :Ankita Jodhani 04/21/2023

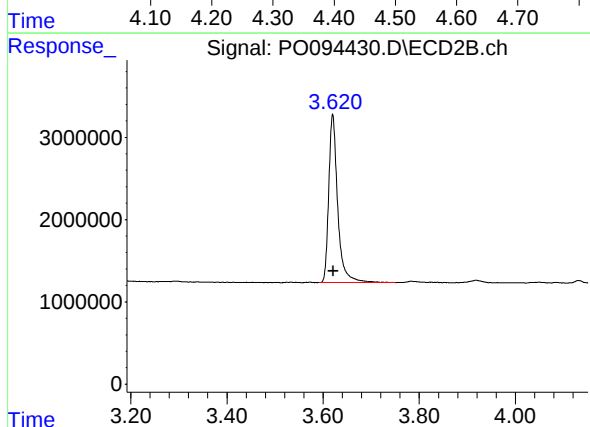


#1 Tetrachloro-m-xylene

R.T.: 3.620 min
Delta R.T.: -0.001 min
Response: 26452396
Conc: 20.48 ng/ml

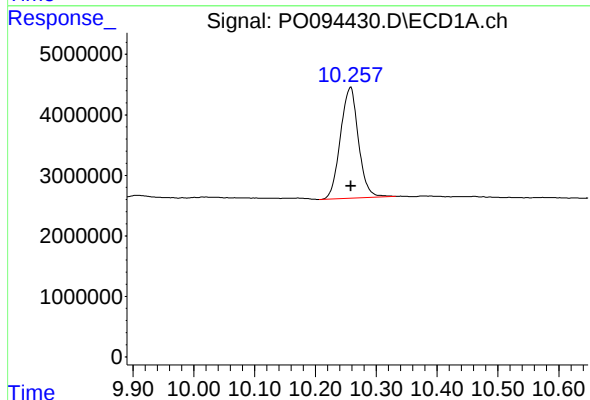


#2 Decachlorobiphenyl

R.T.: 10.258 min
Delta R.T.: -0.001 min
Response: 37820302
Conc: 17.69 ng/ml

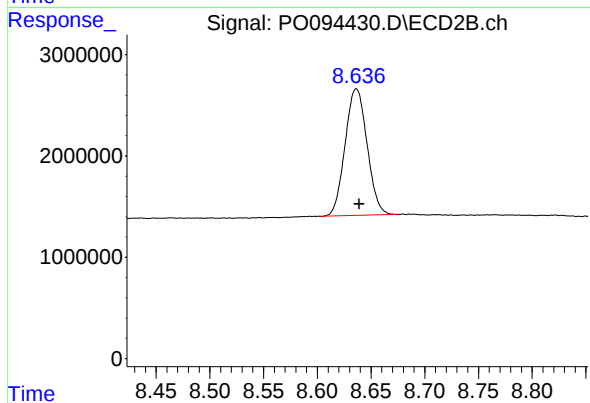

#2 Decachlorobiphenyl

R.T.: 8.636 min
Delta R.T.: -0.003 min
Response: 17828800
Conc: 17.90 ng/ml

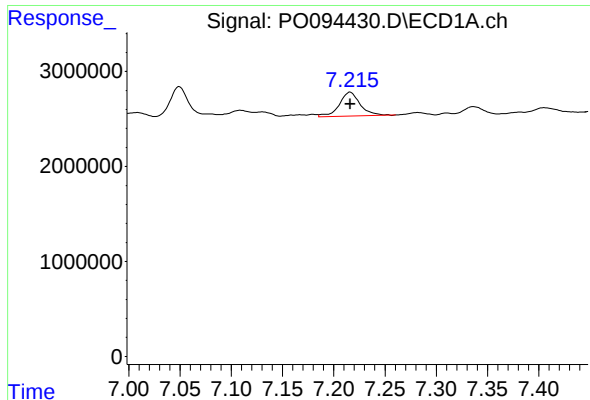


#31 AR-1260-1

R.T.: 7.216 min
Delta R.T.: 0.000 min
Response: 3657787
Conc: 27.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-13-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/21/2023
Supervised By :Ankita Jodhani 04/21/2023

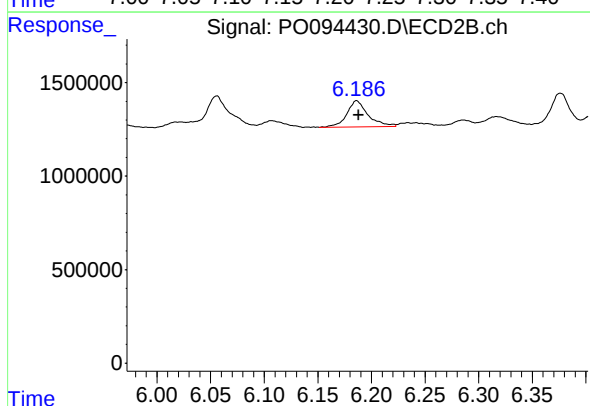


#31 AR-1260-1

R.T.: 6.186 min
Delta R.T.: -0.002 min
Response: 1931180
Conc: 28.77 ng/ml

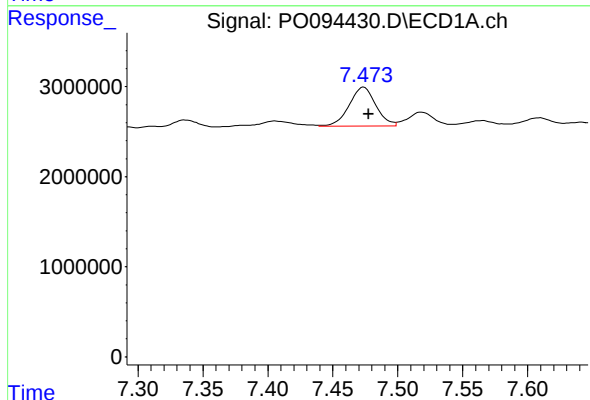


#32 AR-1260-2

R.T.: 7.474 min
Delta R.T.: -0.004 min
Response: 6196577
Conc: 44.27 ng/ml

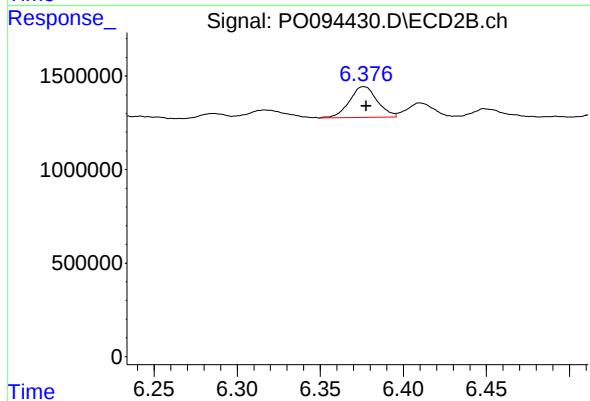

#32 AR-1260-2

R.T.: 6.376 min
Delta R.T.: -0.001 min
Response: 1897932
Conc: 25.53 ng/ml

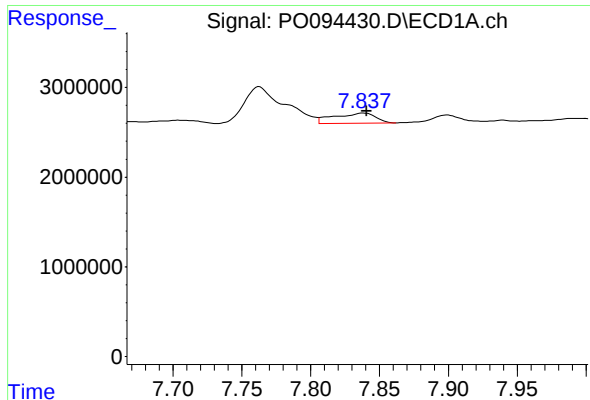


#33 AR-1260-3

R.T.: 7.838 min
Delta R.T.: -0.003 min
Response: 2416331
Conc: 21.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-13-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/21/2023
Supervised By :Ankita Jodhani 04/21/2023

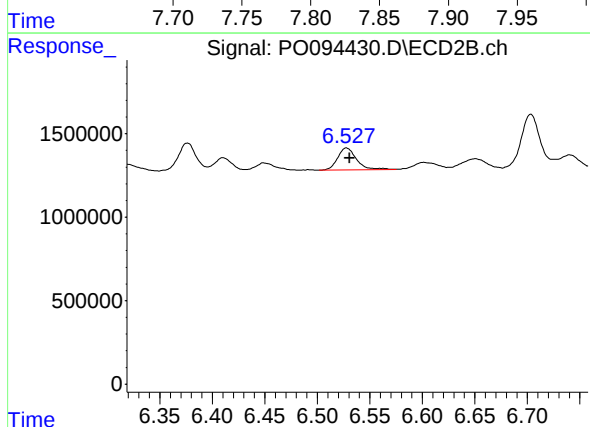


#33 AR-1260-3

R.T.: 6.528 min
Delta R.T.: -0.003 min
Response: 1682269
Conc: 23.55 ng/ml

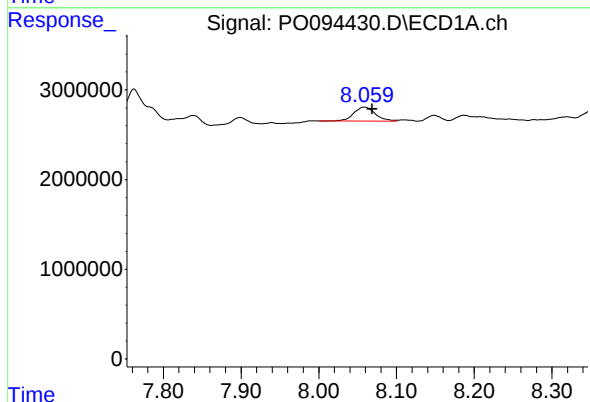


#34 AR-1260-4

R.T.: 8.059 min
Delta R.T.: -0.010 min
Response: 3000084
Conc: 25.07 ng/ml

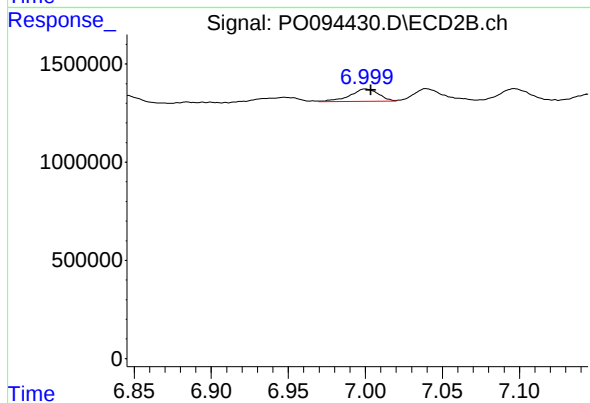

#34 AR-1260-4

R.T.: 7.000 min
Delta R.T.: -0.004 min
Response: 816393
Conc: 13.88 ng/ml

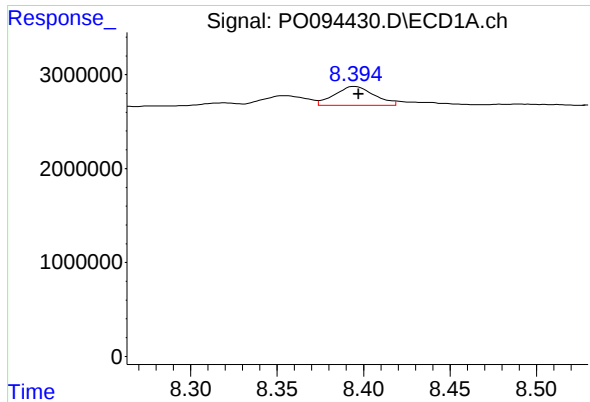


#35 AR-1260-5

R.T.: 8.394 min
Delta R.T.: -0.003 min
Response: 3230570
Conc: 15.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-13-COMP

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/21/2023
Supervised By :Ankita Jodhani 04/21/2023

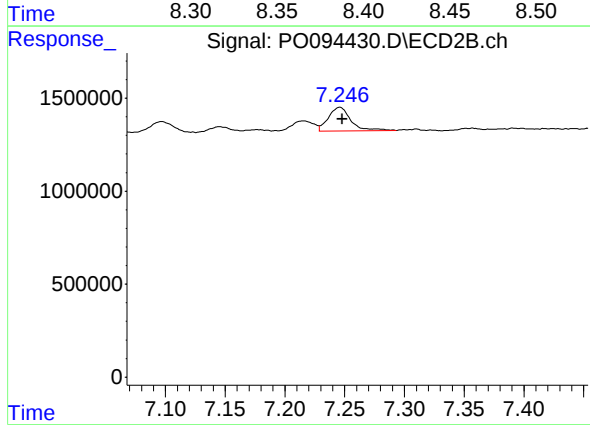

#35 AR-1260-5

R.T.: 7.246 min
Delta R.T.: -0.002 min
Response: 1688400
Conc: 14.85 ng/ml