

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042023\
 Data File : P0094431.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2023 16:23
 Operator : YP/AJ
 Sample : 02406-06
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-14-COMP

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/21/2023
 Supervised By :Ankita Jodhani 04/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 20 21:54:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0041923.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 20 05:15:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.417	3.620	74130983	29323404	23.043	22.701
2) SA Decachlor...	10.256	8.636	49983146	23549935	23.384	23.644m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042023\
Data File : P0094431.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2023 16:23
Operator : YP/AJ
Sample : 02406-06
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-14-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/21/2023
Supervised By :Ankita Jodhani 04/21/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 21:54:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0041923.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 20 05:15:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

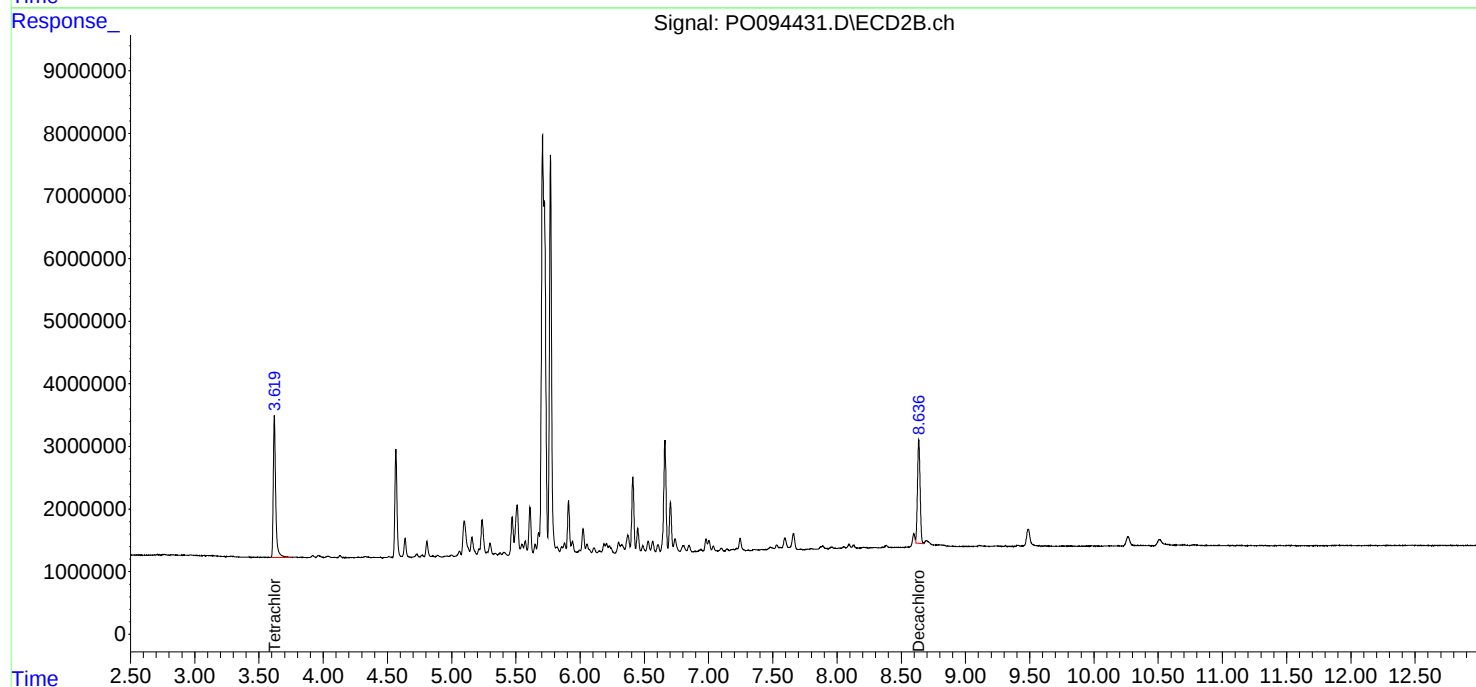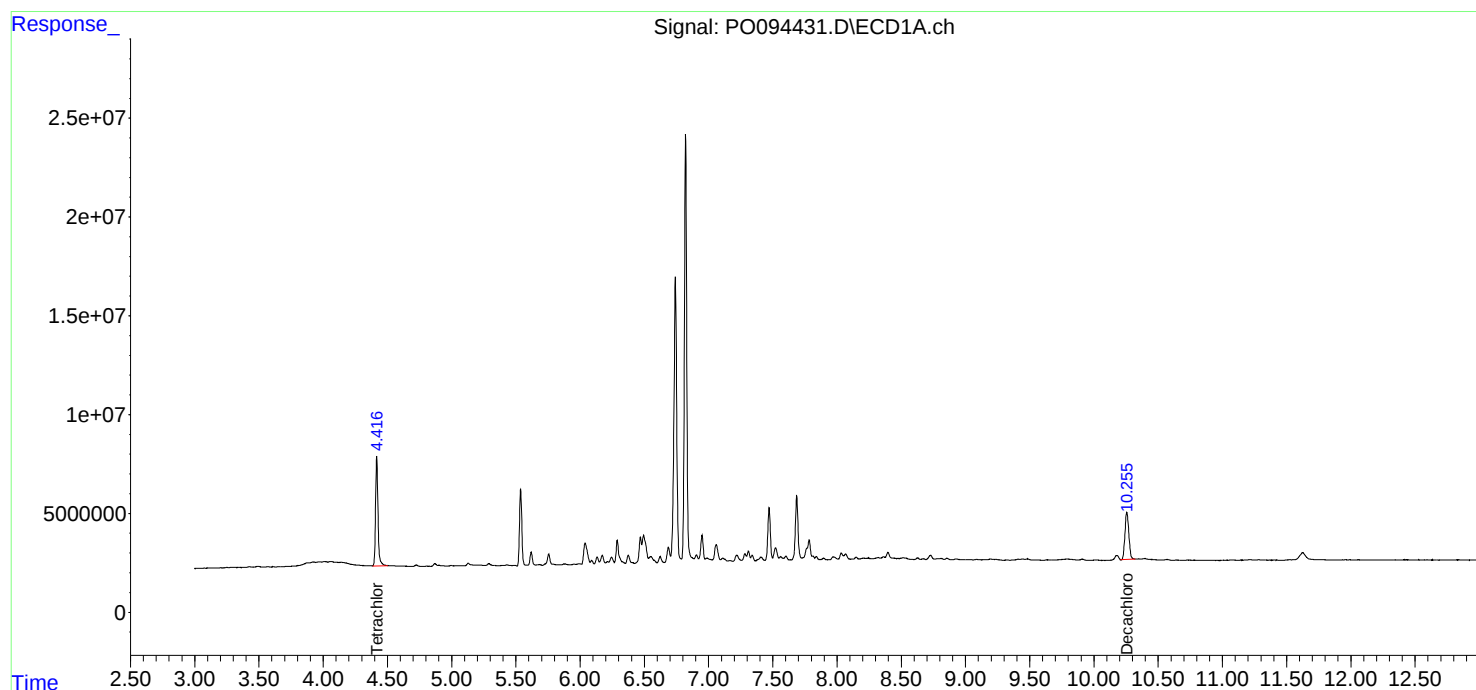

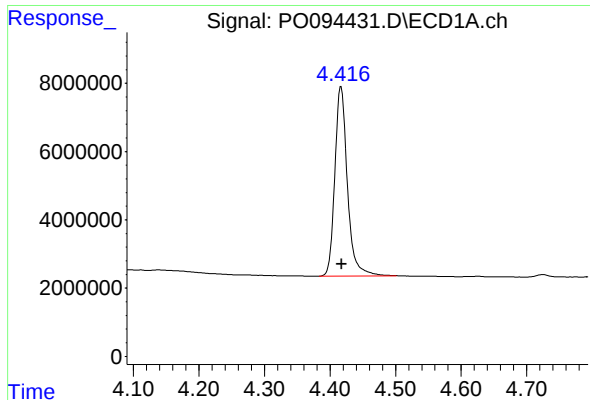


#1 Tetrachloro-m-xylene

R.T.: 4.417 min
Delta R.T.: -0.001 min
Response: 74130983
Conc: 23.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-14-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/21/2023
Supervised By :Ankita Jodhani 04/21/2023

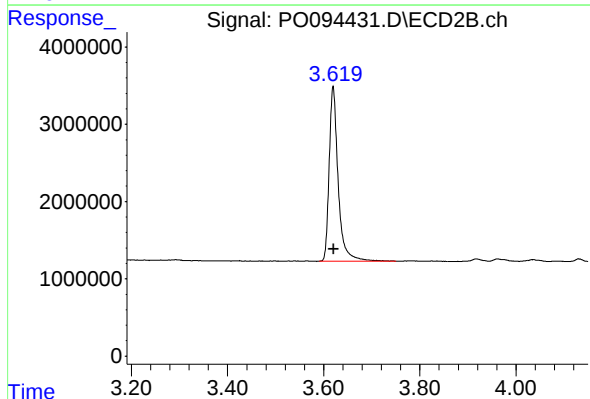


#1 Tetrachloro-m-xylene

R.T.: 3.620 min
Delta R.T.: -0.002 min
Response: 29323404
Conc: 22.70 ng/ml

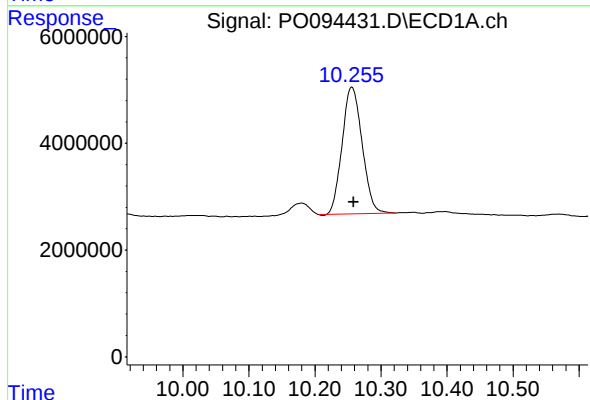

#2 Decachlorobiphenyl

R.T.: 10.256 min
Delta R.T.: -0.003 min
Response: 49983146
Conc: 23.38 ng/ml

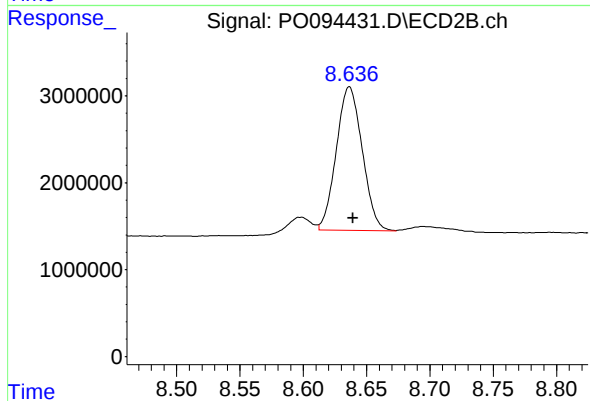

#2 Decachlorobiphenyl

R.T.: 8.636 min
Delta R.T.: -0.003 min
Response: 23549935
Conc: 23.64 ng/ml m