

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042121\
 Data File : P0077060.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Apr 2021 16:33
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 12:10:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 09:50:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.895	3.892	2060971	1043418	19.502	19.832
2) SA Decachlor...	10.861	9.131	2051703	754384	19.762	19.992
Target Compounds						
9) L2 AR-1221-2	5.249	4.241	25645	13741	30.189	30.072



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO042121\
Data File : PO077060.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Apr 2021 16:33
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 12:10:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 09:50:22 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

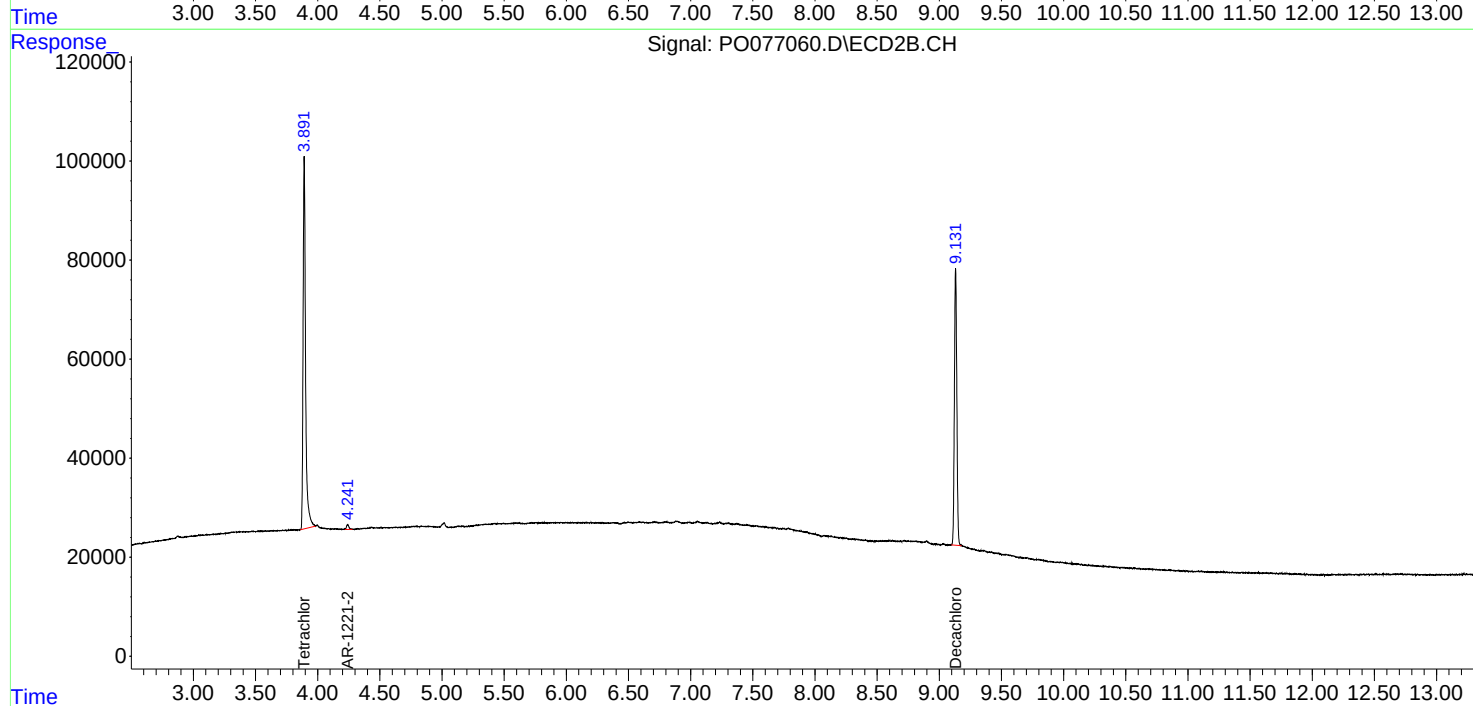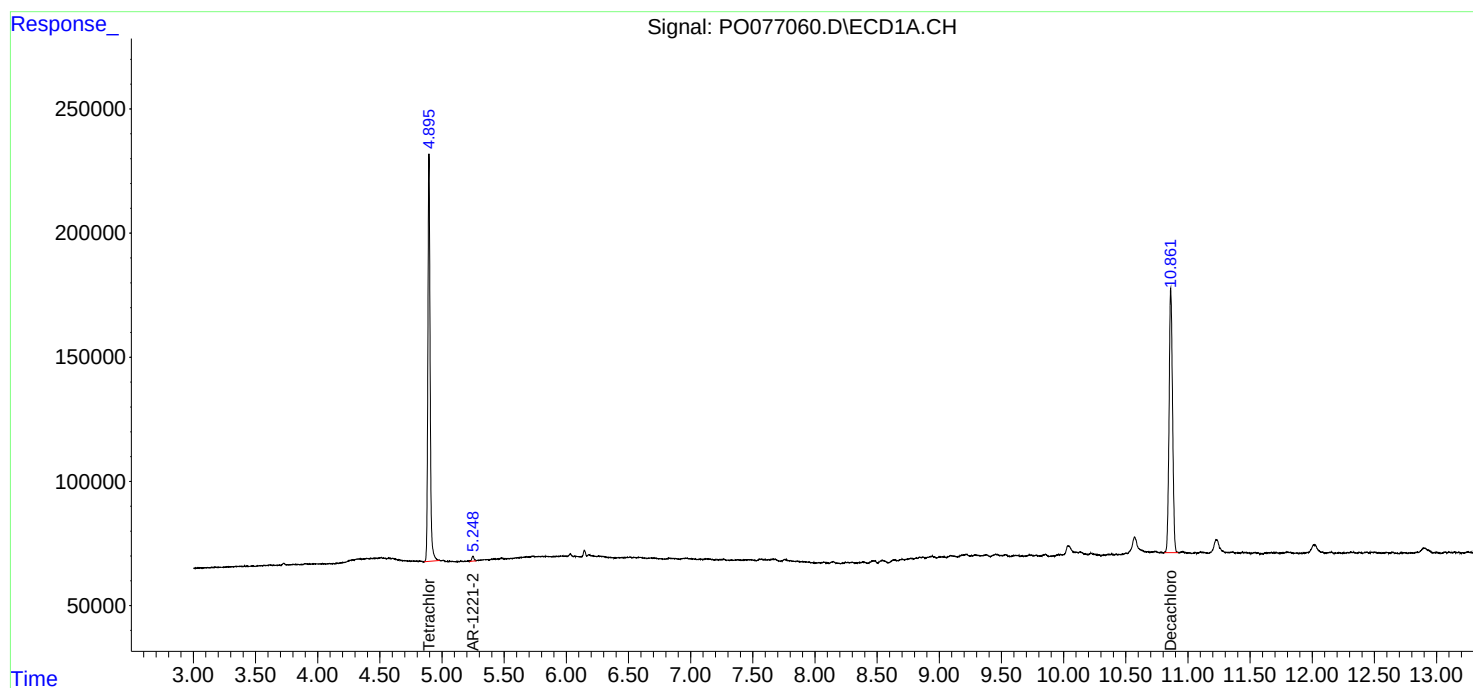


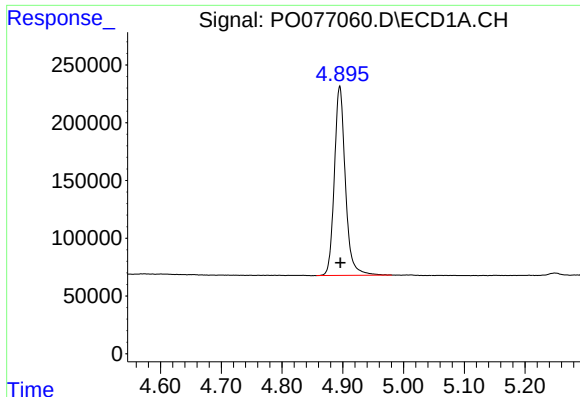

#1 Tetrachloro-m-xylene


R.T.: 4.895 min
Delta R.T.: 0.000 min
Response: 2060971
Conc: 19.50 ng/ml

Instrument :
ECD_O
ClientSampleId :

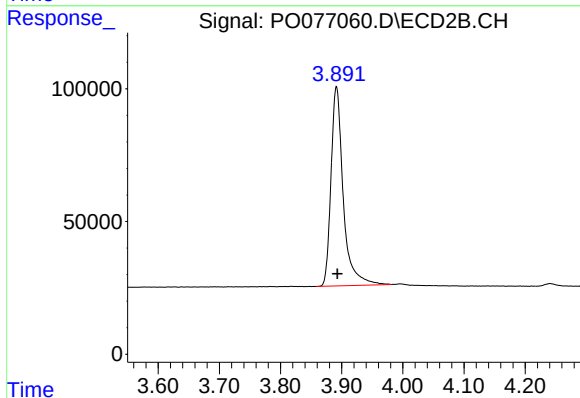


#1 Tetrachloro-m-xylene

R.T.: 3.892 min
Delta R.T.: -0.001 min
Response: 1043418
Conc: 19.83 ng/ml

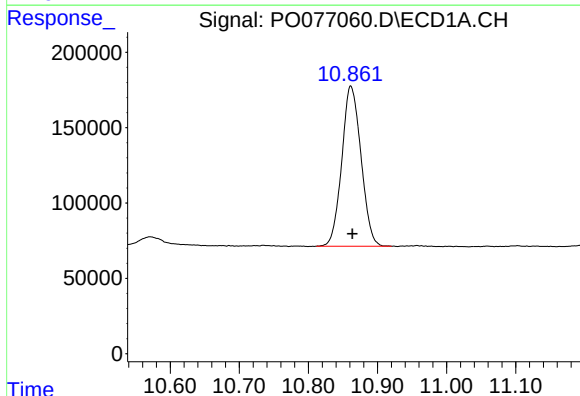


#2 Decachlorobiphenyl

R.T.: 10.861 min
Delta R.T.: -0.002 min
Response: 2051703
Conc: 19.76 ng/ml

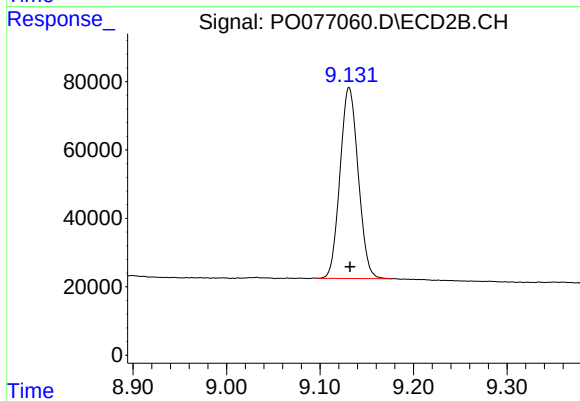

#2 Decachlorobiphenyl


R.T.: 9.131 min
Delta R.T.: -0.001 min
Response: 754384
Conc: 19.99 ng/ml

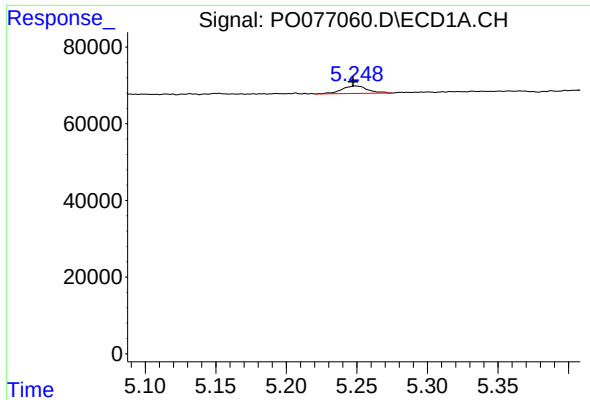

#9 AR-1221-2

R.T.: 5.249 min
Delta R.T.: 0.002 min
Response: 25645
Conc: 30.19 ng/ml

Instrument :
ECD_O
ClientSampleId :

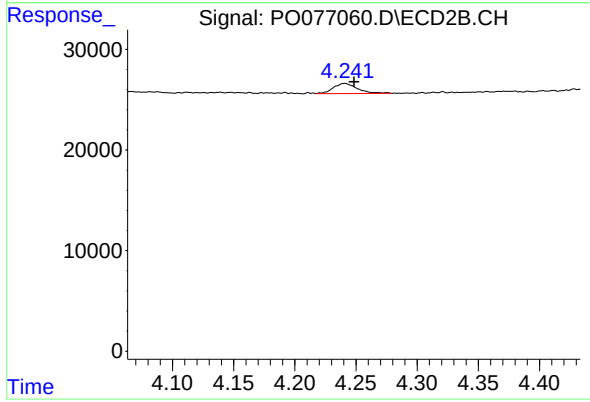

#9 AR-1221-2

R.T.: 4.241 min
Delta R.T.: -0.007 min
Response: 13741
Conc: 30.07 ng/ml