

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042121\
 Data File : P0077116.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Apr 2021 13:51
 Operator : DD\AJ
 Sample : M2080-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 2516

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 14:11:17 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 09:50:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.897	3.892	2434347	1225413	23.035	23.292
2)	SA Decachlor...	10.866	9.133	2380962	849274	22.933	22.507
Target Compounds							
7)	L1 AR-1016-5	0.000	5.618	0	27082	N.D.	18.306 #
8)	L2 AR-1221-1	5.156	0.000	127226	0	112.173	N.D. #
9)	L2 AR-1221-2	5.250	4.240	27943	12871	32.894	28.169
15)	L3 AR-1232-5	0.000	5.618	0	27082	N.D.	45.470 #
24)	L5 AR-1248-4	0.000	5.618	0	27082	N.D.	14.432 #
30)	L6 AR-1254-5	8.468	0.000	84646	0	15.205	N.D. #
31)	L7 AR-1260-1	0.000	6.717	0	12424	N.D.	4.162 #
34)	L7 AR-1260-4	8.737f	0.000	33032	0	6.828	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042121\
Data File : P0077116.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Apr 2021 13:51
Operator : DD\AJ
Sample : M2080-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
2516

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 14:11:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 09:50:22 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

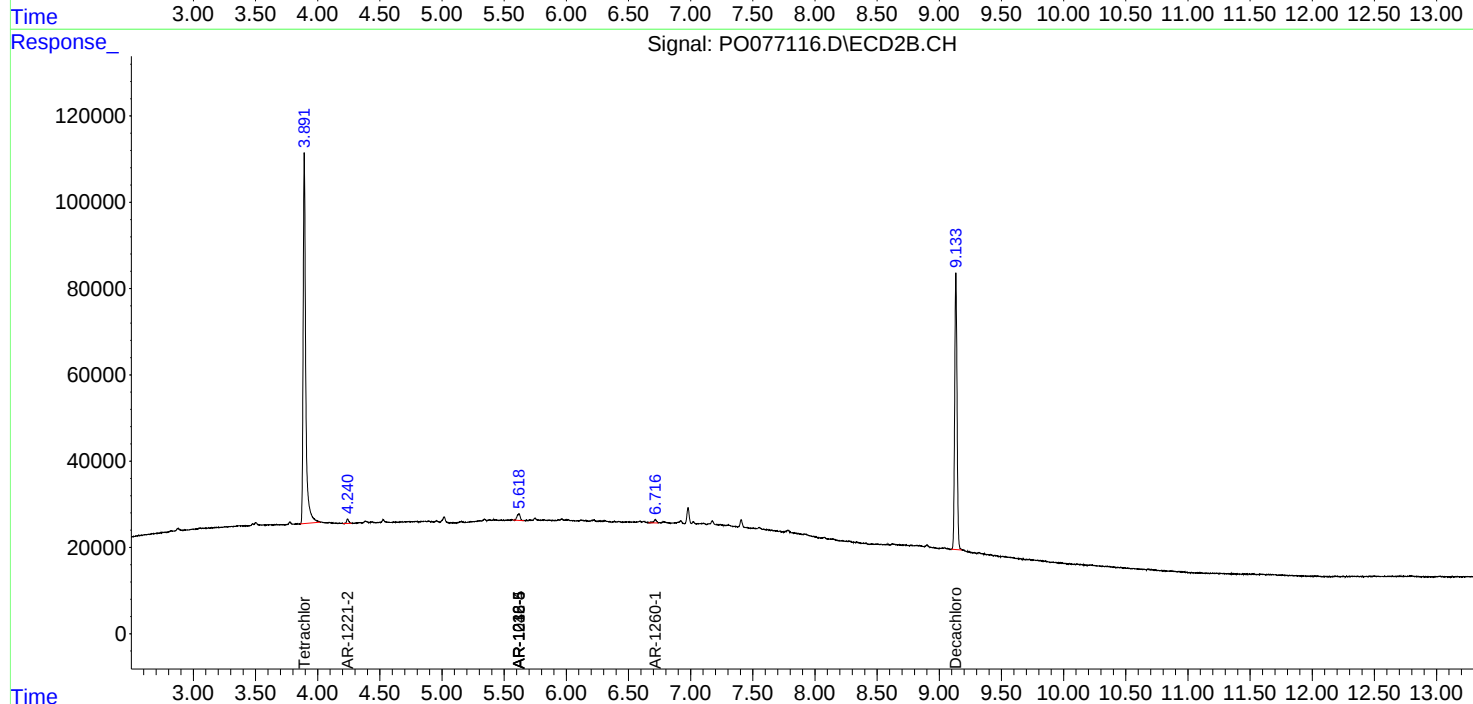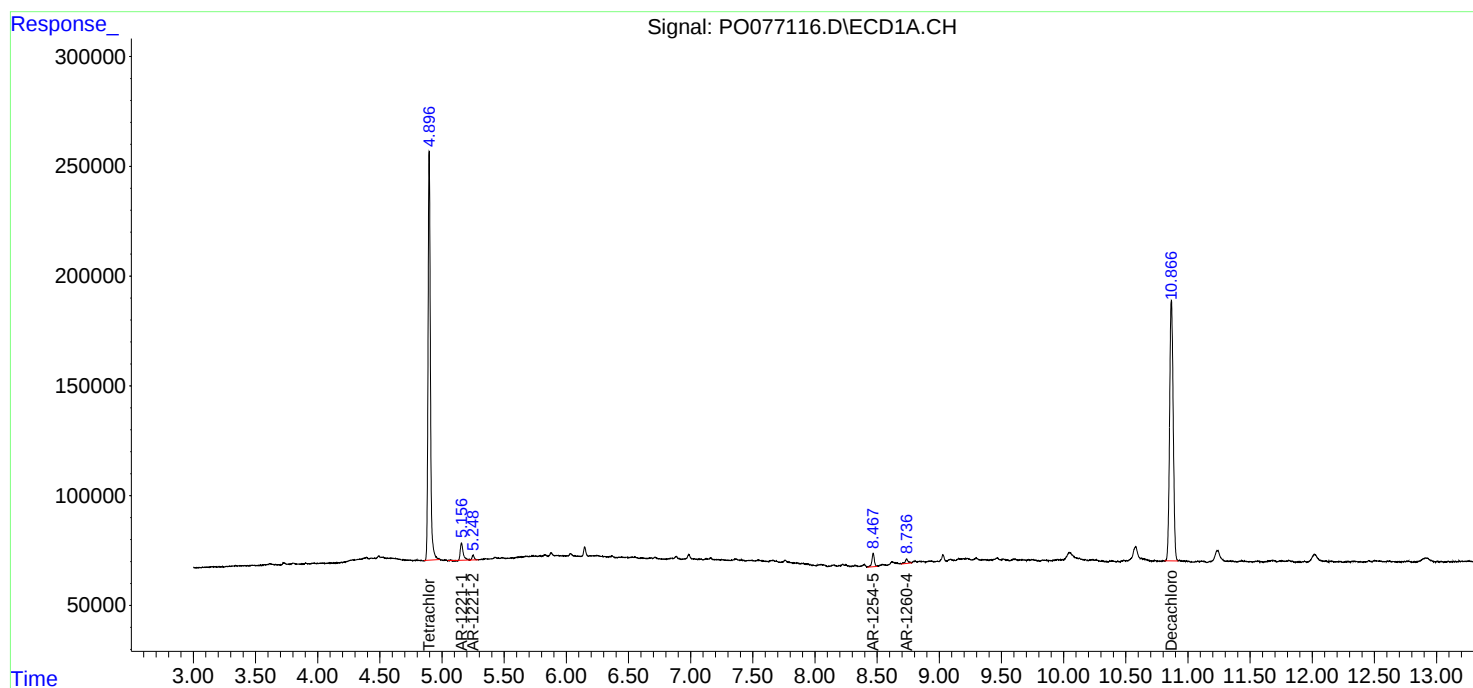


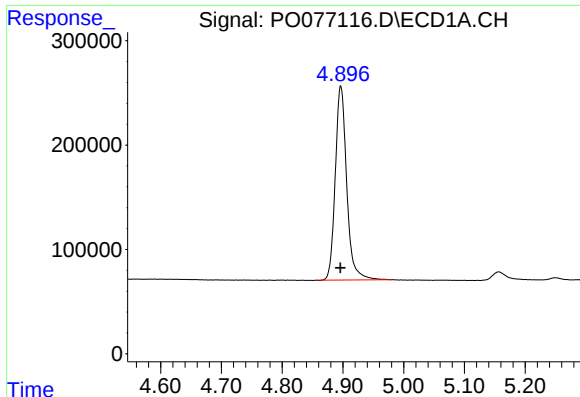

#1 Tetrachloro-m-xylene


R.T.: 4.897 min
Delta R.T.: 0.000 min
Response: 2434347
Conc: 23.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
2516

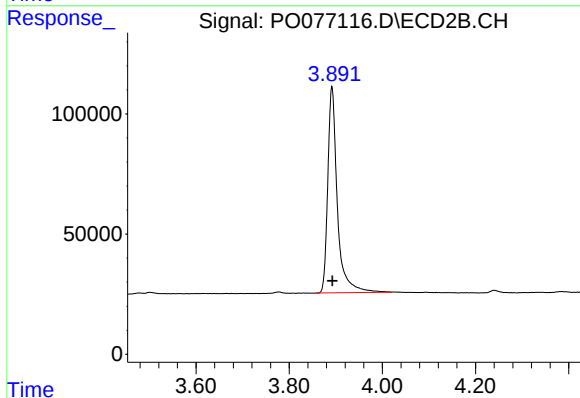


#1 Tetrachloro-m-xylene

R.T.: 3.892 min
Delta R.T.: 0.000 min
Response: 1225413
Conc: 23.29 ng/ml

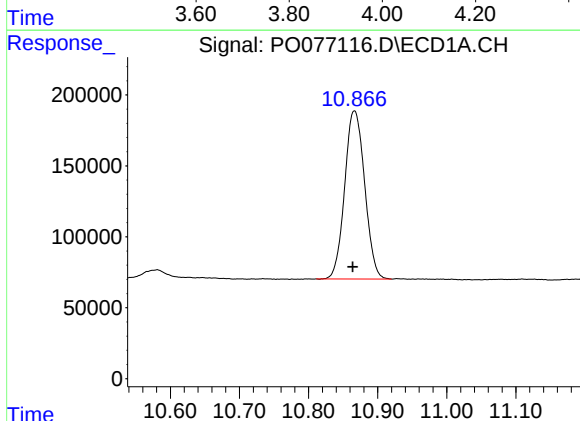


#2 Decachlorobiphenyl

R.T.: 10.866 min
Delta R.T.: 0.003 min
Response: 2380962
Conc: 22.93 ng/ml

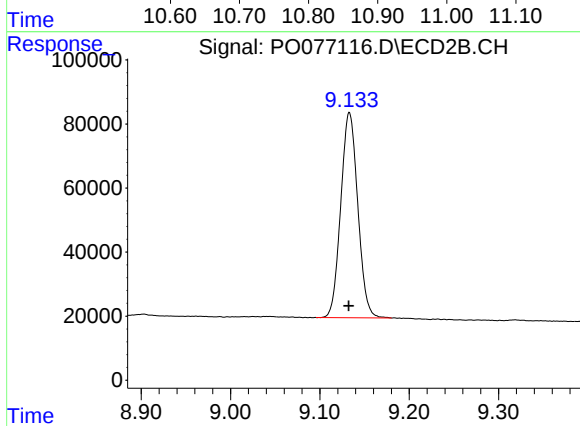

#2 Decachlorobiphenyl


R.T.: 9.133 min
Delta R.T.: 0.000 min
Response: 849274
Conc: 22.51 ng/ml

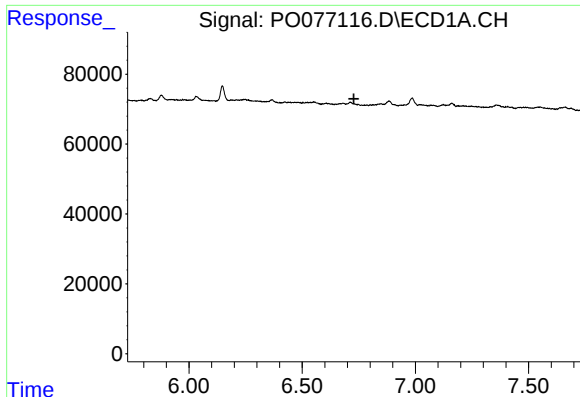

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 6.729 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
2516

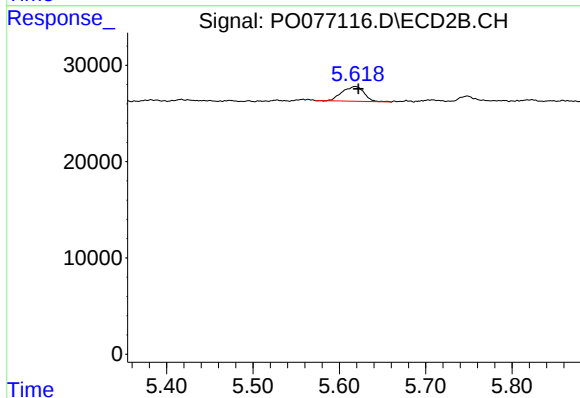


#7 AR-1016-5

R.T.: 5.618 min
Delta R.T.: -0.004 min
Response: 27082
Conc: 18.31 ng/ml

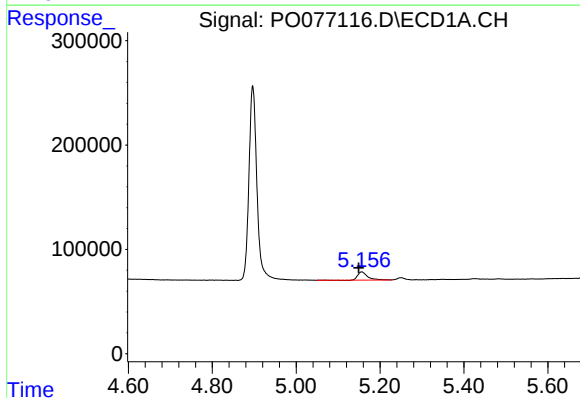


#8 AR-1221-1

R.T.: 5.156 min
Delta R.T.: 0.007 min
Response: 127226
Conc: 112.17 ng/ml

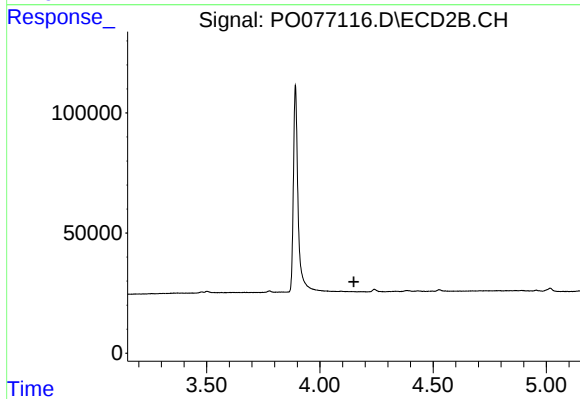

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T.: 4.150 min
Response: 0
Conc: N.D.

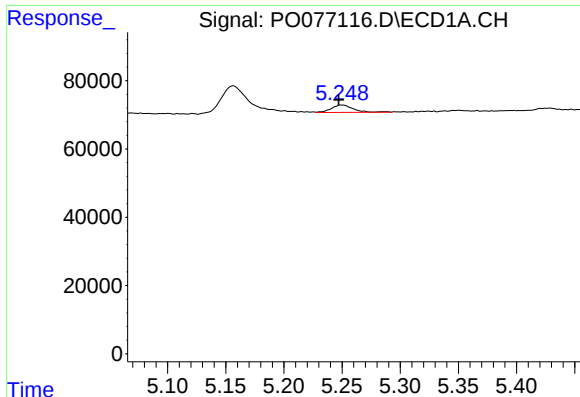

#9 AR-1221-2


R.T.: 5.250 min
Delta R.T.: 0.003 min
Response: 27943
Conc: 32.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
2516

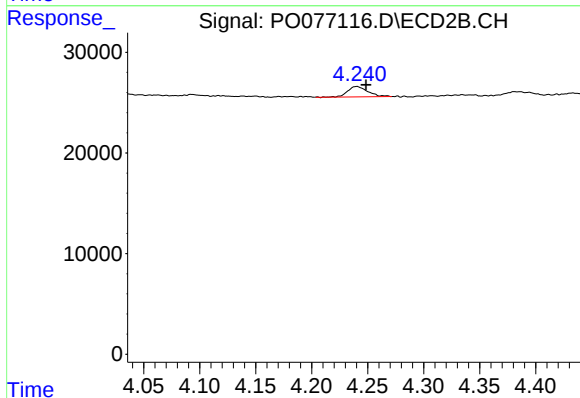


#9 AR-1221-2

R.T.: 4.240 min
Delta R.T.: -0.008 min
Response: 12871
Conc: 28.17 ng/ml

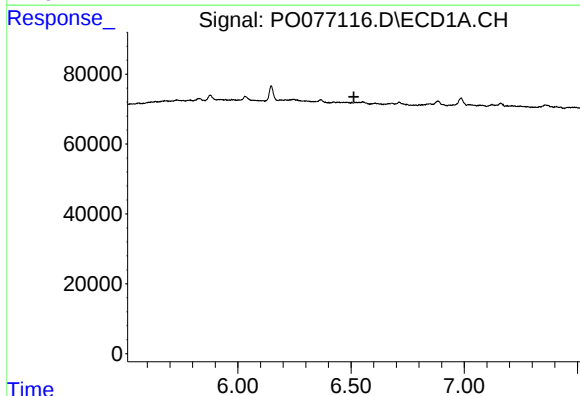


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 6.512 min
Response: 0
Conc: N.D.

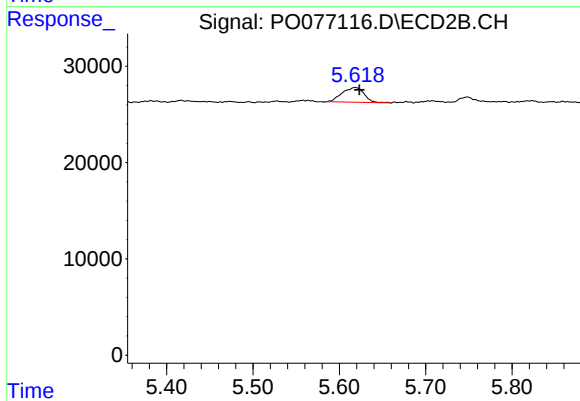

#15 AR-1232-5


R.T.: 5.618 min
Delta R.T.: -0.005 min
Response: 27082
Conc: 45.47 ng/ml

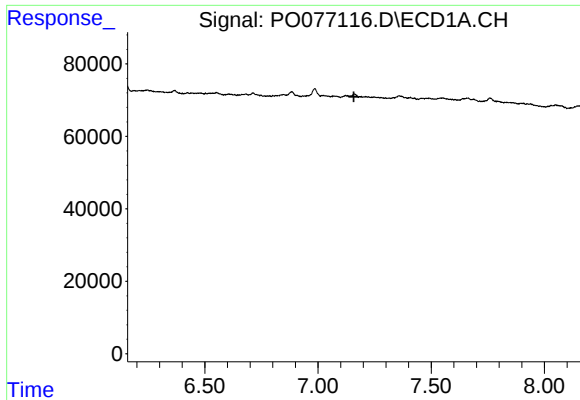

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 7.158 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
2516

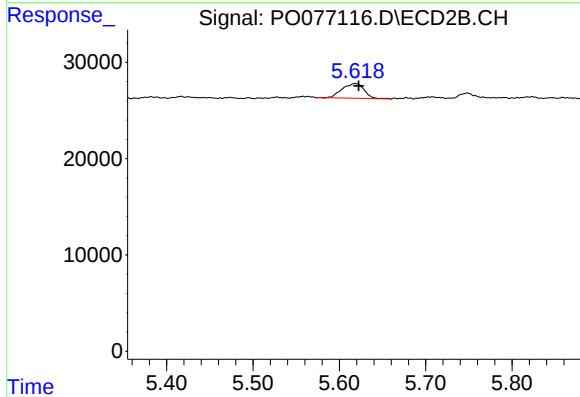


#24 AR-1248-4

R.T.: 5.618 min
Delta R.T.: -0.004 min
Response: 27082
Conc: 14.43 ng/ml

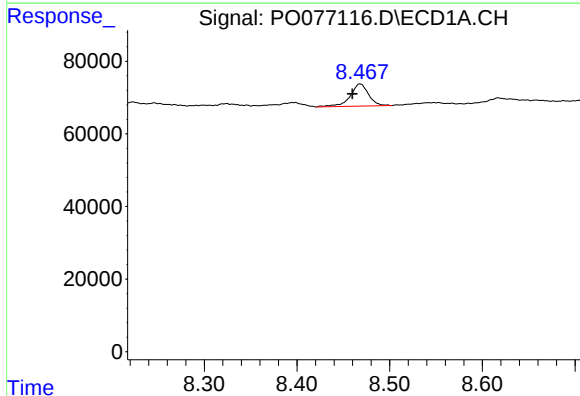


#30 AR-1254-5

R.T.: 8.468 min
Delta R.T.: 0.008 min
Response: 84646
Conc: 15.21 ng/ml

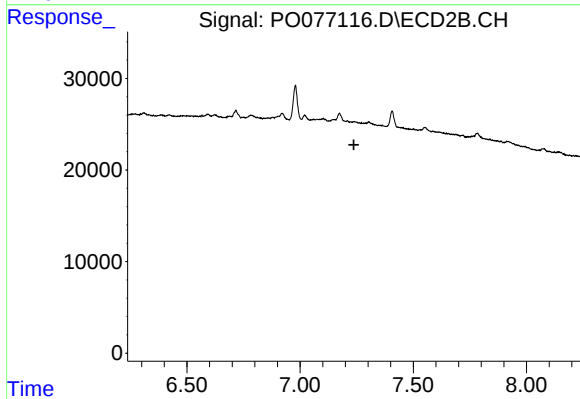

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T.: 7.237 min
Response: 0
Conc: N.D.

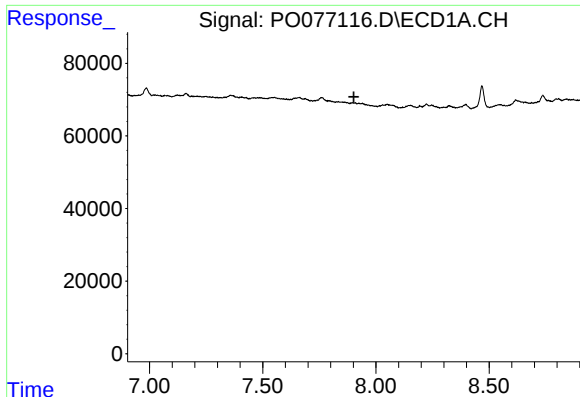

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 7.903 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
2516

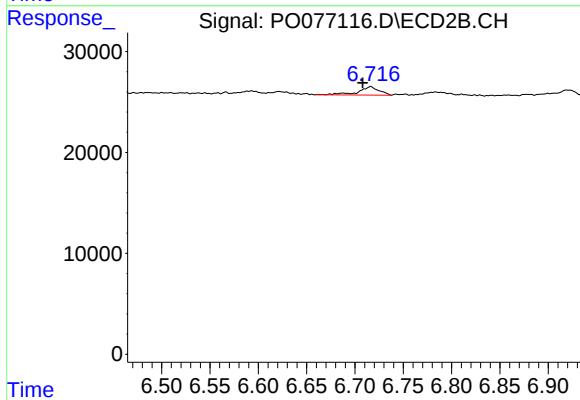


#31 AR-1260-1

R.T.: 6.717 min
Delta R.T.: 0.008 min
Response: 12424
Conc: 4.16 ng/ml

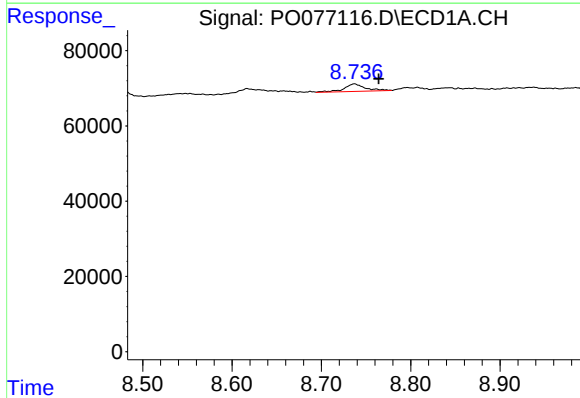

#34 AR-1260-4

R.T.: 8.737 min
Delta R.T.: -0.027 min
Response: 33032
Conc: 6.83 ng/ml

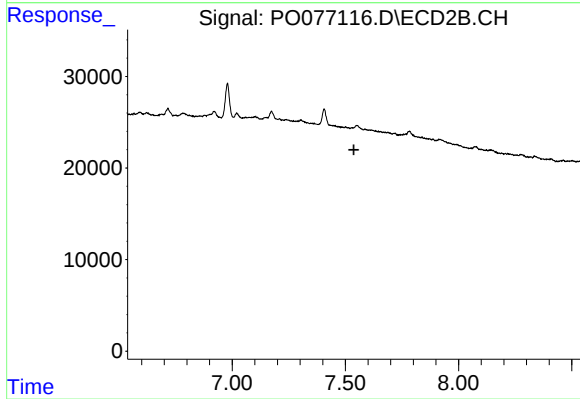

#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 7.537 min
Response: 0
Conc: N.D.