

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042221\
 Data File : P0077130.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Apr 2021 17:51
 Operator : DD\AJ
 Sample : M2075-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-2-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 01:57:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 09:50:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.897	3.893	2294537	1157005	21.712	21.991
2)	SA Decachlor...	10.862	9.133	2201796	785279	21.207	20.811
Target Compounds							
7)	L1 AR-1016-5	0.000	5.606f	0	25111	N.D.	16.974 #
8)	L2 AR-1221-1	5.158	0.000	74045	0	65.284	N.D. #
9)	L2 AR-1221-2	5.250	4.241	25072	12517	29.514	27.394
15)	L3 AR-1232-5	0.000	5.606f	0	25111	N.D.	42.161 #
24)	L5 AR-1248-4	0.000	5.606f	0	25111	N.D.	13.381 #
28)	L6 AR-1254-3	7.760f	0.000	23463	0	3.467	N.D. #
34)	L7 AR-1260-4	8.737f	0.000	44663	0	9.232	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042221\
Data File : P0077130.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Apr 2021 17:51
Operator : DD\AJ
Sample : M2075-07
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-2-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 01:57:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 09:50:22 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

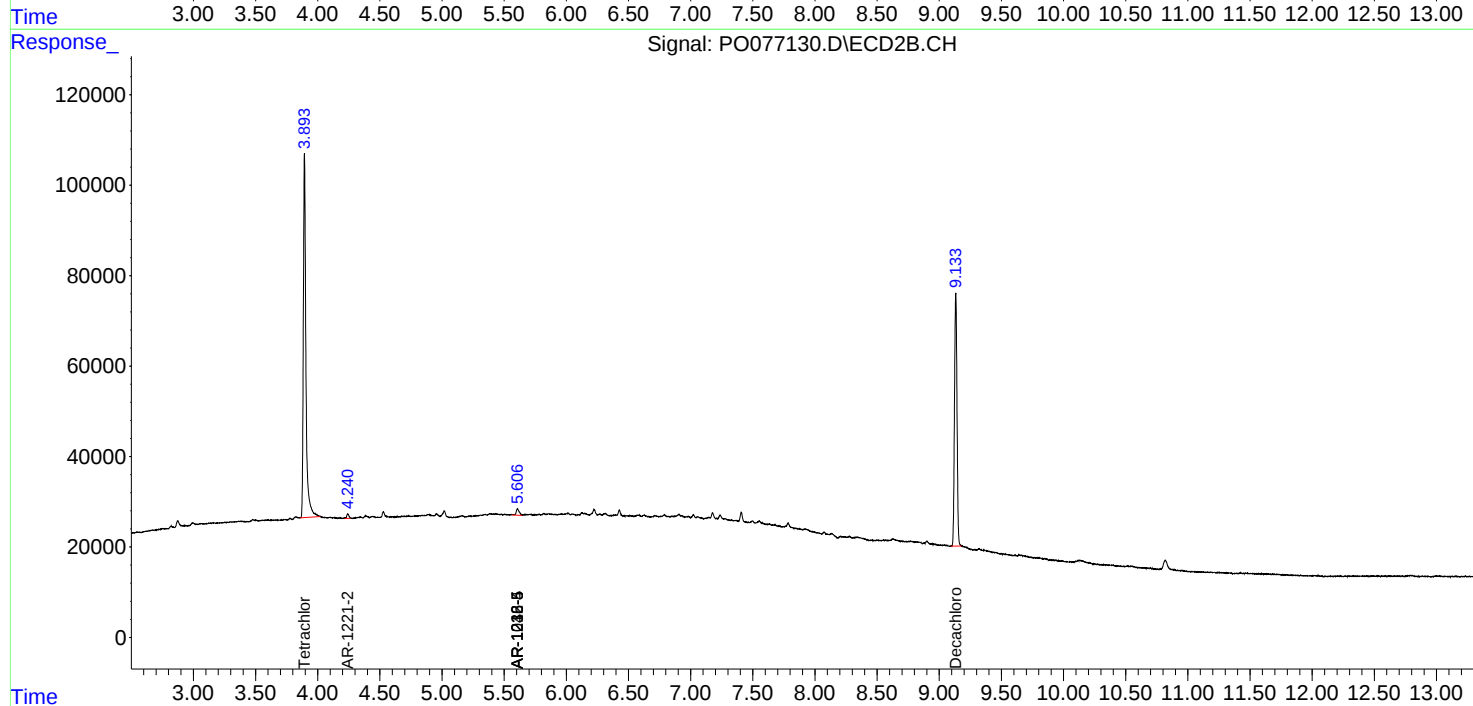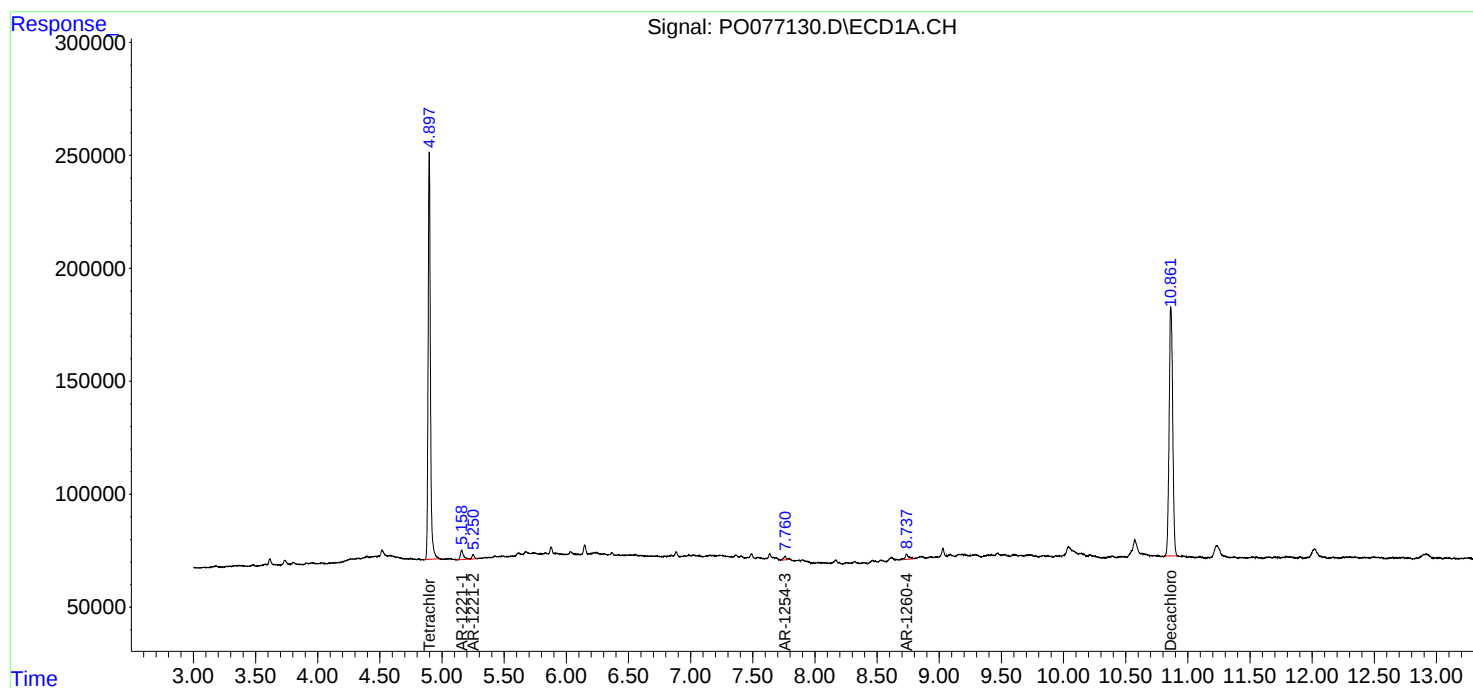


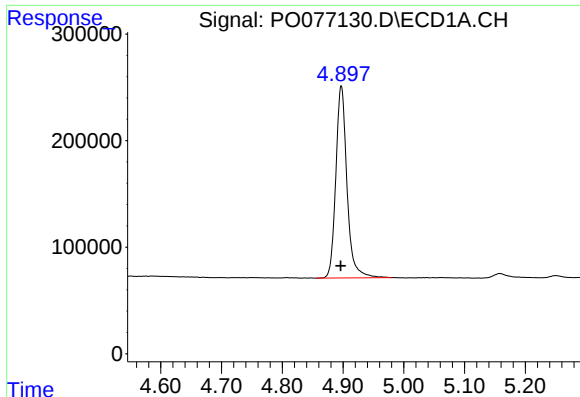

#1 Tetrachloro-m-xylene


R.T.: 4.897 min
Delta R.T.: 0.001 min
Response: 2294537
Conc: 21.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-2-S

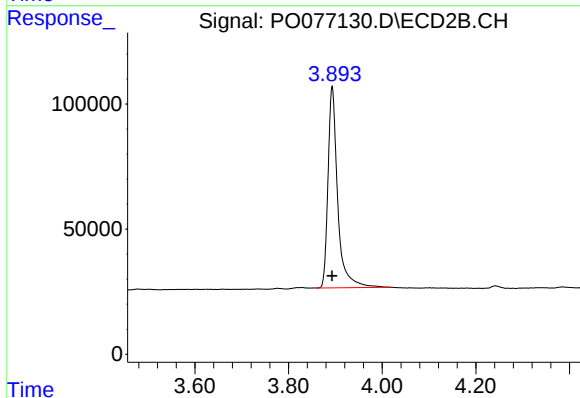


#1 Tetrachloro-m-xylene

R.T.: 3.893 min
Delta R.T.: 0.000 min
Response: 1157005
Conc: 21.99 ng/ml

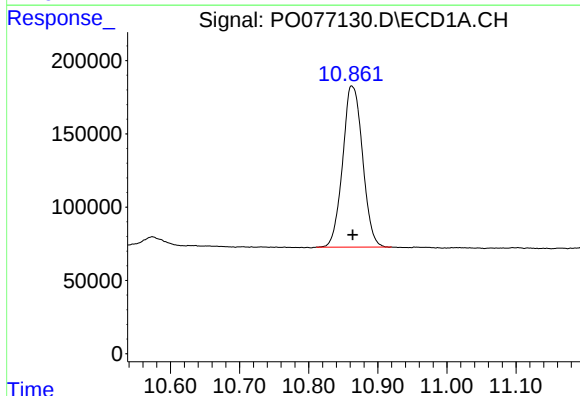


#2 Decachlorobiphenyl

R.T.: 10.862 min
Delta R.T.: -0.001 min
Response: 2201796
Conc: 21.21 ng/ml

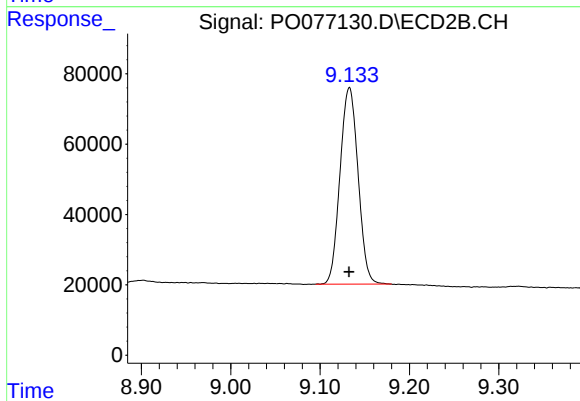

#2 Decachlorobiphenyl


R.T.: 9.133 min
Delta R.T.: 0.000 min
Response: 785279
Conc: 20.81 ng/ml

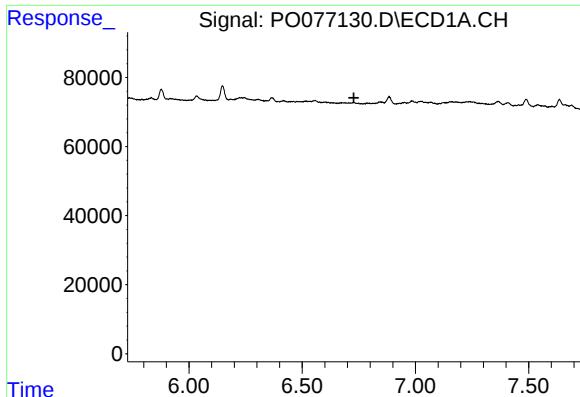

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 6.729 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-2-S

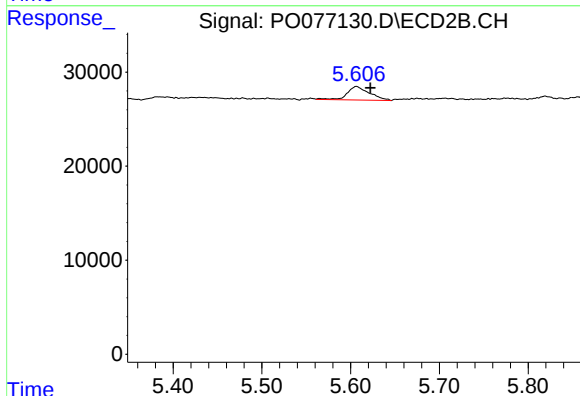


#7 AR-1016-5

R.T.: 5.606 min
Delta R.T.: -0.016 min
Response: 25111
Conc: 16.97 ng/ml

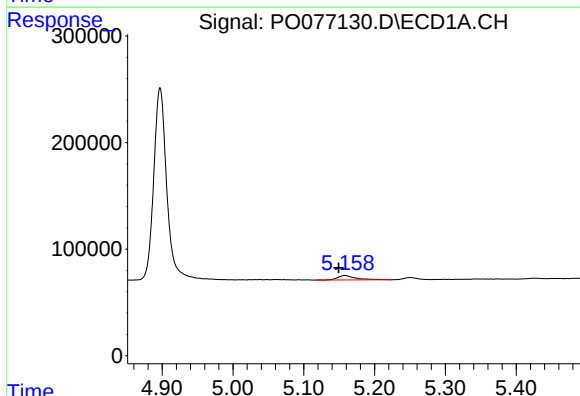


#8 AR-1221-1

R.T.: 5.158 min
Delta R.T.: 0.009 min
Response: 74045
Conc: 65.28 ng/ml

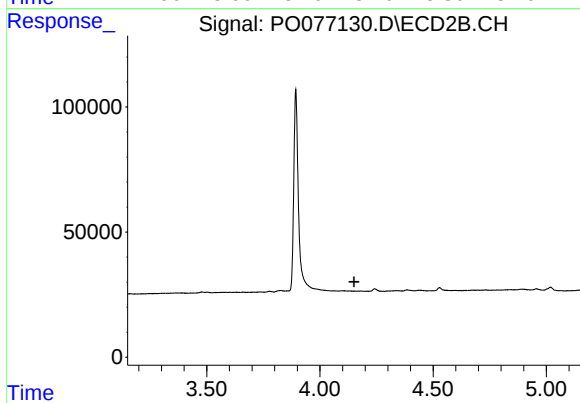

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T.: 4.150 min
Response: 0
Conc: N.D.

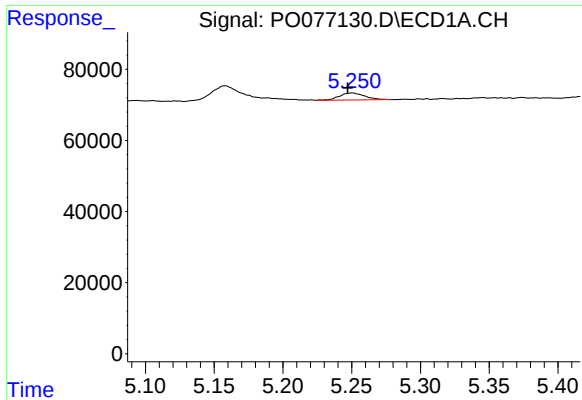

#9 AR-1221-2


R.T.: 5.250 min
Delta R.T.: 0.003 min
Response: 25072
Conc: 29.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-2-S

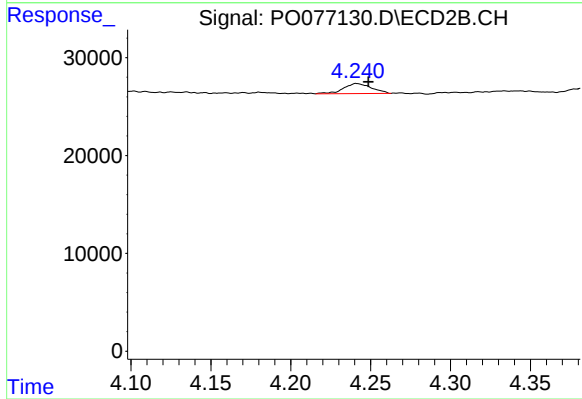


#9 AR-1221-2

R.T.: 4.241 min
Delta R.T.: -0.008 min
Response: 12517
Conc: 27.39 ng/ml

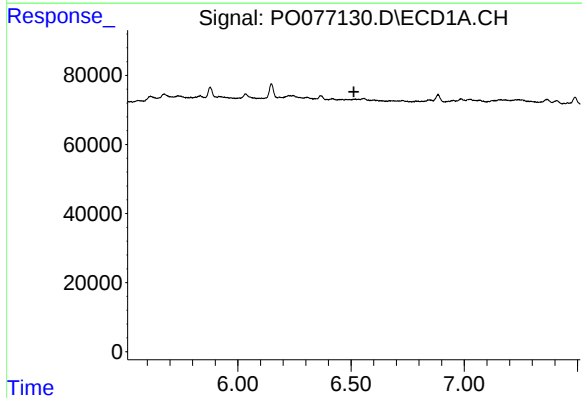


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 6.512 min
Response: 0
Conc: N.D.

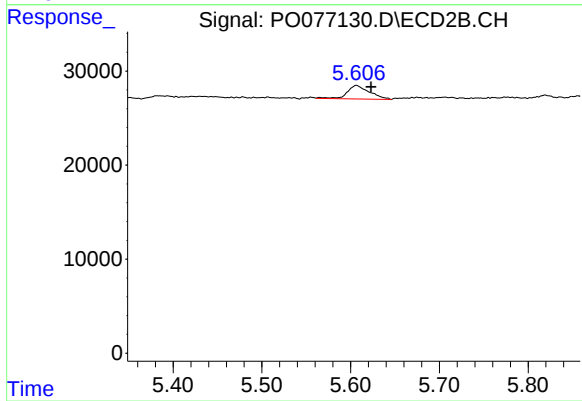

#15 AR-1232-5


R.T.: 5.606 min
Delta R.T.: -0.017 min
Response: 25111
Conc: 42.16 ng/ml

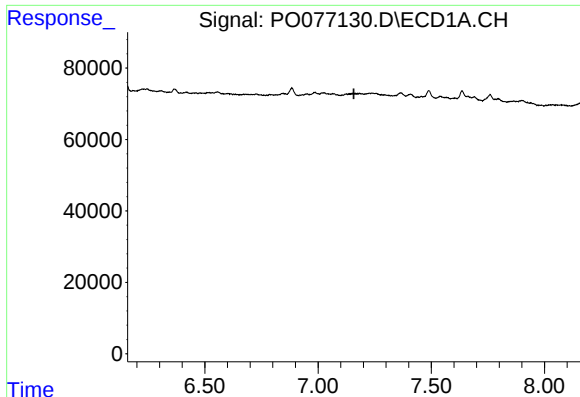

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 7.158 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-2-S

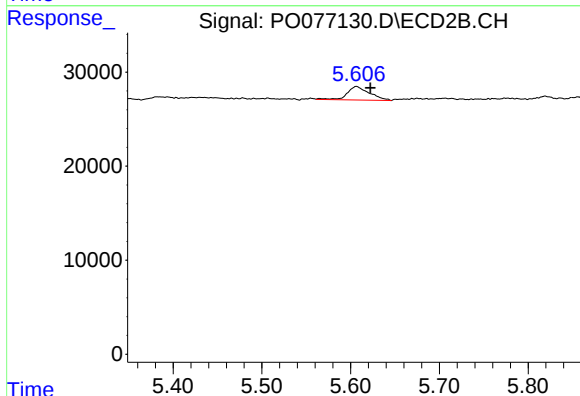


#24 AR-1248-4

R.T.: 5.606 min
Delta R.T.: -0.016 min
Response: 25111
Conc: 13.38 ng/ml

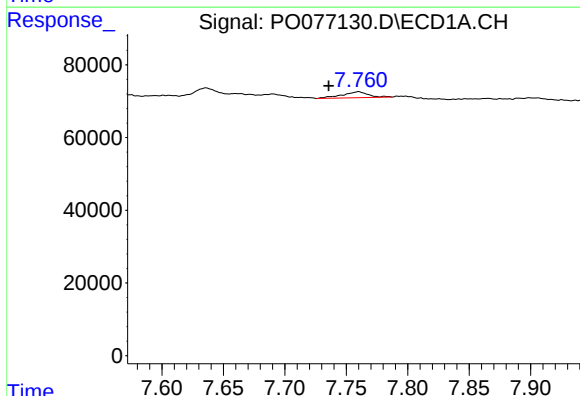


#28 AR-1254-3

R.T.: 7.760 min
Delta R.T.: 0.024 min
Response: 23463
Conc: 3.47 ng/ml

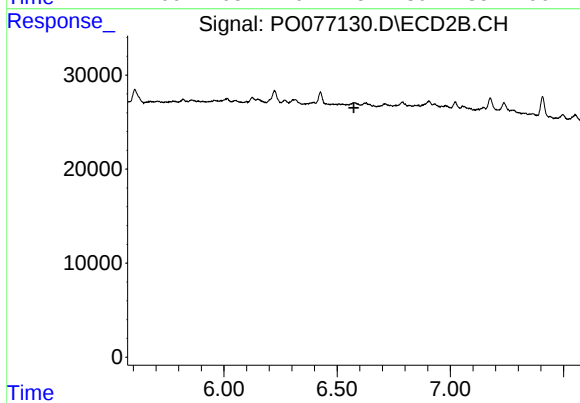

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T.: 6.574 min
Response: 0
Conc: N.D.

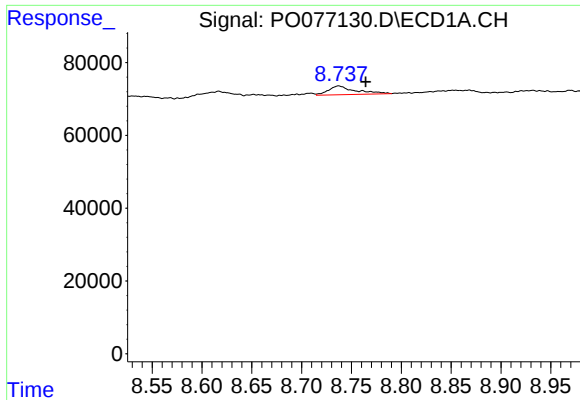

#34 AR-1260-4

R.T.: 8.737 min
Delta R.T.: -0.027 min
Response: 44663
Conc: 9.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-2-S

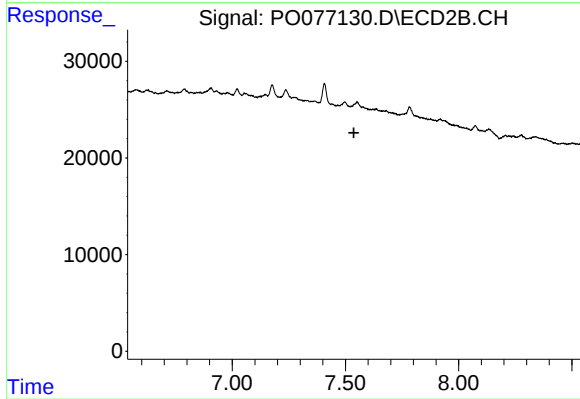

#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.537 min
Response: 0
Conc: N.D.