

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0042121\
 Data File : P0077110.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Apr 2021 12:05
 Operator : DD\AJ
 Sample : M2063-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP3-2-4

Manual Integrations
 APPROVED

Ankita
 4/22/2021 9:47:34 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 13:06:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 09:50:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.895	3.891	2470327	1263460	23.375	24.015
2)	SA Decachlor...	10.864	9.131	2236204	787681	21.539	20.875
Target Compounds							
26)	L6 AR-1254-1	7.127	5.996	205030	74800	49.859m	25.913 #
27)	L6 AR-1254-2	7.354	6.155	251595	74603	38.873m	28.896 #
28)	L6 AR-1254-3	7.739	6.572	143902	97863	21.266	25.013m
29)	L6 AR-1254-4	8.034	6.813	117127	42539	23.817	18.723m
30)	L6 AR-1254-5	8.463	7.233	231281	175330	41.546	48.356m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO042121\
Data File : PO077110.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Apr 2021 12:05
Operator : DD\AJ
Sample : M2063-11
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
TP3-2-4


Manual Integrations
APPROVED

Ankita
4/22/2021 9:47:34 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 13:06:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 09:50:22 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

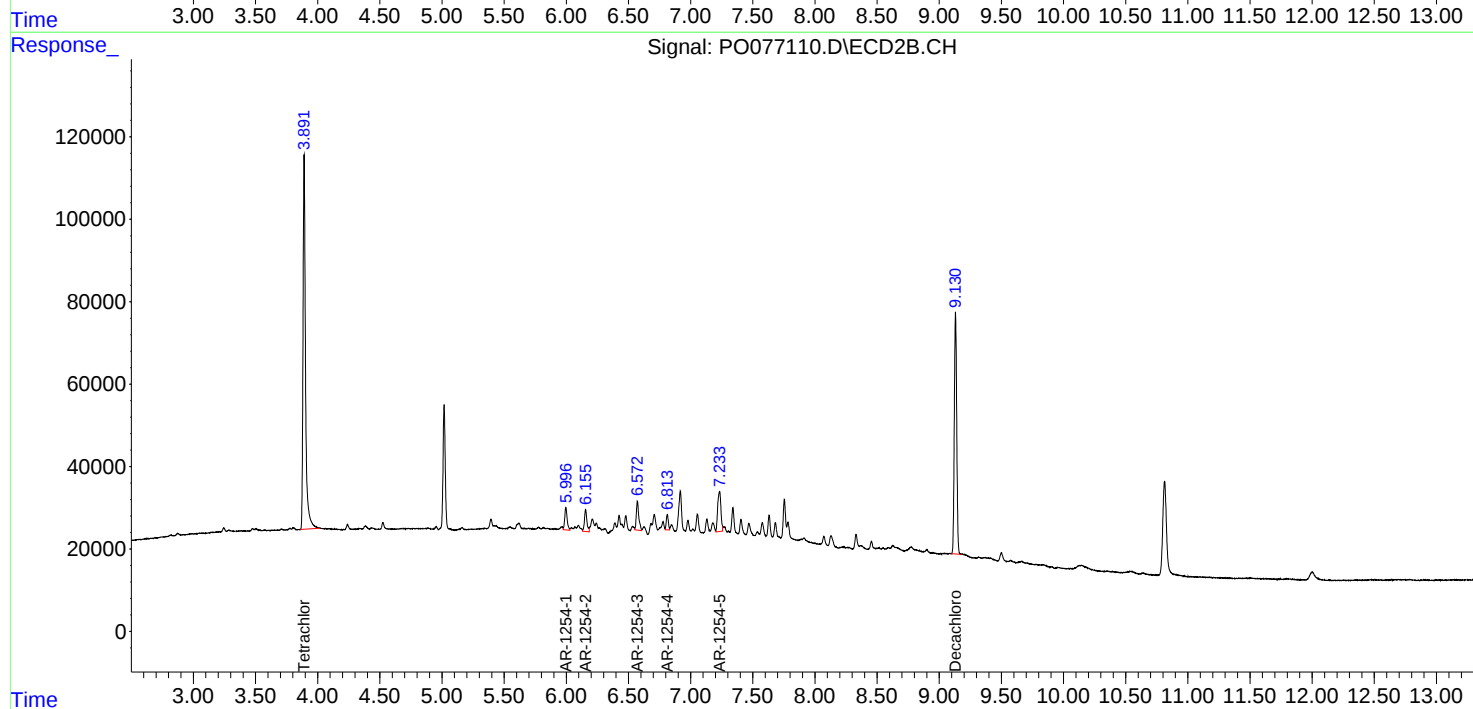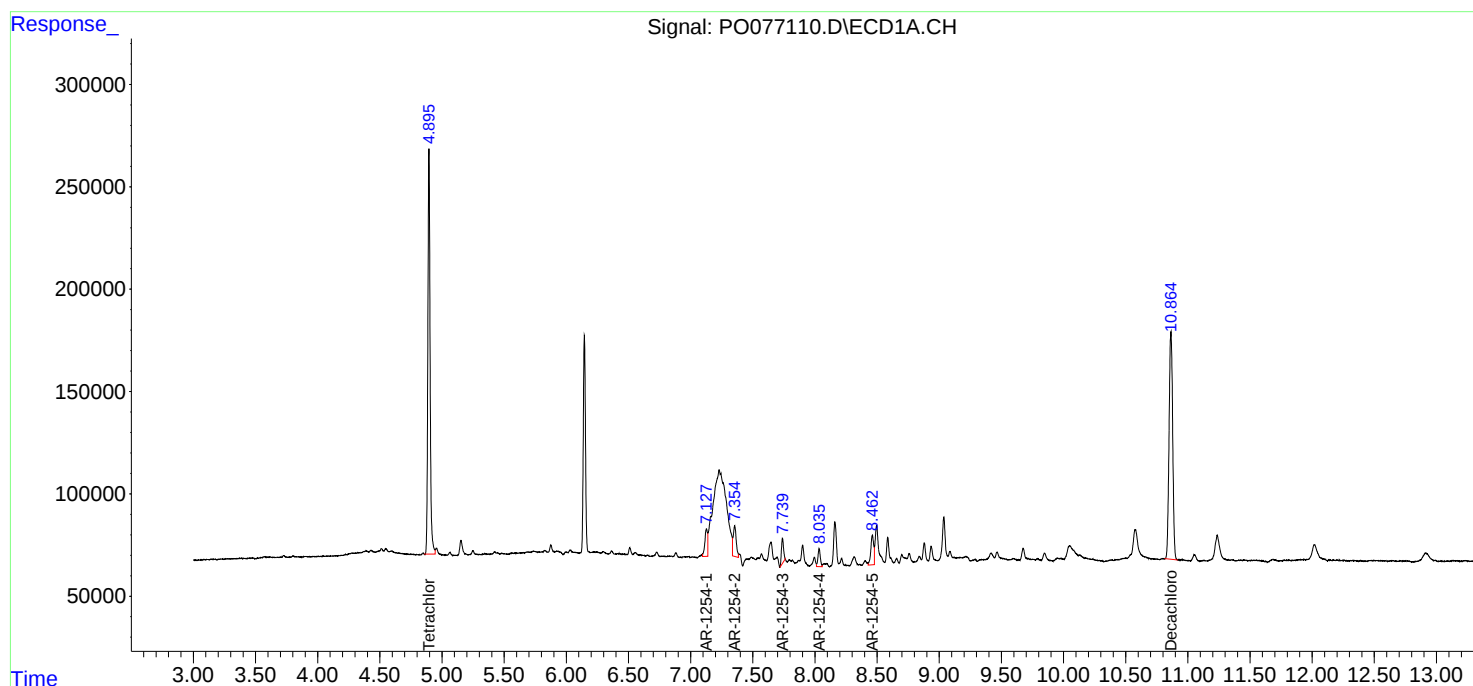

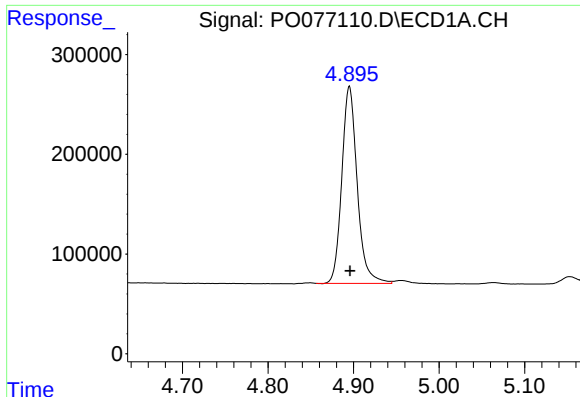


#1 Tetrachloro-m-xylene

R.T.: 4.895 min
Delta R.T.: 0.000 min
Response: 2470327
Conc: 23.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP3-2-4


Manual Integrations
APPROVED

Ankita
4/22/2021 9:47:34 AM

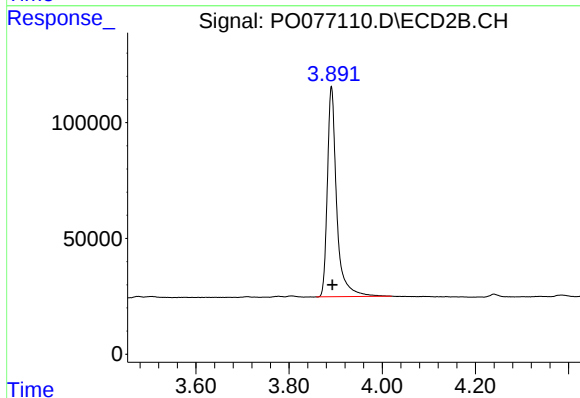


#1 Tetrachloro-m-xylene

R.T.: 3.891 min
Delta R.T.: -0.002 min
Response: 1263460
Conc: 24.01 ng/ml

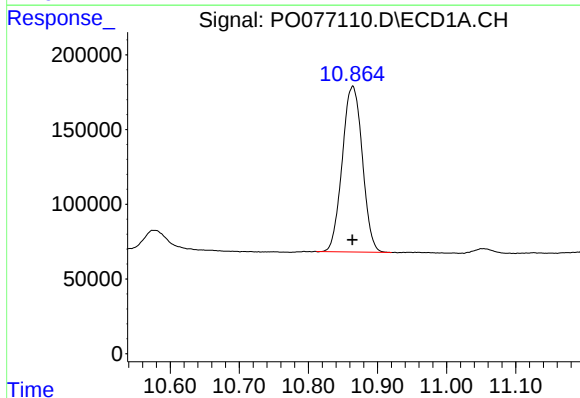


#2 Decachlorobiphenyl

R.T.: 10.864 min
Delta R.T.: 0.000 min
Response: 2236204
Conc: 21.54 ng/ml

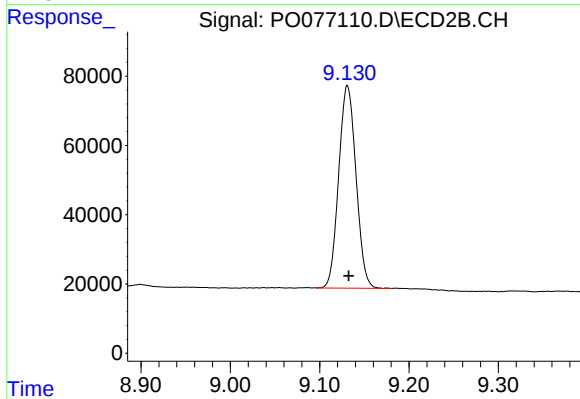

#2 Decachlorobiphenyl

R.T.: 9.131 min
Delta R.T.: -0.001 min
Response: 787681
Conc: 20.87 ng/ml

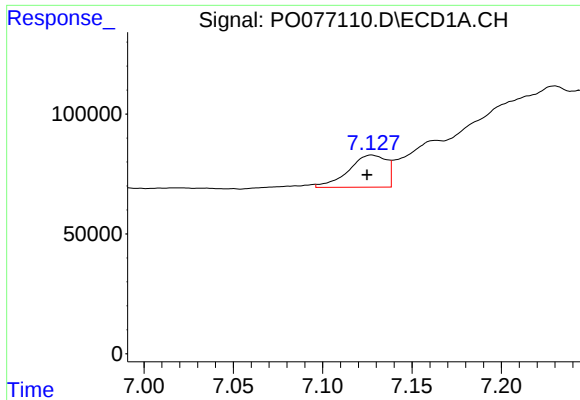


#26 AR-1254-1

R.T.: 7.127 min
Delta R.T.: 0.002 min
Response: 205030
Conc: 49.86 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP3-2-4


Manual Integrations
APPROVED

Ankita
4/22/2021 9:47:34 AM

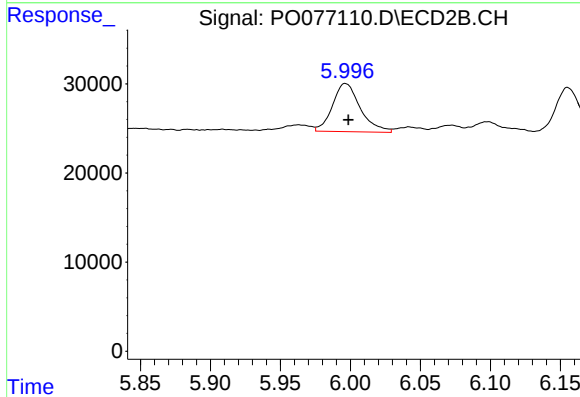


#26 AR-1254-1

R.T.: 5.996 min
Delta R.T.: -0.002 min
Response: 74800
Conc: 25.91 ng/ml

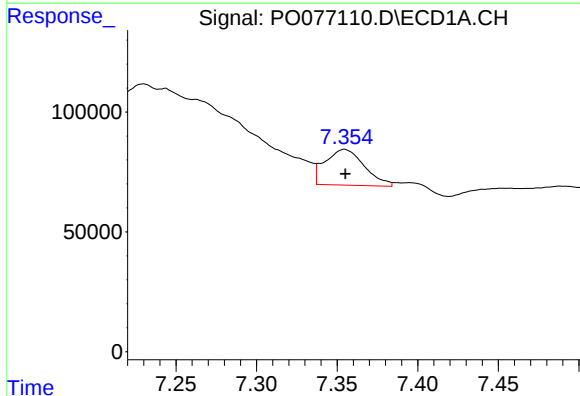


#27 AR-1254-2

R.T.: 7.354 min
Delta R.T.: 0.000 min
Response: 251595
Conc: 38.87 ng/ml m

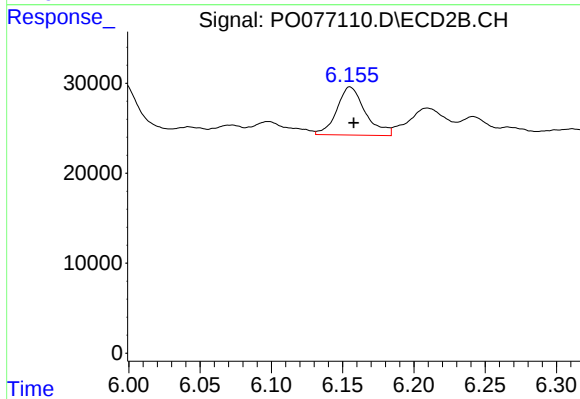

#27 AR-1254-2

R.T.: 6.155 min
Delta R.T.: -0.002 min
Response: 74603
Conc: 28.90 ng/ml

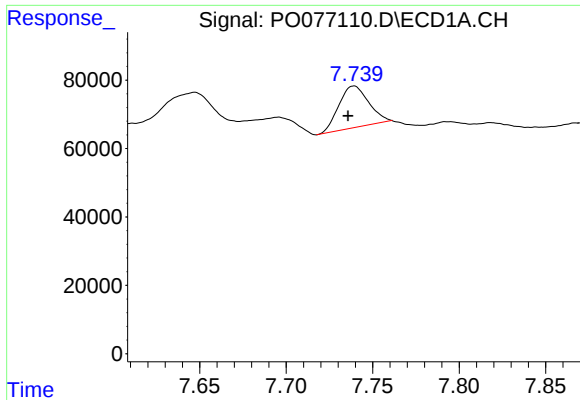


#28 AR-1254-3

R.T.: 7.739 min
Delta R.T.: 0.003 min
Response: 143902
Conc: 21.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP3-2-4


Manual Integrations
APPROVED

Ankita
4/22/2021 9:47:34 AM

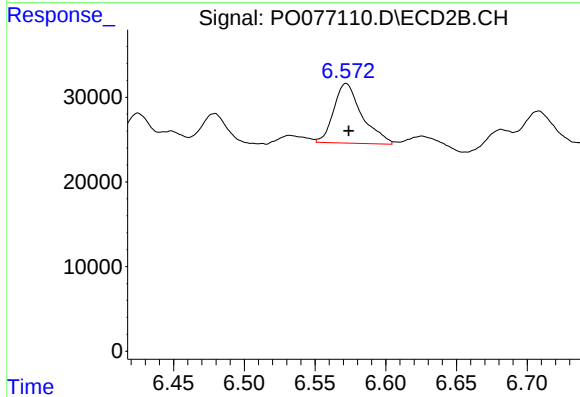


#28 AR-1254-3

R.T.: 6.572 min
Delta R.T.: -0.002 min
Response: 97863
Conc: 25.01 ng/ml m

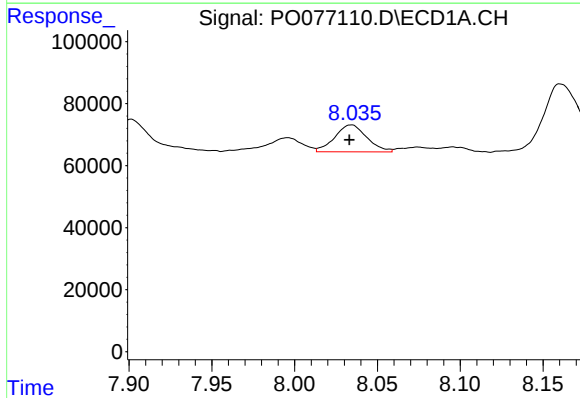


#29 AR-1254-4

R.T.: 8.034 min
Delta R.T.: 0.001 min
Response: 117127
Conc: 23.82 ng/ml

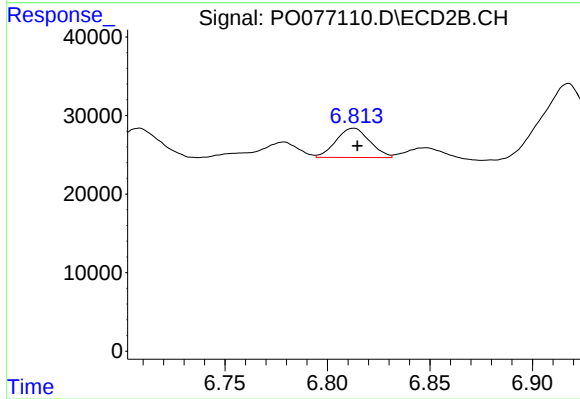

#29 AR-1254-4

R.T.: 6.813 min
Delta R.T.: -0.002 min
Response: 42539
Conc: 18.72 ng/ml m

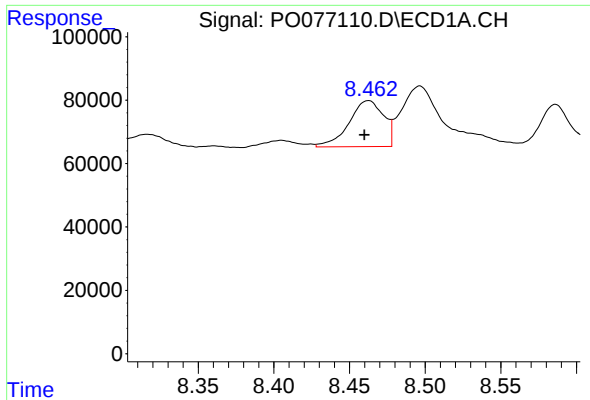


#30 AR-1254-5

R.T.: 8.463 min
Delta R.T.: 0.003 min
Response: 231281
Conc: 41.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP3-2-4

Manual Integrations
APPROVED

Ankita
4/22/2021 9:47:34 AM

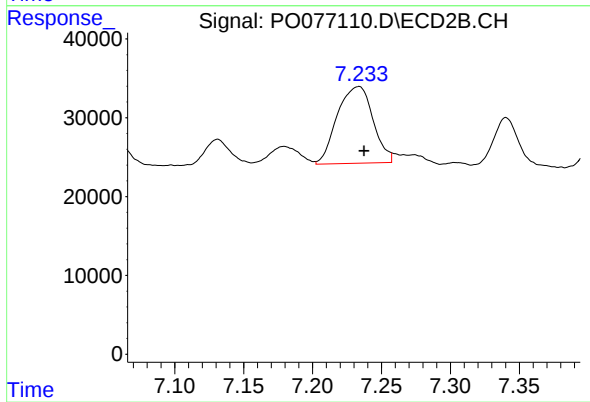

#30 AR-1254-5

R.T.: 7.233 min
Delta R.T.: -0.004 min
Response: 175330
Conc: 48.36 ng/ml m