

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042121\
 Data File : P0077121.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Apr 2021 15:16
 Operator : DD\AJ
 Sample : M2069-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MH20A-BNM-1-D-WATER-BAG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 16:39:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 09:50:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.896	3.892	2419350	1215663	22.893	23.106
2) SA Decachlor...	10.863	9.132	1732311	619559	16.685	16.419

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042121\
Data File : P0077121.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Apr 2021 15:16
Operator : DD\AJ
Sample : M2069-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MH20A-BNM-1-D-WATER-BAG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 16:39:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 09:50:22 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

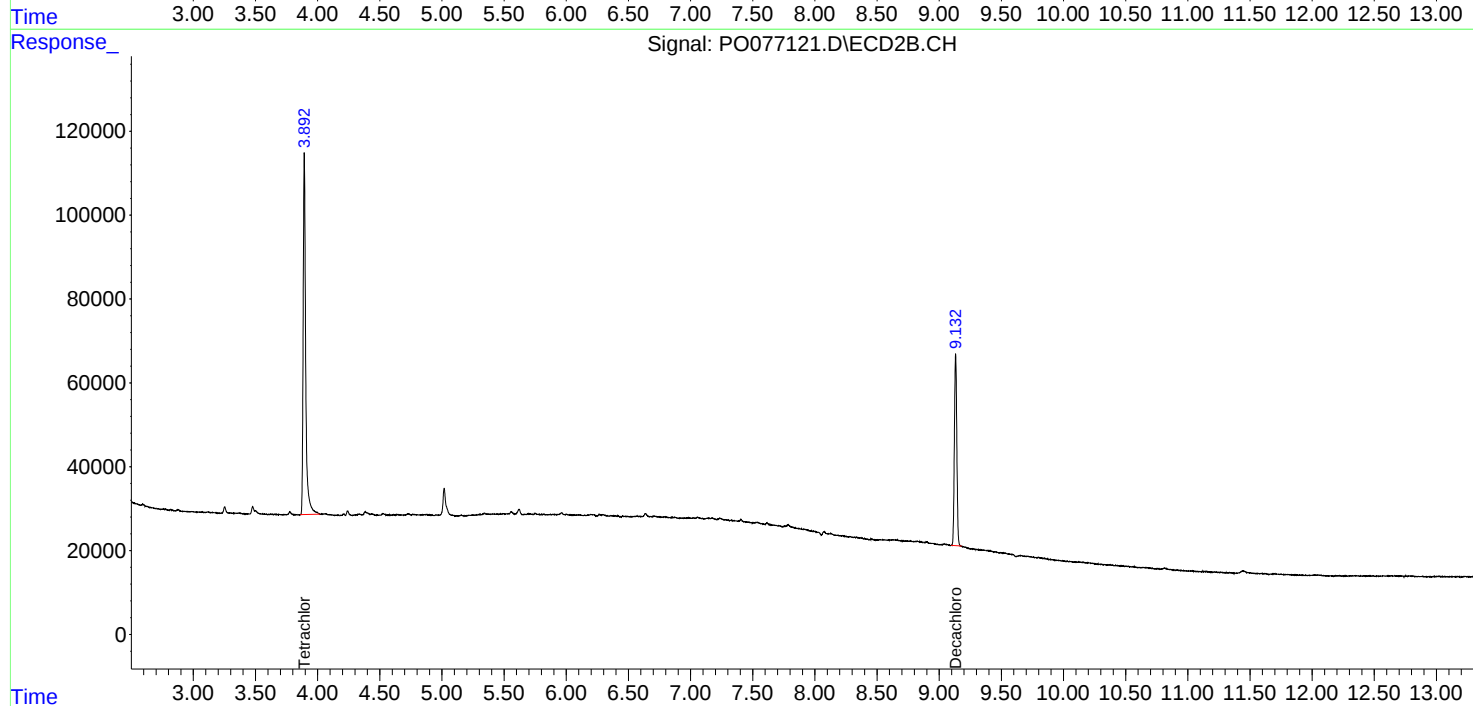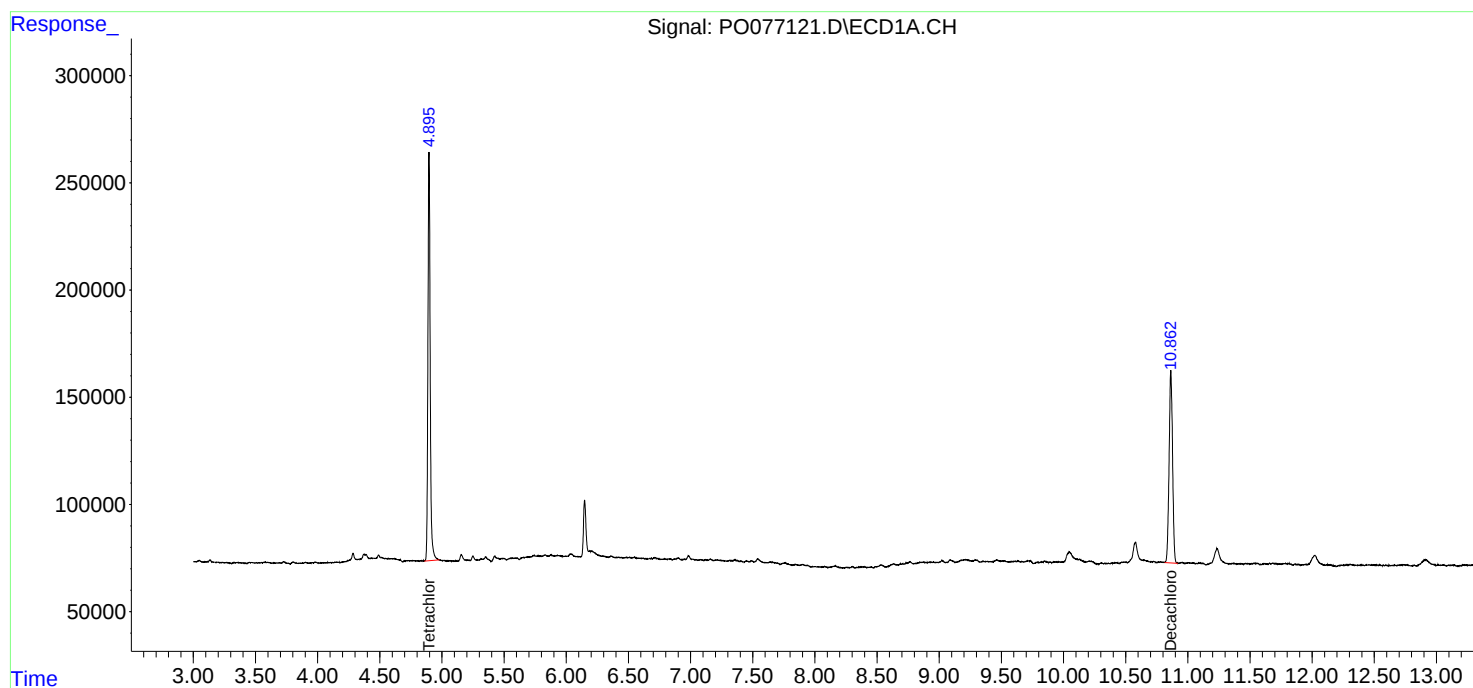


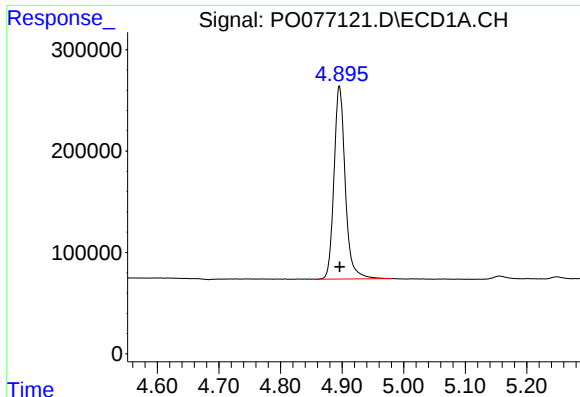

#1 Tetrachloro-m-xylene


R.T.: 4.896 min
Delta R.T.: 0.000 min
Response: 2419350
Conc: 22.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
MH20A-BNM-1-D-WATER-BAG

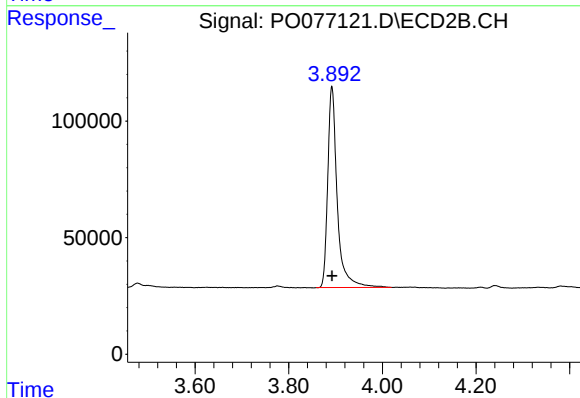


#1 Tetrachloro-m-xylene

R.T.: 3.892 min
Delta R.T.: 0.000 min
Response: 1215663
Conc: 23.11 ng/ml

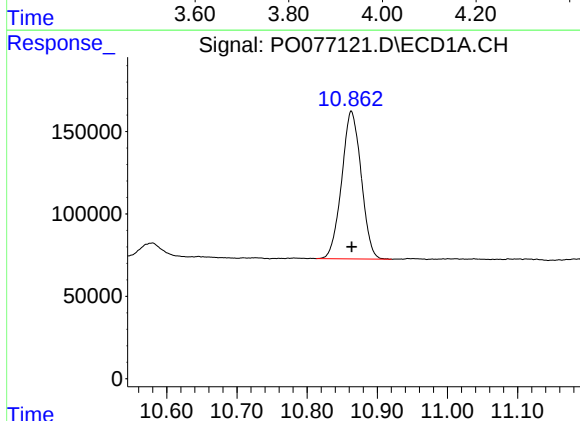

#2 Decachlorobiphenyl

R.T.: 10.863 min
Delta R.T.: 0.000 min
Response: 1732311
Conc: 16.69 ng/ml

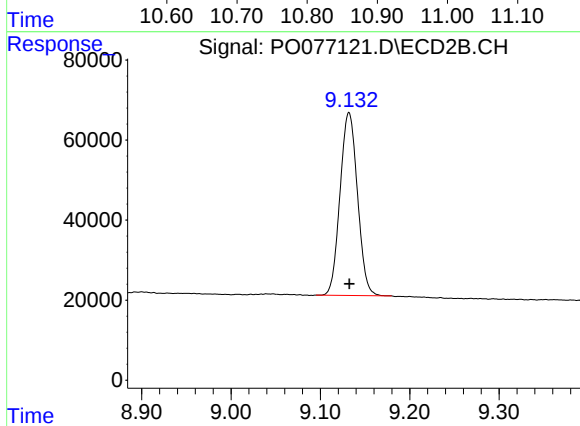

#2 Decachlorobiphenyl

R.T.: 9.132 min
Delta R.T.: 0.000 min
Response: 619559
Conc: 16.42 ng/ml