

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042123\
 Data File : P0094526.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2023 01:00
 Operator : YP/AJ
 Sample : 02430-02
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AUD-40228

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/24/2023
 Supervised By :Ankita Jodhani 04/24/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 24 04:30:39 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0041923.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 20 05:15:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.415	3.617	85368608	32267519	26.536	24.981m
2) SA Decachlor...	10.253	8.632	56471614	23439944	26.420	23.534

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042123\
Data File : P0094526.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2023 01:00
Operator : YP/AJ
Sample : 02430-02
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AUD-40228


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/24/2023
Supervised By :Ankita Jodhani 04/24/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 24 04:30:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0041923.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 20 05:15:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

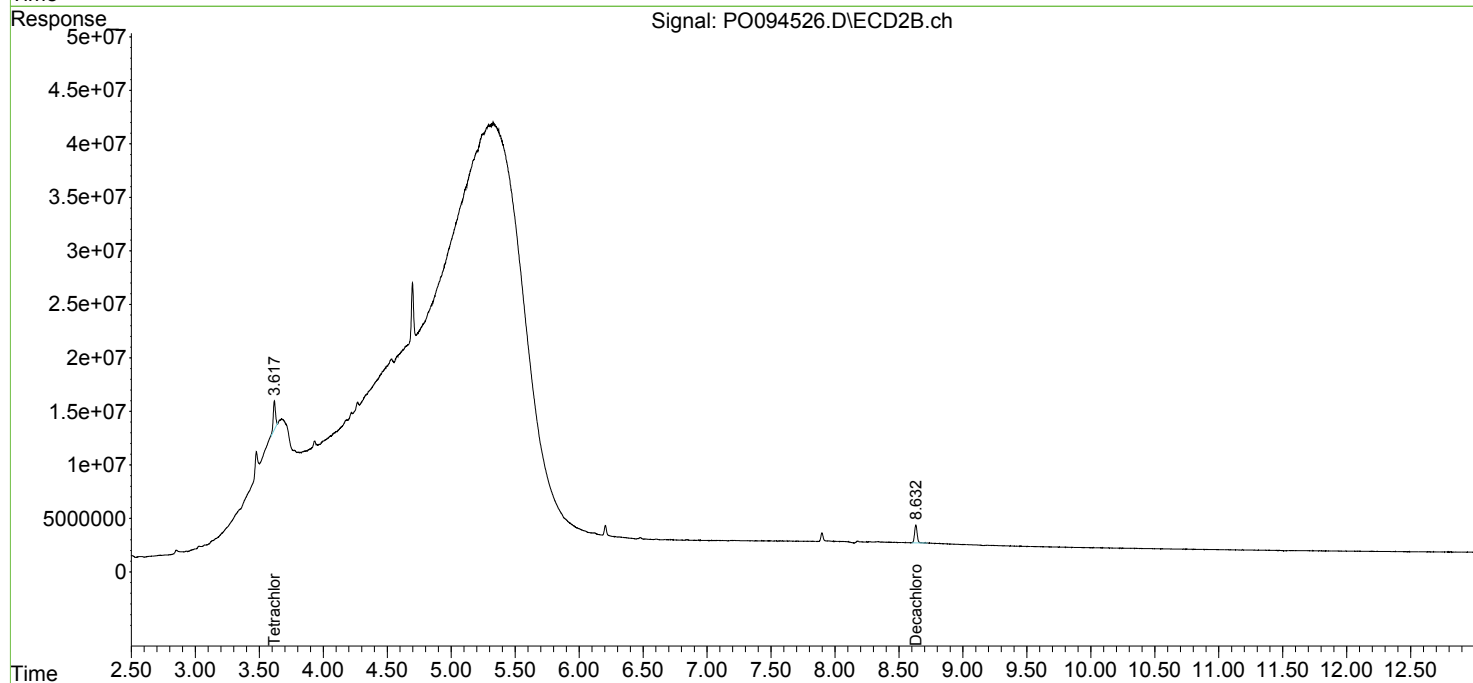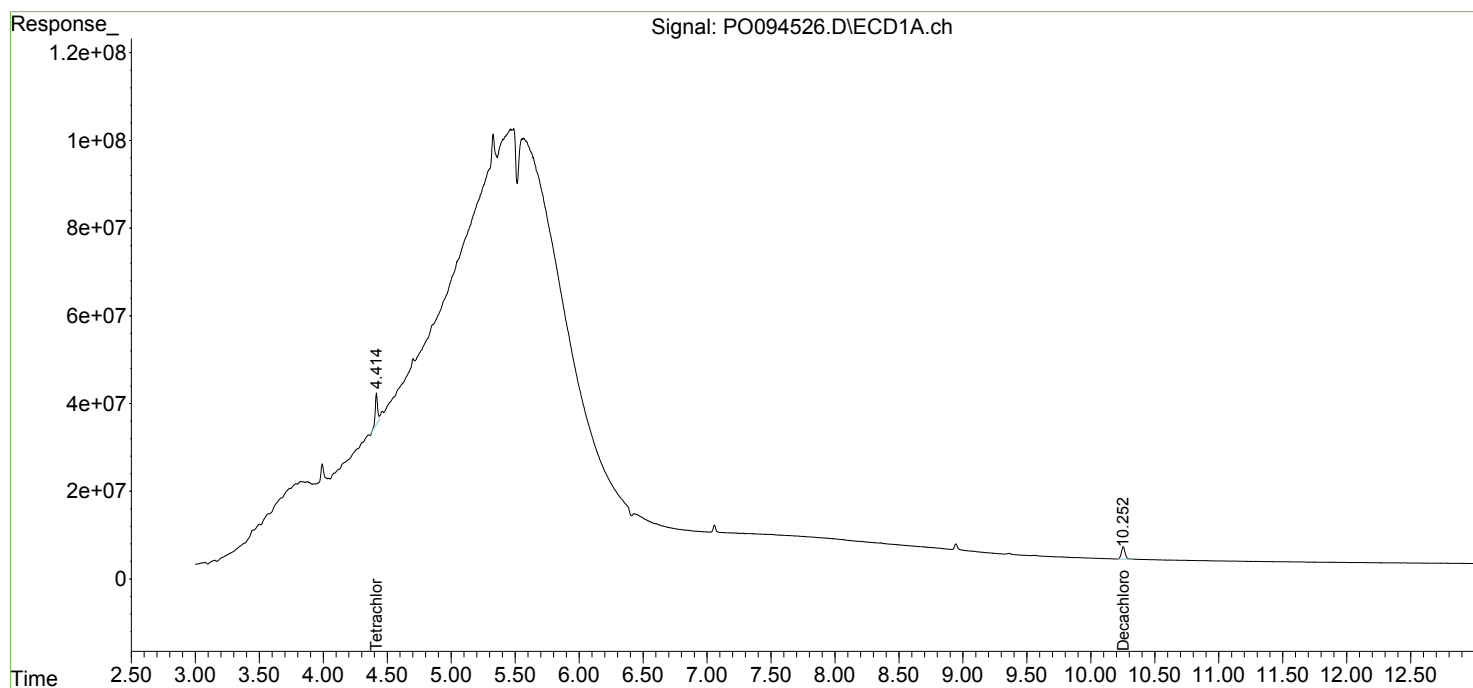

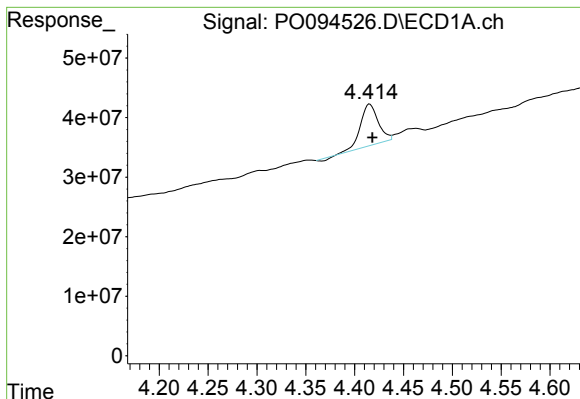


#1 Tetrachloro-m-xylene

R.T.: 4.415 min
Delta R.T.: -0.003 min
Response: 85368608
Conc: 26.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
AUD-40228


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/24/2023
Supervised By :Ankita Jodhani 04/24/2023

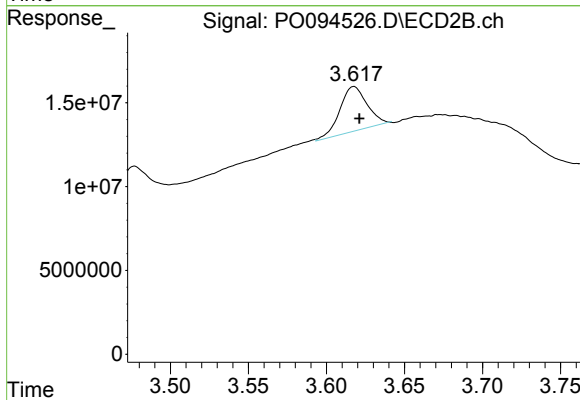


#1 Tetrachloro-m-xylene

R.T.: 3.617 min
Delta R.T.: -0.004 min
Response: 32267519
Conc: 24.98 ng/ml m

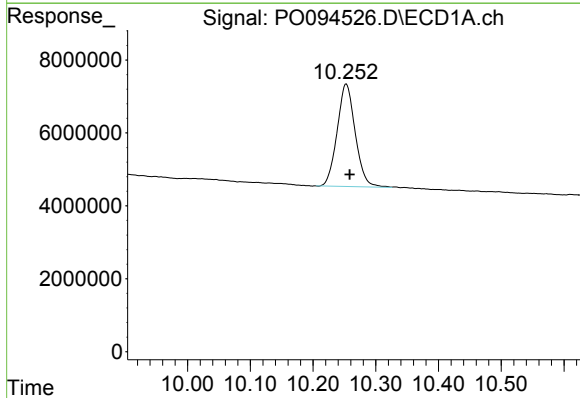

#2 Decachlorobiphenyl

R.T.: 10.253 min
Delta R.T.: -0.006 min
Response: 56471614
Conc: 26.42 ng/ml

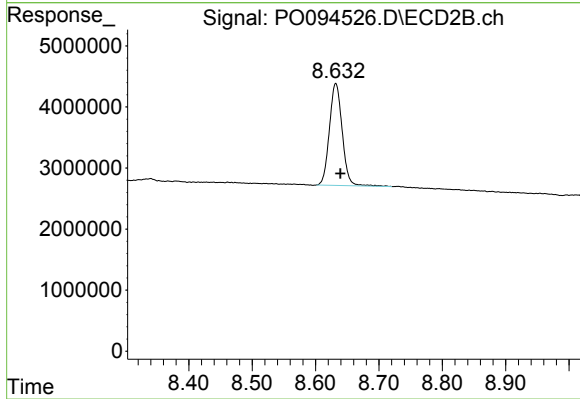

#2 Decachlorobiphenyl

R.T.: 8.632 min
Delta R.T.: -0.007 min
Response: 23439944
Conc: 23.53 ng/ml