

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042125\
Data File : P0110585.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2025 01:42
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 03:35:21 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0041025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 11 02:12:41 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	3.685	3.685	165.0E6	88594400	18.860	17.755
2) SA Decachlor...	8.730	8.683	147.3E6	37102138	18.659	19.274

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO042125\
Data File : PO110585.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2025 01:42
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 03:35:21 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO041025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 11 02:12:41 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

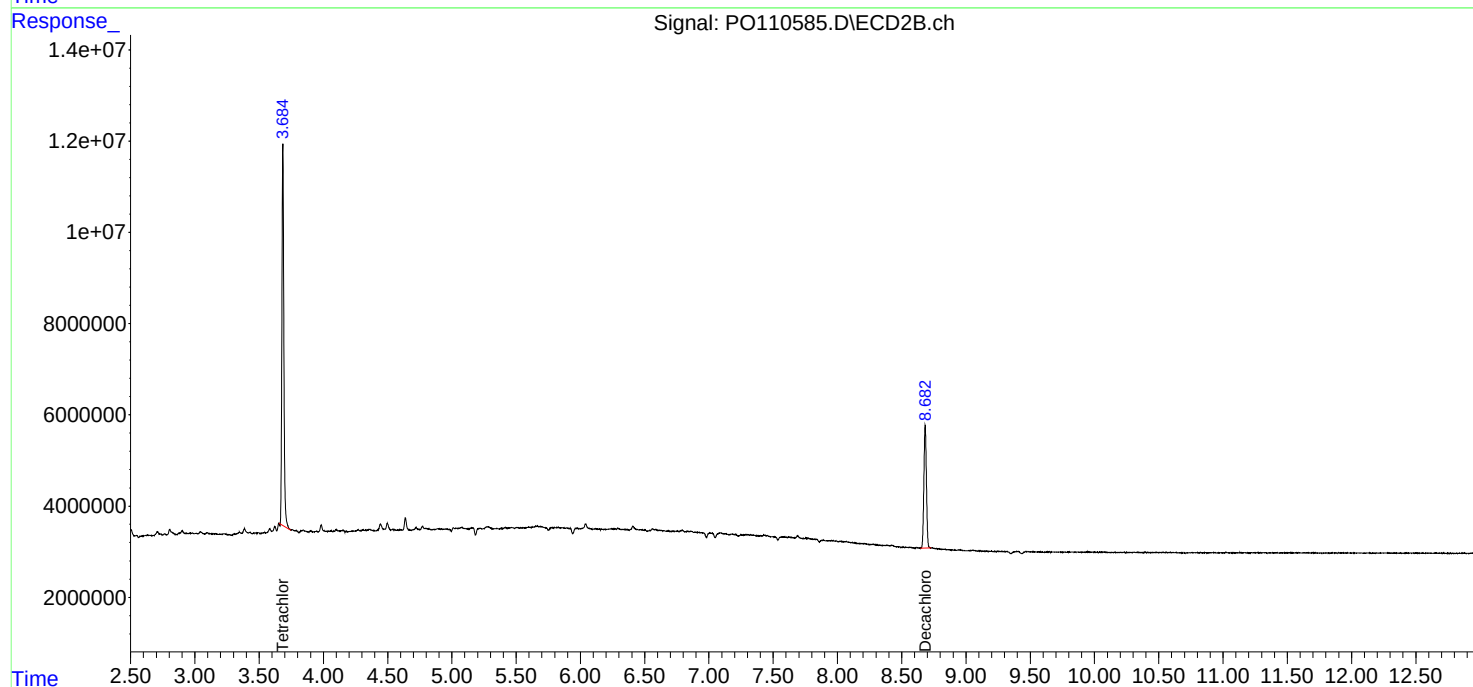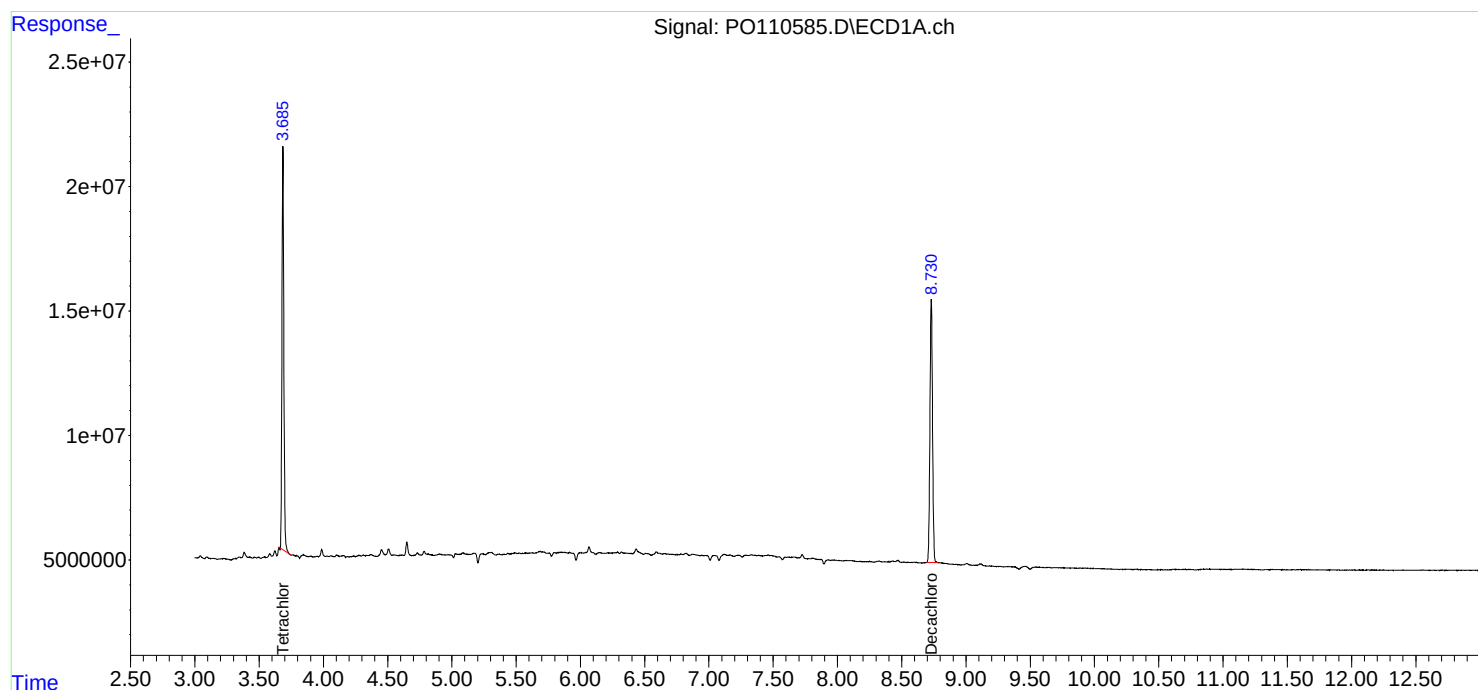


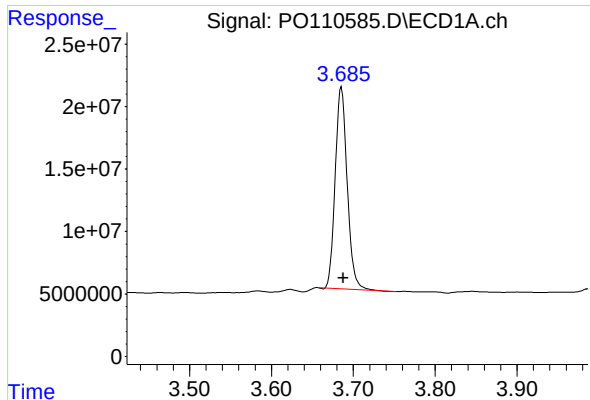

#1 Tetrachloro-m-xylene


R.T.: 3.685 min
Delta R.T.: -0.003 min
Response: 165003063
Conc: 18.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

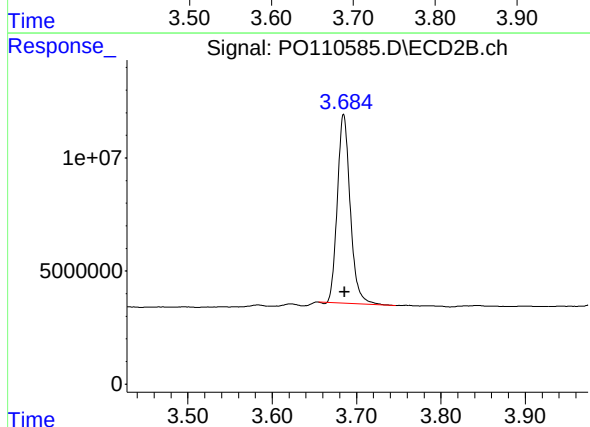


#1 Tetrachloro-m-xylene

R.T.: 3.685 min
Delta R.T.: -0.001 min
Response: 88594400
Conc: 17.76 ng/ml

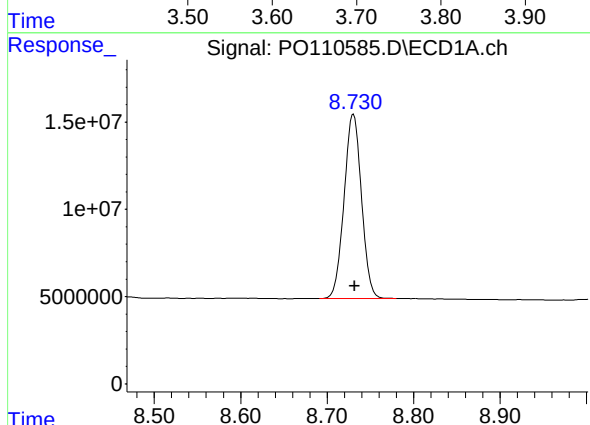

#2 Decachlorobiphenyl

R.T.: 8.730 min
Delta R.T.: -0.001 min
Response: 147309245
Conc: 18.66 ng/ml

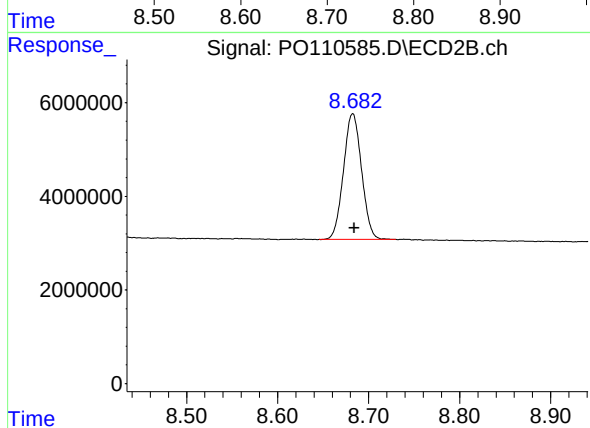

#2 Decachlorobiphenyl

R.T.: 8.683 min
Delta R.T.: -0.002 min
Response: 37102138
Conc: 19.27 ng/ml