

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042221\
 Data File : P0077130.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Apr 2021 17:51
 Operator : DD\AJ
 Sample : M2075-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-2-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 01:57:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 09:50:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.897	3.893	2294537	1157005	21.712	21.991
2) SA Decachlor...	10.862	9.133	2201796	785279	21.207	20.811

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042221\
Data File : P0077130.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Apr 2021 17:51
Operator : DD\AJ
Sample : M2075-07
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-2-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 01:57:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 09:50:22 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

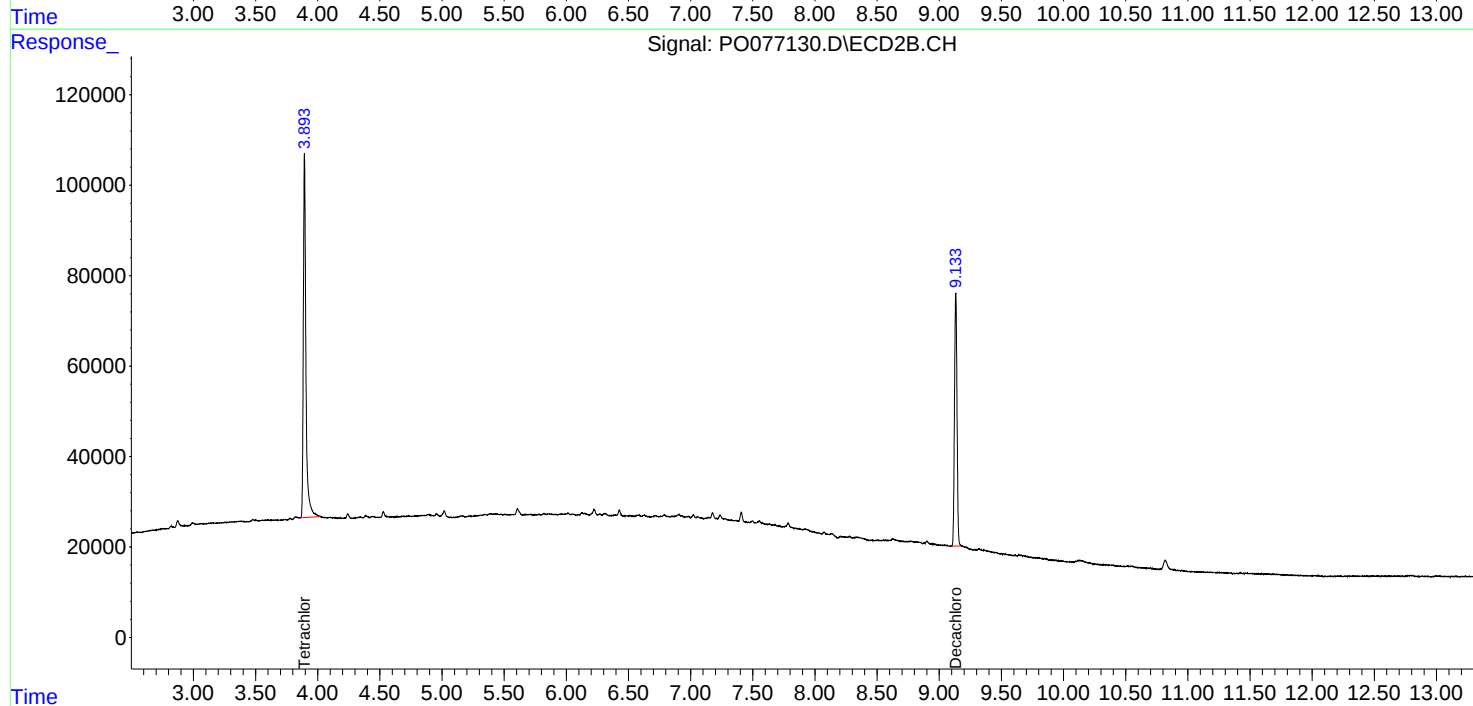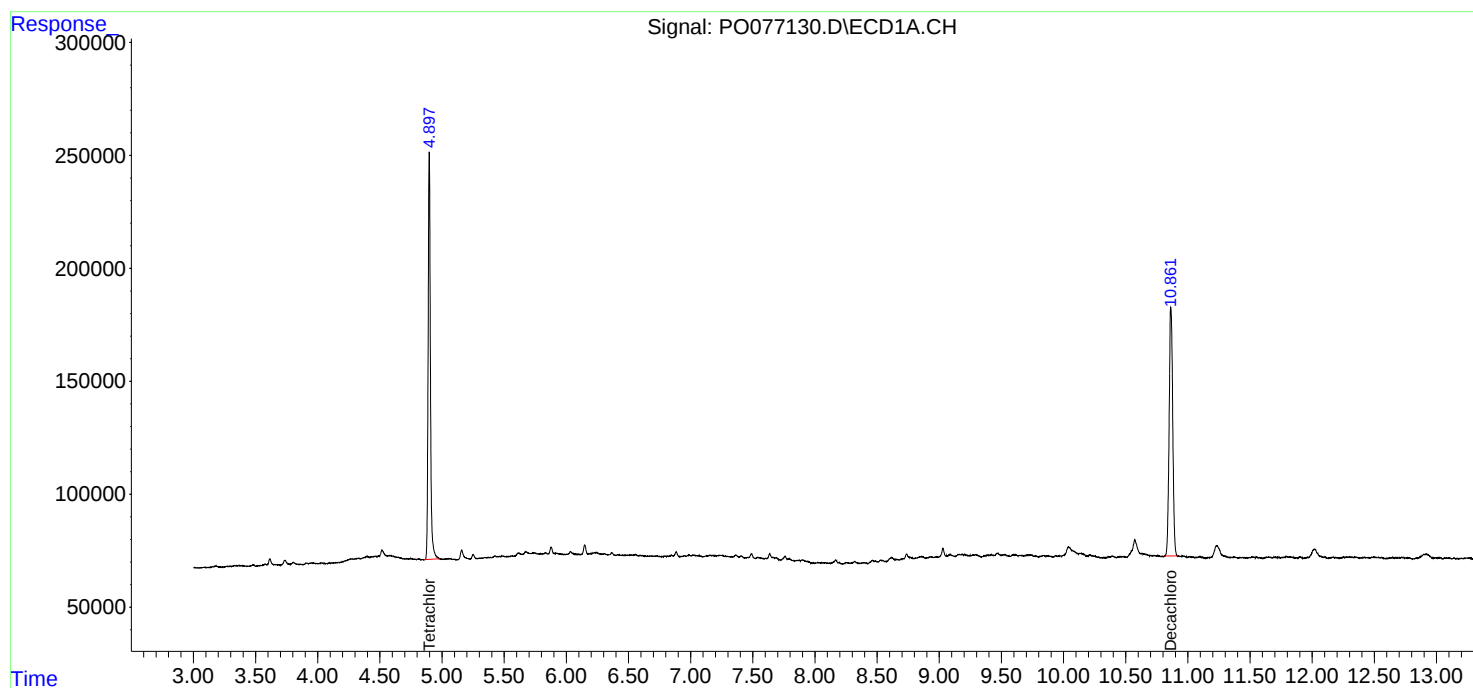


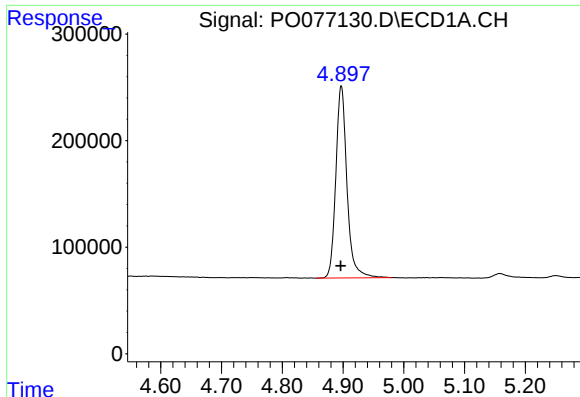

#1 Tetrachloro-m-xylene


R.T.: 4.897 min
Delta R.T.: 0.001 min
Response: 2294537
Conc: 21.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-2-S

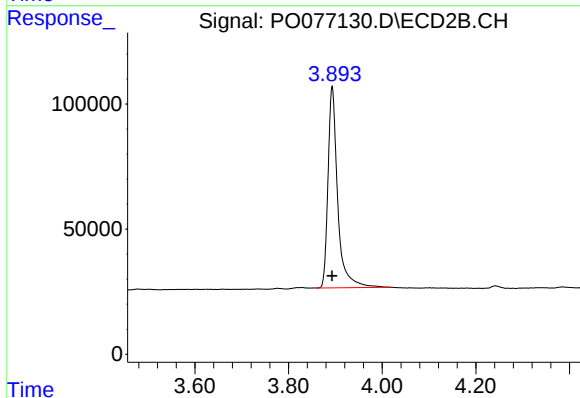


#1 Tetrachloro-m-xylene

R.T.: 3.893 min
Delta R.T.: 0.000 min
Response: 1157005
Conc: 21.99 ng/ml

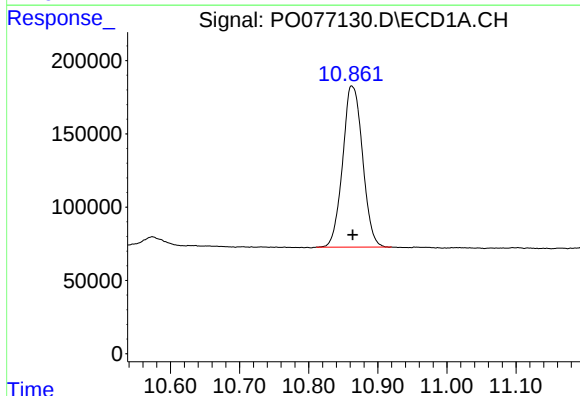

#2 Decachlorobiphenyl

R.T.: 10.862 min
Delta R.T.: -0.001 min
Response: 2201796
Conc: 21.21 ng/ml

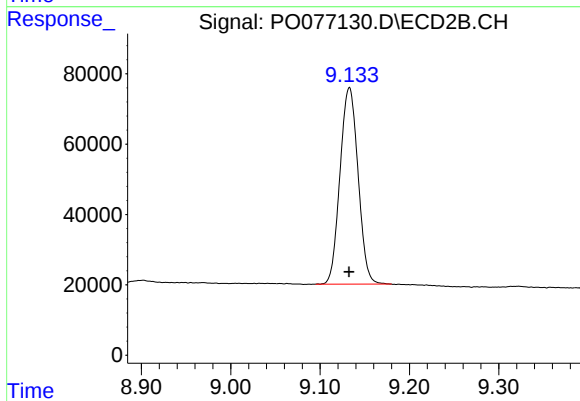

#2 Decachlorobiphenyl

R.T.: 9.133 min
Delta R.T.: 0.000 min
Response: 785279
Conc: 20.81 ng/ml