

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042221\
 Data File : P0077143.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Apr 2021 21:34
 Operator : DD\AJ
 Sample : M2075-28
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-8-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 02:04:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 09:50:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.896	3.890	2245441	1113071	21.247	21.156
2) SA Decachlor...	10.861	9.131	2109110	742803	20.314	19.686

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042221\
Data File : P0077143.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Apr 2021 21:34
Operator : DD\AJ
Sample : M2075-28
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-8-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 02:04:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 09:50:22 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

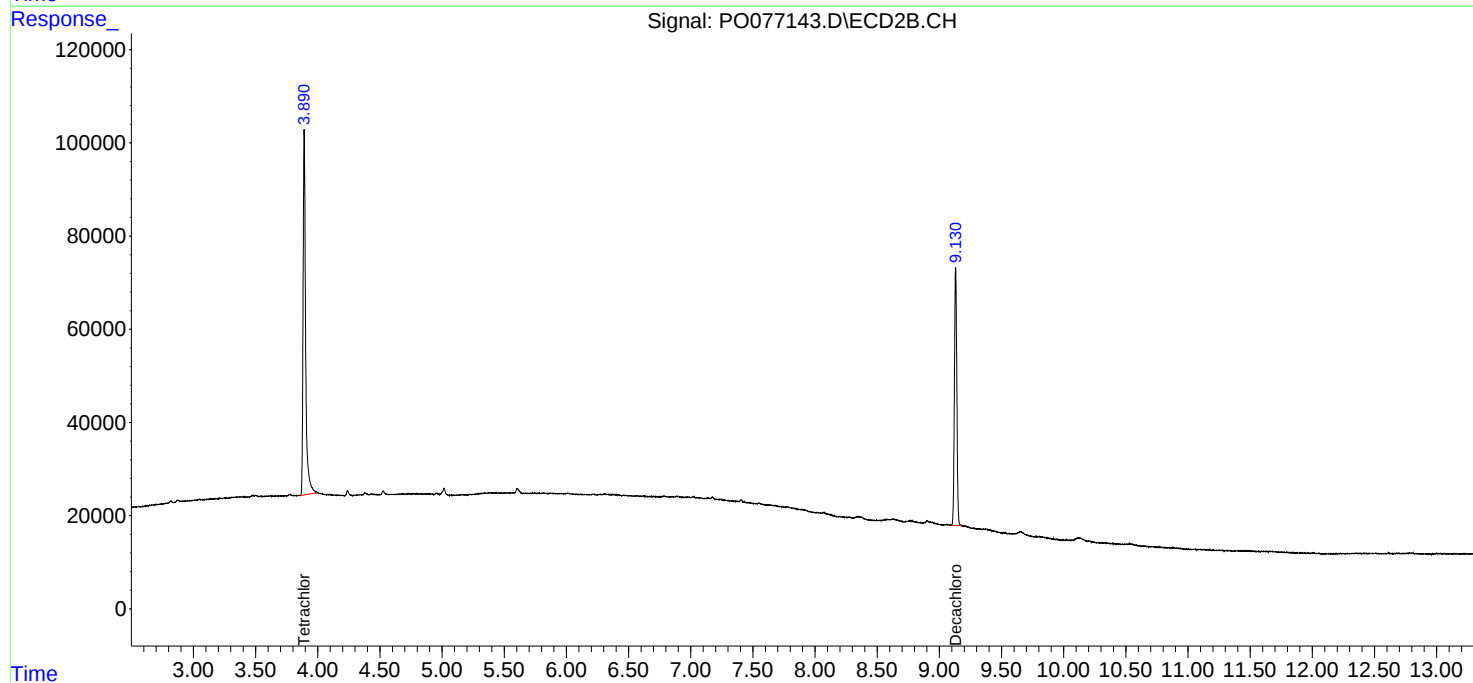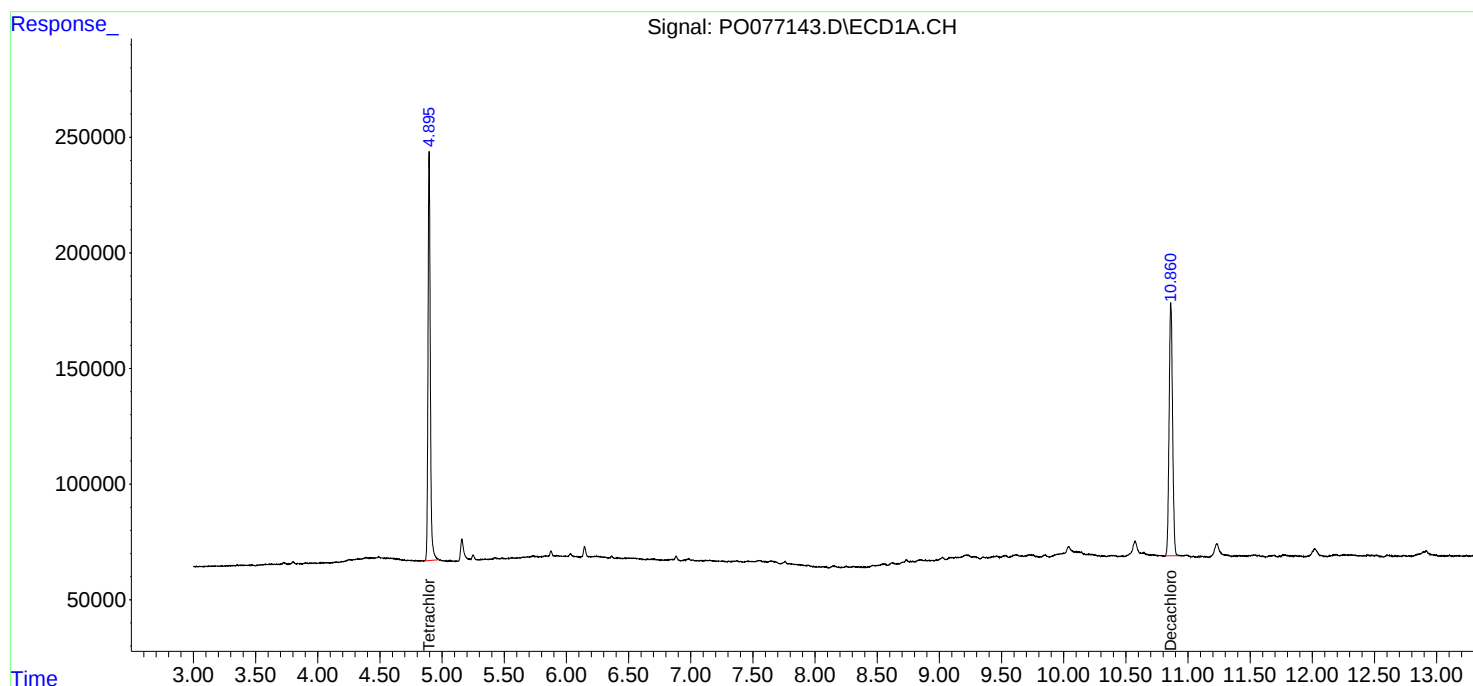


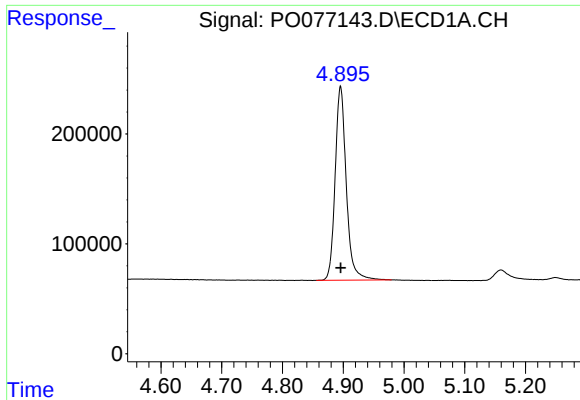

#1 Tetrachloro-m-xylene


R.T.: 4.896 min
Delta R.T.: 0.000 min
Response: 2245441
Conc: 21.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-8-D

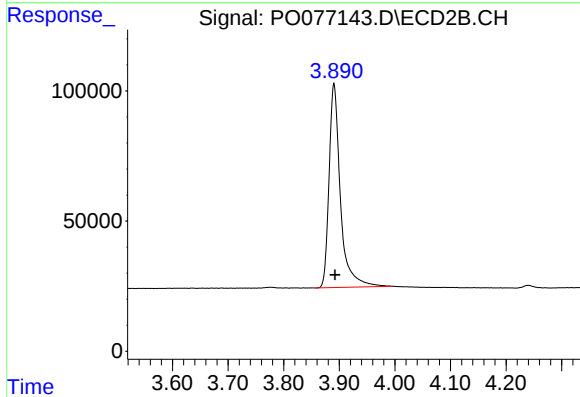


#1 Tetrachloro-m-xylene

R.T.: 3.890 min
Delta R.T.: -0.002 min
Response: 1113071
Conc: 21.16 ng/ml

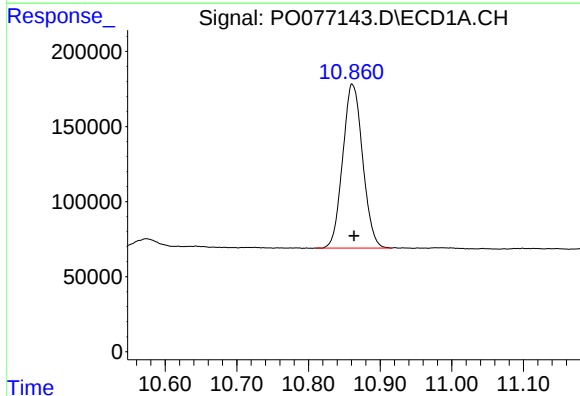

#2 Decachlorobiphenyl

R.T.: 10.861 min
Delta R.T.: -0.003 min
Response: 2109110
Conc: 20.31 ng/ml

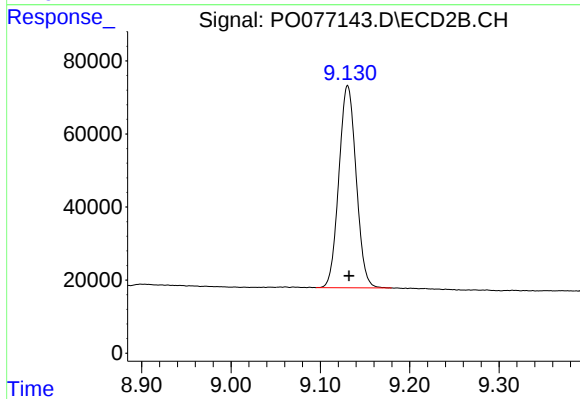

#2 Decachlorobiphenyl

R.T.: 9.131 min
Delta R.T.: -0.002 min
Response: 742803
Conc: 19.69 ng/ml