

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042221\
 Data File : P0077168.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Apr 2021 9:18
 Operator : DD\AJ
 Sample : M2091-01 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC248170L0Z-END-1-1

Manual Integrations
 APPROVED

Ankita
 4/22/2021 4:47:48 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 09:34:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 09:50:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.895	3.890	246898	132206	2.336m	2.513
2) SA Decachlor...	10.863	9.132	225336	79427	2.170	2.105
Target Compounds						
26) L6 AR-1254-1	7.123	5.996	56017	38293	13.622m	13.266
27) L6 AR-1254-2	7.354	6.154	94646	43073	14.623	16.684
28) L6 AR-1254-3	7.736	6.570	99255	68409	14.668	17.485
29) L6 AR-1254-4	8.032	6.811	79856	45046	16.238	19.826
30) L6 AR-1254-5	8.459	7.234	97912	75578	17.588m	20.845

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042221\
Data File : P0077168.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Apr 2021 9:18
Operator : DD\AJ
Sample : M2091-01 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BC248170L0Z-END-1-1


Manual Integrations
APPROVED

Ankita
4/22/2021 4:47:48 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 09:34:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 09:50:22 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

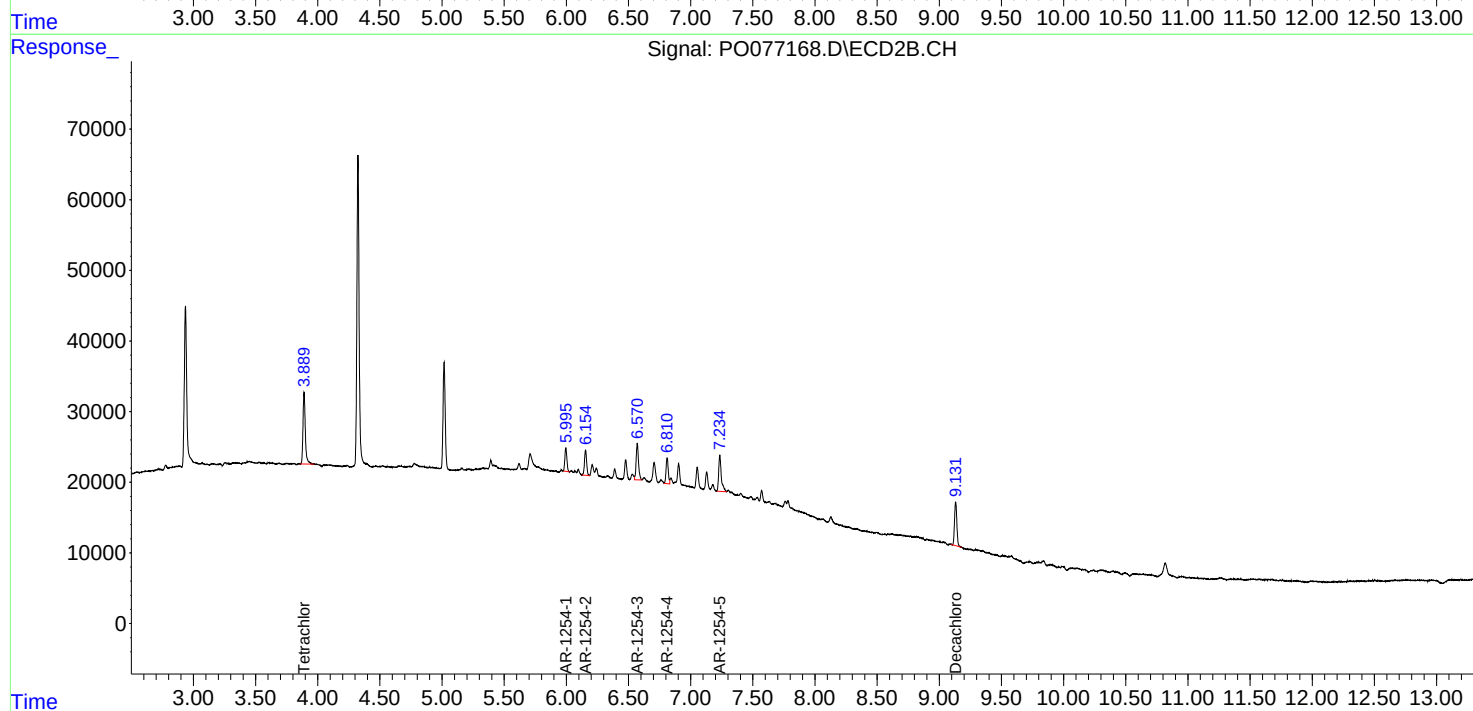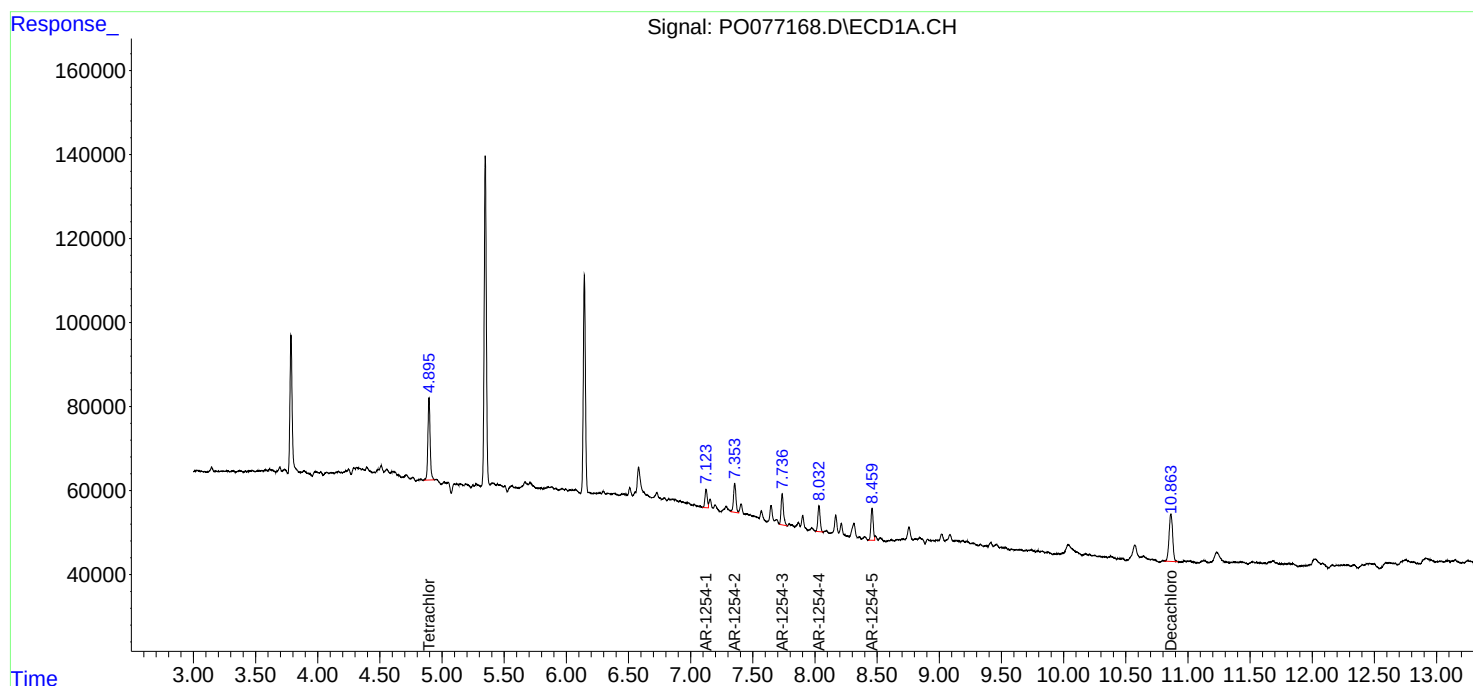

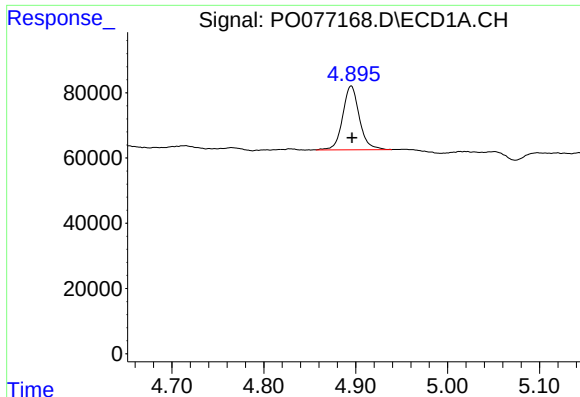


#1 Tetrachloro-m-xylene

R.T.: 4.895 min
Delta R.T.: -0.001 min
Response: 246898
Conc: 2.34 ng/ml m

Instrument :
ECD_O
ClientSampleId :
BC248170L0Z-END-1-1


Manual Integrations
APPROVED

Ankita
4/22/2021 4:47:48 PM

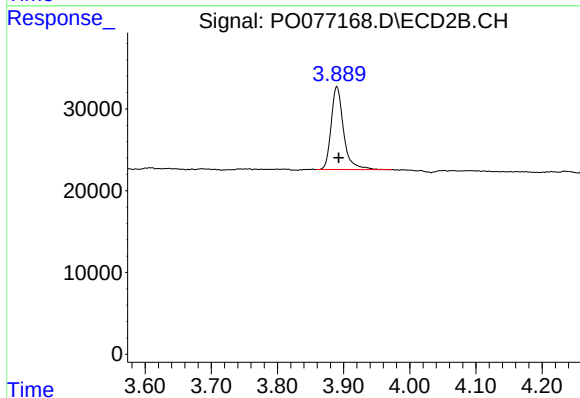


#1 Tetrachloro-m-xylene

R.T.: 3.890 min
Delta R.T.: -0.003 min
Response: 132206
Conc: 2.51 ng/ml

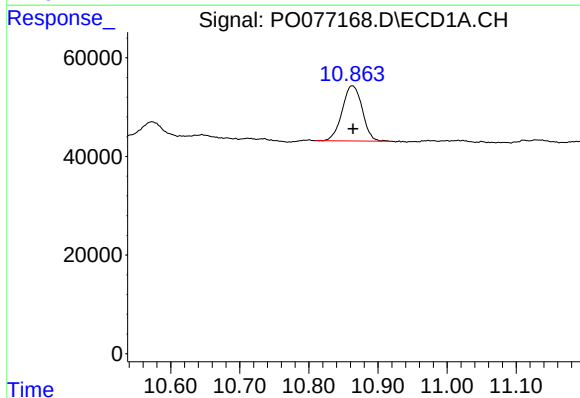


#2 Decachlorobiphenyl

R.T.: 10.863 min
Delta R.T.: 0.000 min
Response: 225336
Conc: 2.17 ng/ml

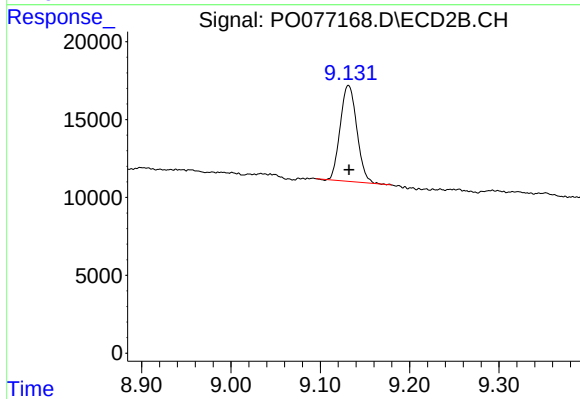

#2 Decachlorobiphenyl

R.T.: 9.132 min
Delta R.T.: 0.000 min
Response: 79427
Conc: 2.10 ng/ml

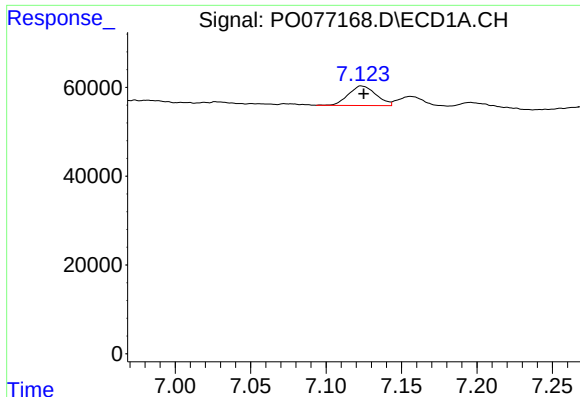


#26 AR-1254-1

R.T.: 7.123 min
Delta R.T.: -0.002 min
Response: 56017
Conc: 13.62 ng/ml m

Instrument :
ECD_O
ClientSampleId :
BC248170L0Z-END-1-1


Manual Integrations
APPROVED

Ankita
4/22/2021 4:47:48 PM

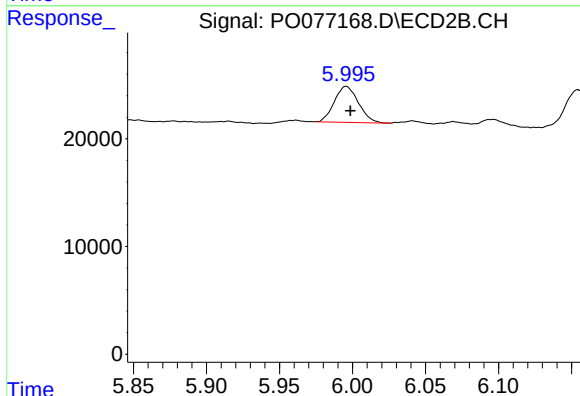


#26 AR-1254-1

R.T.: 5.996 min
Delta R.T.: -0.003 min
Response: 38293
Conc: 13.27 ng/ml

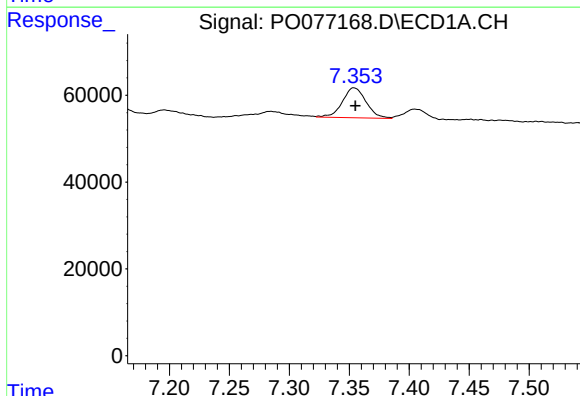


#27 AR-1254-2

R.T.: 7.354 min
Delta R.T.: 0.000 min
Response: 94646
Conc: 14.62 ng/ml

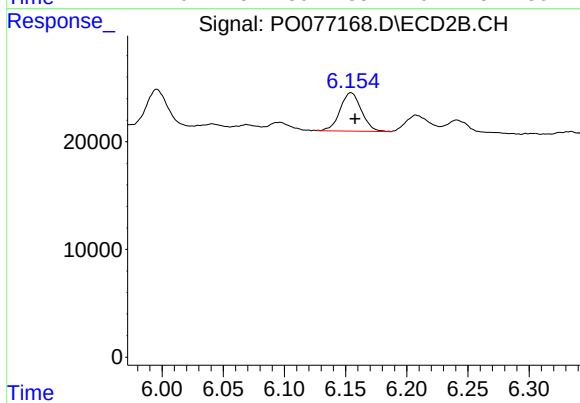

#27 AR-1254-2

R.T.: 6.154 min
Delta R.T.: -0.003 min
Response: 43073
Conc: 16.68 ng/ml

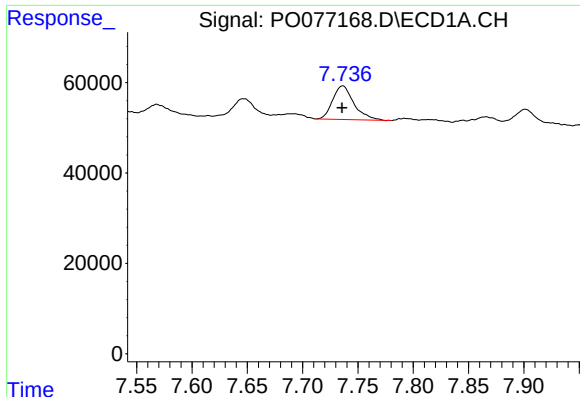


#28 AR-1254-3

R.T.: 7.736 min
Delta R.T.: 0.000 min
Response: 99255
Conc: 14.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC248170L0Z-END-1-1


Manual Integrations
APPROVED

Ankita
4/22/2021 4:47:48 PM

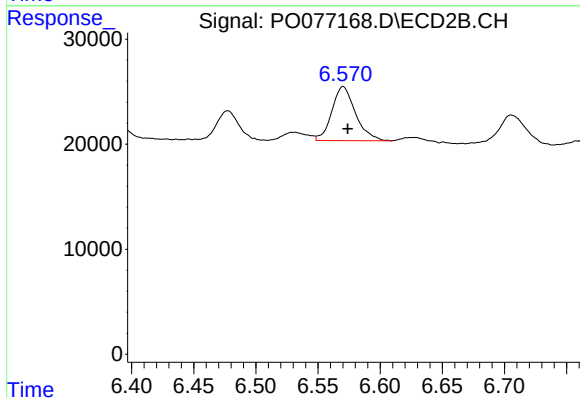


#28 AR-1254-3

R.T.: 6.570 min
Delta R.T.: -0.004 min
Response: 68409
Conc: 17.48 ng/ml

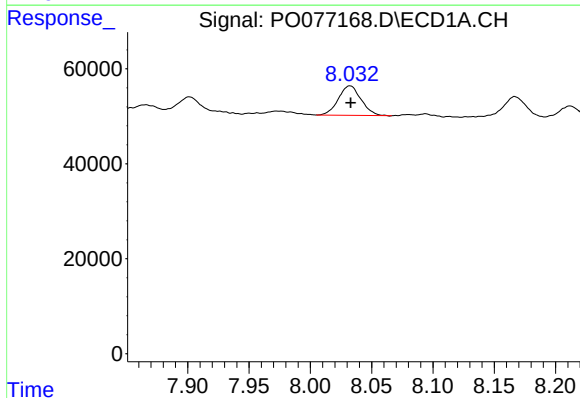


#29 AR-1254-4

R.T.: 8.032 min
Delta R.T.: 0.000 min
Response: 79856
Conc: 16.24 ng/ml

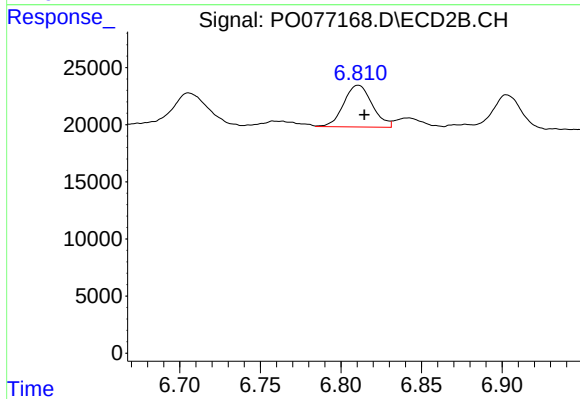

#29 AR-1254-4

R.T.: 6.811 min
Delta R.T.: -0.004 min
Response: 45046
Conc: 19.83 ng/ml

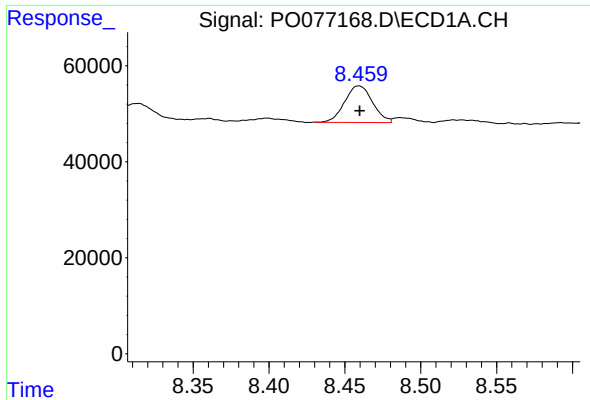


#30 AR-1254-5

R.T.: 8.459 min
Delta R.T.: 0.000 min
Response: 97912
Conc: 17.59 ng/ml m

Instrument :
ECD_O
ClientSampleId :
BC248170L0Z-END-1-1

Manual Integrations
APPROVED

Ankita
4/22/2021 4:47:48 PM

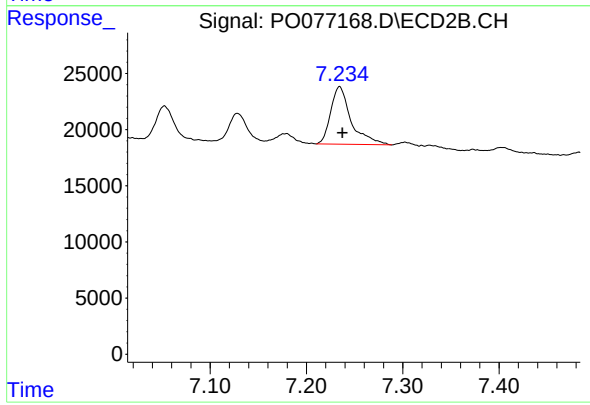

#30 AR-1254-5

R.T.: 7.234 min
Delta R.T.: -0.003 min
Response: 75578
Conc: 20.84 ng/ml