

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042319\
 Data File : P0055544.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Apr 2019 14:43
 Operator : SM/SJ
 Sample : K2201-05RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PL-01-041819-CRE

Manual Integrations
 APPROVED

mohammad
 4/25/2019 8:36:31 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 15:02:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.290	3.601	579431	587267	16.696	18.402m
2) SA Decachlor...	9.903	8.562	543641	367872	11.028	11.551

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO042319\
Data File : PO055544.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Apr 2019 14:43
Operator : SM/SJ
Sample : K2201-05RE
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PL-01-041819-CRE


Manual Integrations
APPROVED

mohammad
4/25/2019 8:36:31 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 15:02:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

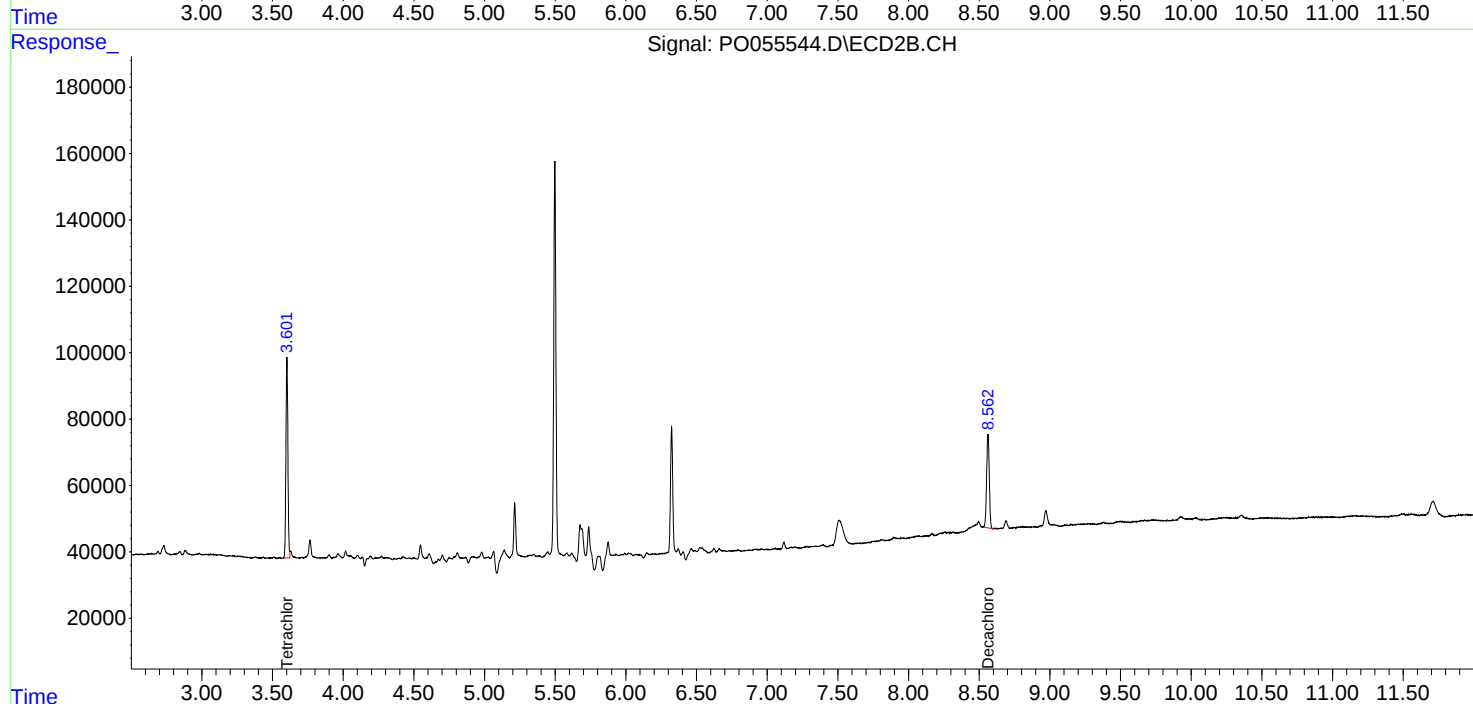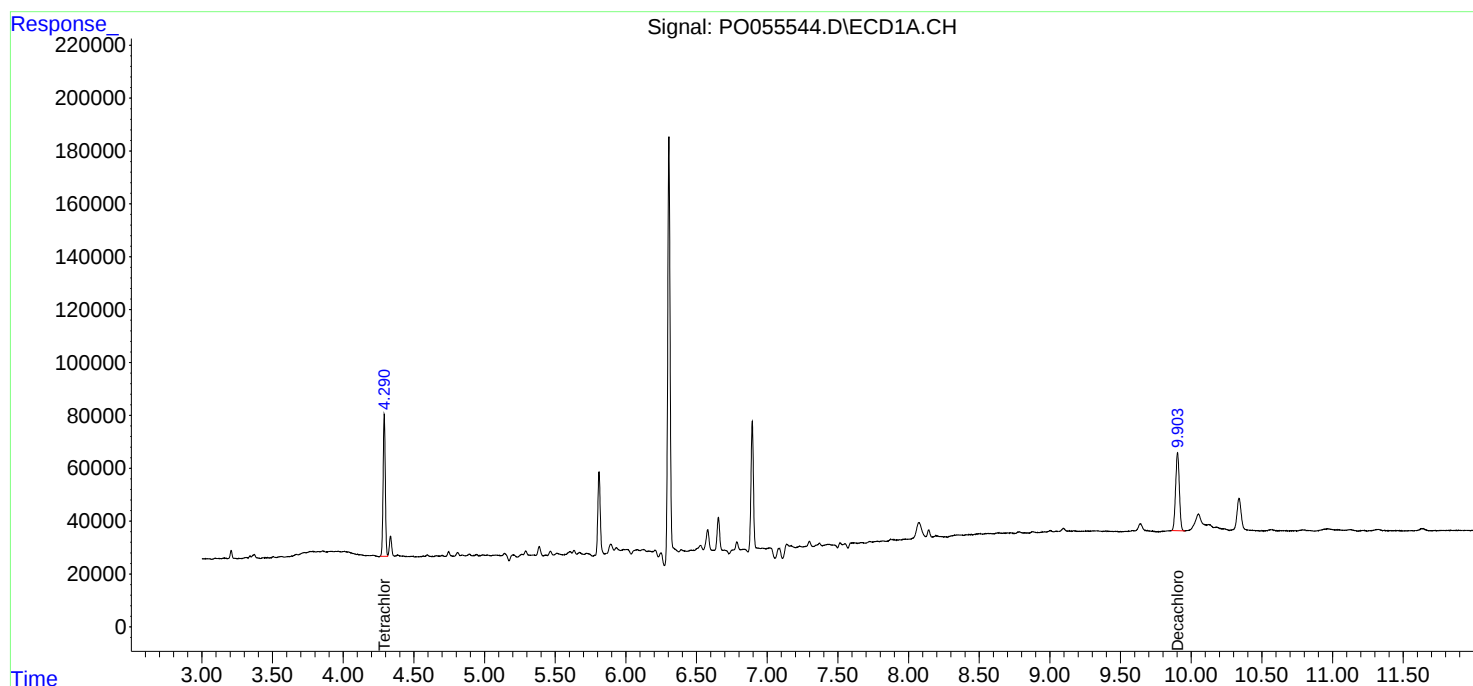

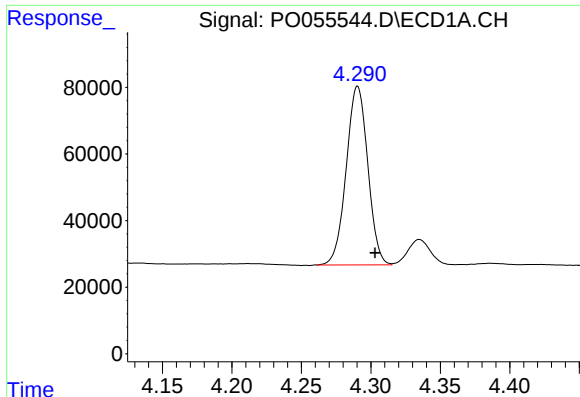


#1 Tetrachloro-m-xylene

R.T.: 4.290 min
Delta R.T.: -0.013 min
Response: 579431
Conc: 16.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
PL-01-041819-CRE


Manual Integrations
APPROVED

mohammad
4/25/2019 8:36:31 AM

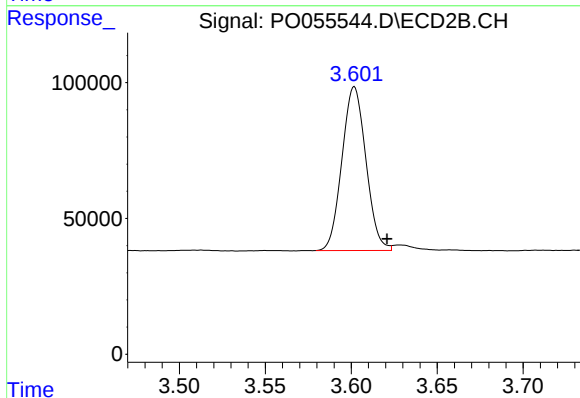


#1 Tetrachloro-m-xylene

R.T.: 3.601 min
Delta R.T.: -0.019 min
Response: 587267
Conc: 18.40 ng/ml m

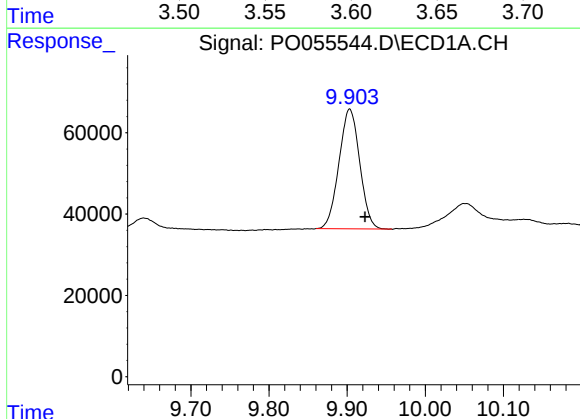

#2 Decachlorobiphenyl

R.T.: 9.903 min
Delta R.T.: -0.020 min
Response: 543641
Conc: 11.03 ng/ml

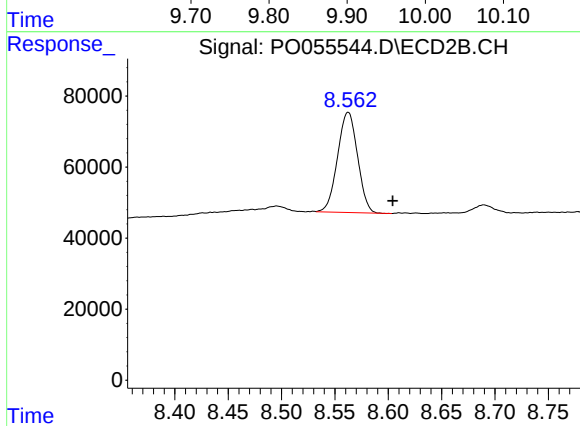

#2 Decachlorobiphenyl

R.T.: 8.562 min
Delta R.T.: -0.042 min
Response: 367872
Conc: 11.55 ng/ml