

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042319\
 Data File : P0055545.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Apr 2019 15:00
 Operator : SM/SJ
 Sample : K2201-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PL-01-041819-D

Manual Integrations
 APPROVED

mohammad
 4/25/2019 8:36:27 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 15:17:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.291	3.602	682417	700759	19.663	21.959m
2) SA Decachlor...	9.902	8.563	593687	397604	12.043	12.484

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042319\
Data File : P0055545.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Apr 2019 15:00
Operator : SM/SJ
Sample : K2201-07
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PL-01-041819-D


Manual Integrations
APPROVED

mohammad
4/25/2019 8:36:27 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 15:17:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

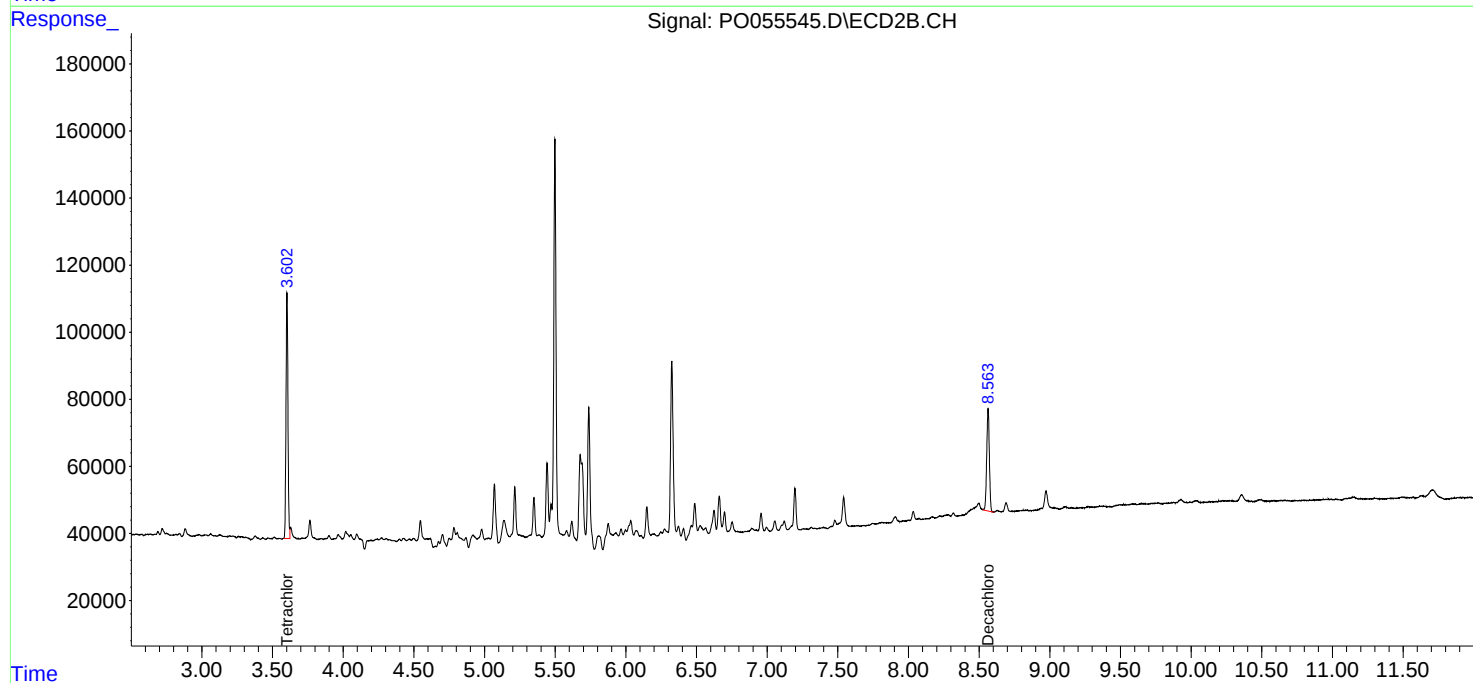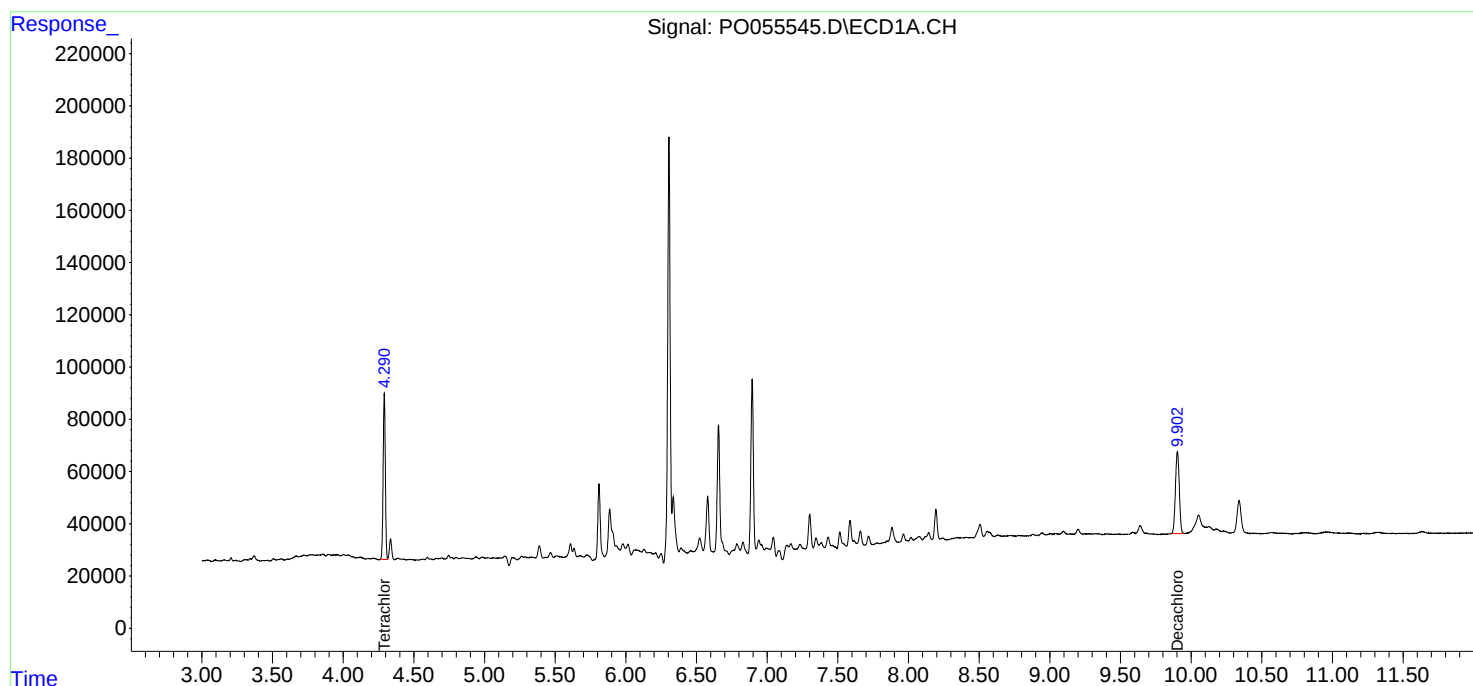

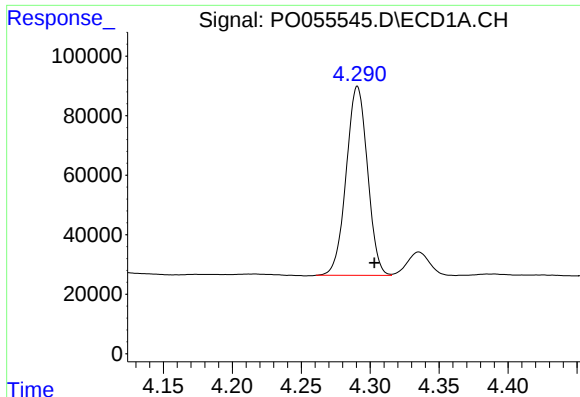


#1 Tetrachloro-m-xylene

R.T.: 4.291 min
Delta R.T.: -0.012 min
Response: 682417
Conc: 19.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
PL-01-041819-D


Manual Integrations
APPROVED

mohammad
4/25/2019 8:36:27 AM

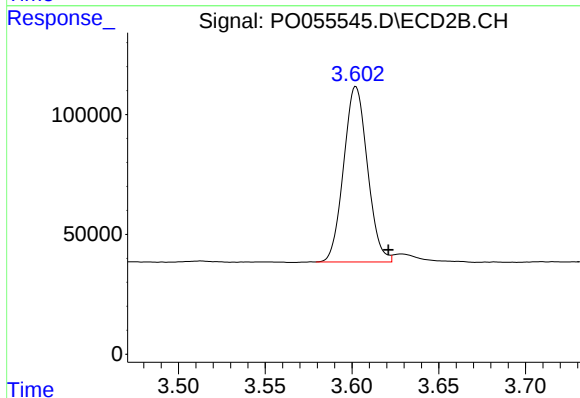


#1 Tetrachloro-m-xylene

R.T.: 3.602 min
Delta R.T.: -0.019 min
Response: 700759
Conc: 21.96 ng/ml m

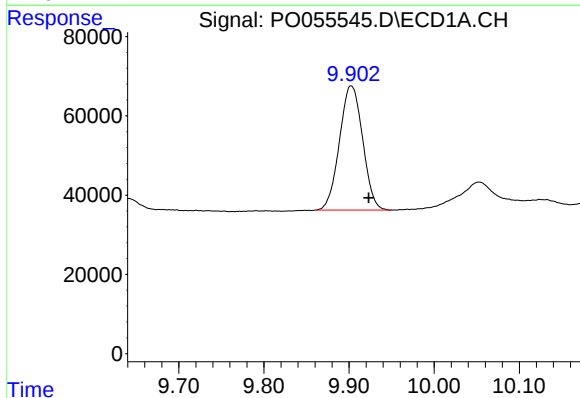

#2 Decachlorobiphenyl

R.T.: 9.902 min
Delta R.T.: -0.021 min
Response: 593687
Conc: 12.04 ng/ml

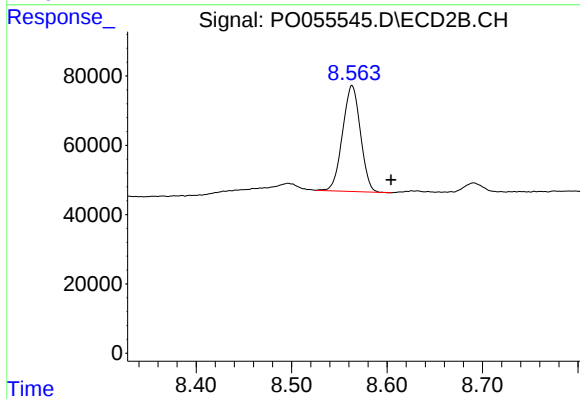

#2 Decachlorobiphenyl

R.T.: 8.563 min
Delta R.T.: -0.041 min
Response: 397604
Conc: 12.48 ng/ml