

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042319\
Data File : P0055548.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Apr 2019 15:54
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Manual Integrations
APPROVED

mohammad
4/25/2019 8:36:40 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 24 00:24:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.297	3.603	664858	735967	19.157	23.062
2) SA Decachlor...	9.911	8.564	674281	437005	13.678	13.721m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042319\
Data File : P0055548.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Apr 2019 15:54
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

mohammad
4/25/2019 8:36:40 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 24 00:24:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

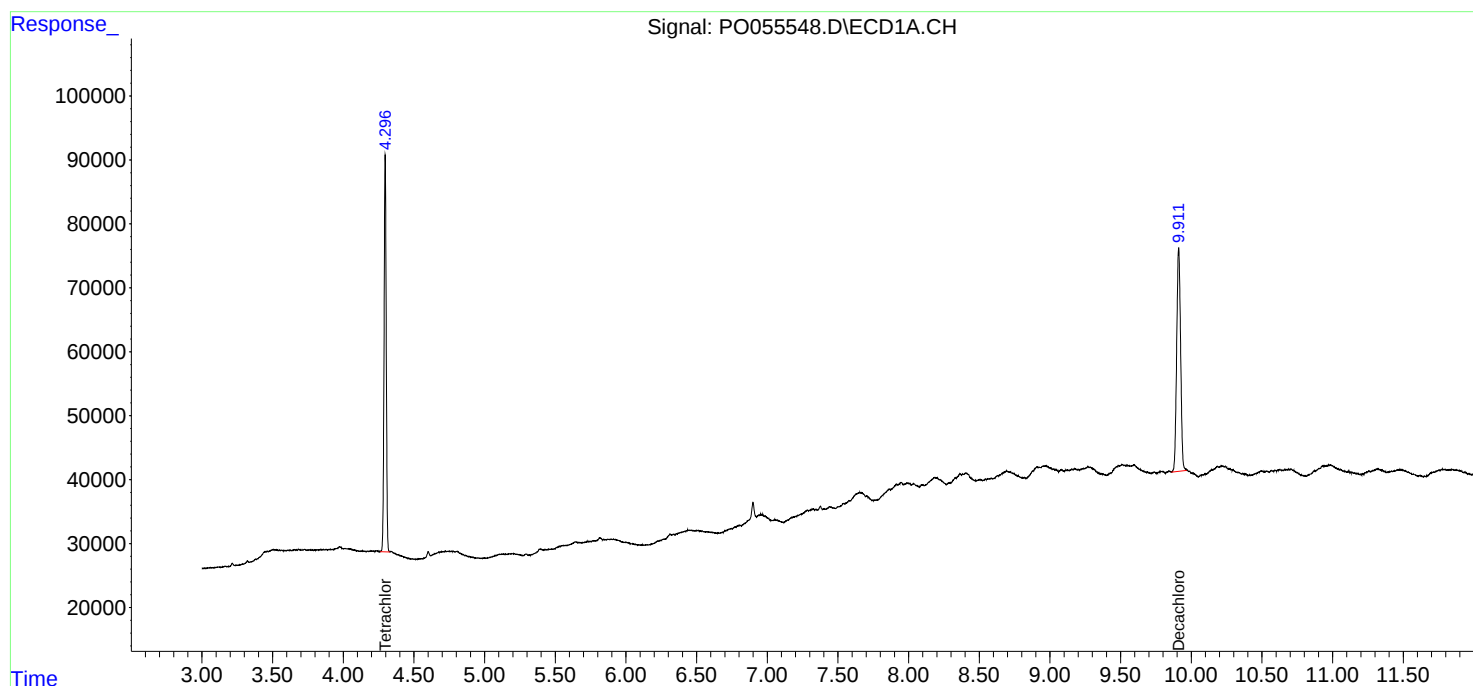

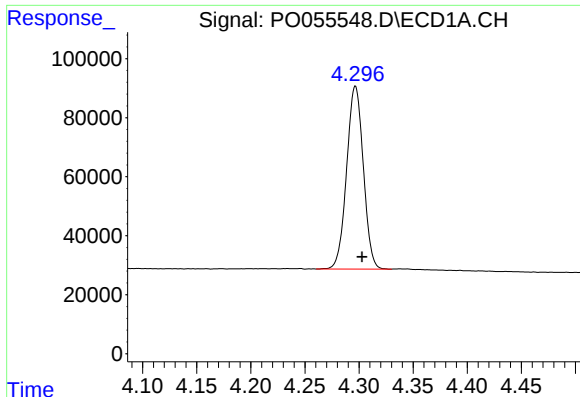


#1 Tetrachloro-m-xylene

R.T.: 4.297 min
Delta R.T.: -0.006 min
Response: 664858
Conc: 19.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

mohammad
4/25/2019 8:36:40 AM

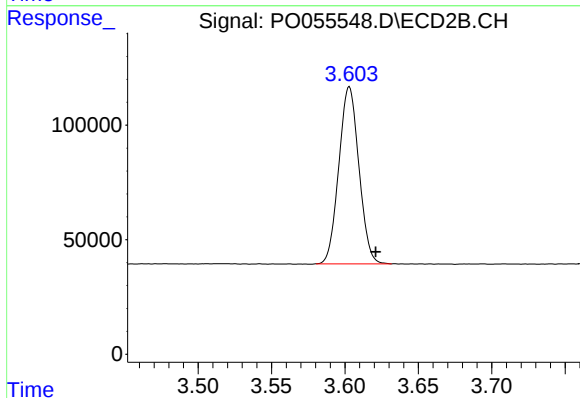


#1 Tetrachloro-m-xylene

R.T.: 3.603 min
Delta R.T.: -0.018 min
Response: 735967
Conc: 23.06 ng/ml

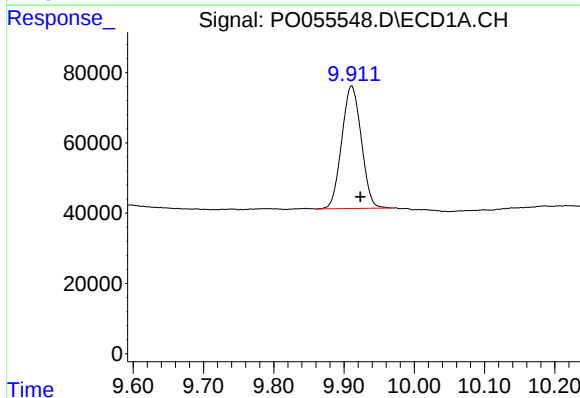

#2 Decachlorobiphenyl

R.T.: 9.911 min
Delta R.T.: -0.012 min
Response: 674281
Conc: 13.68 ng/ml

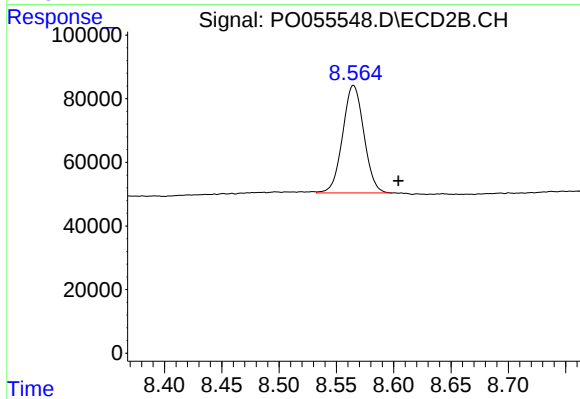

#2 Decachlorobiphenyl

R.T.: 8.564 min
Delta R.T.: -0.040 min
Response: 437005
Conc: 13.72 ng/ml m