

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042319\
 Data File : P0055552.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Apr 2019 20:40
 Operator : SM/SJ
 Sample : K2514-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-EF-01-007-ABCD

Manual Integrations
 APPROVED

mohammad
 4/25/2019 8:36:52 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 24 00:26:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.289	3.601	740232	789268	21.329m	24.732m
2) SA Decachlor...	9.901	8.562	631024	419359	12.800	13.167

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042319\
Data File : P0055552.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Apr 2019 20:40
Operator : SM/SJ
Sample : K2514-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FK-EF-01-007-ABCD


Manual Integrations
APPROVED

mohammad
4/25/2019 8:36:52 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 24 00:26:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

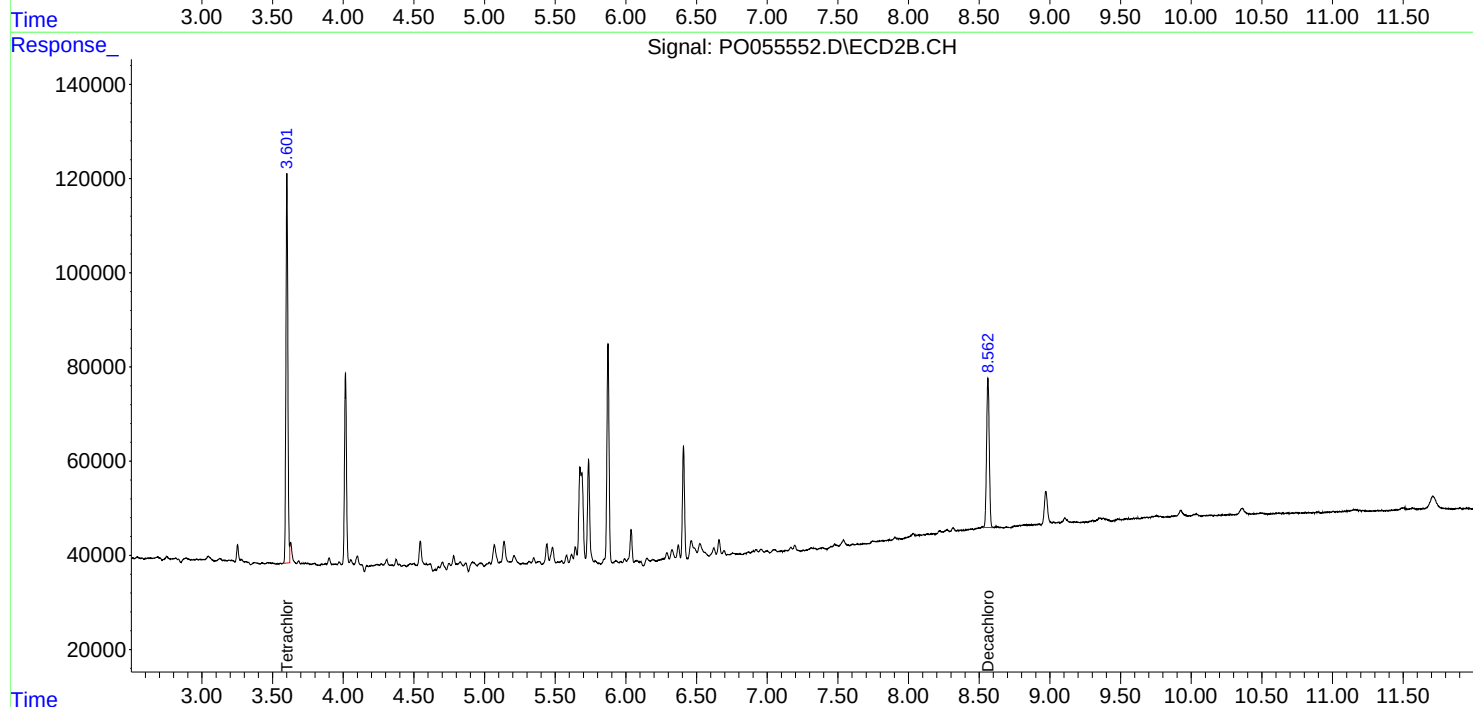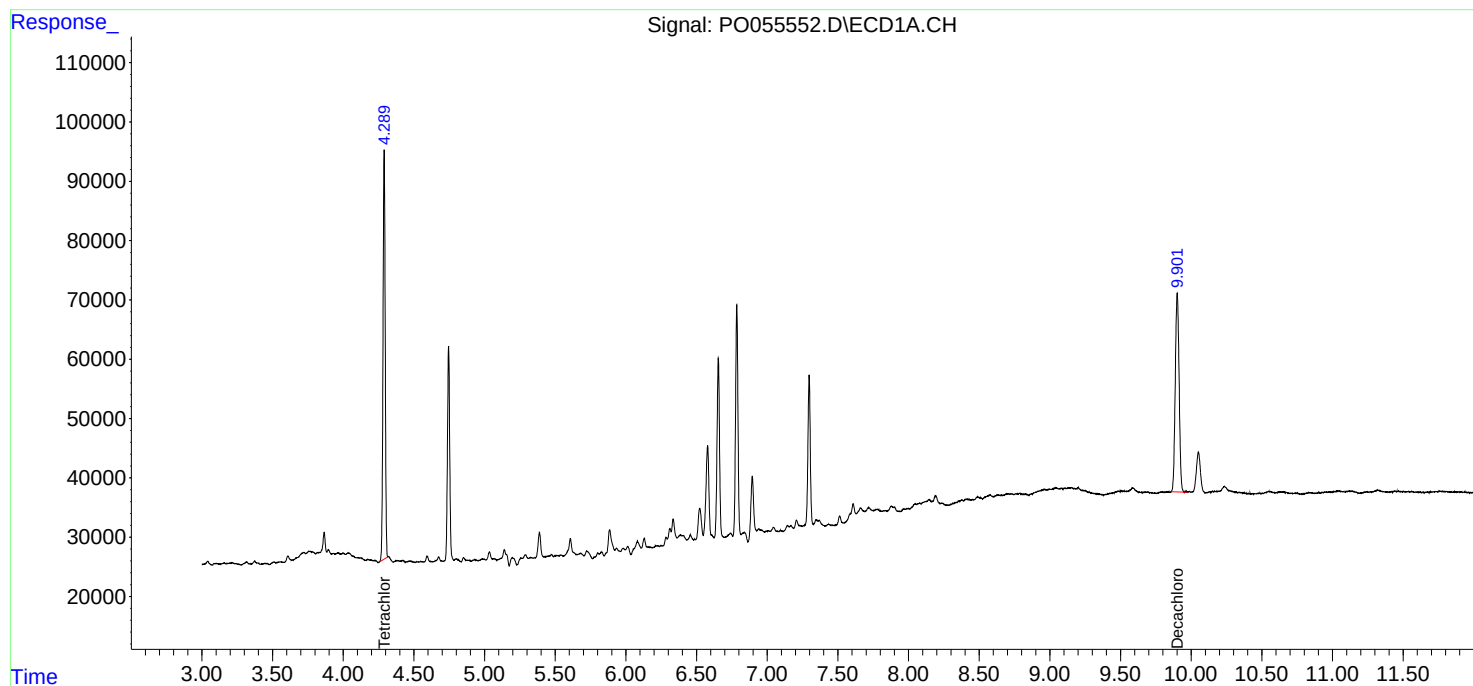

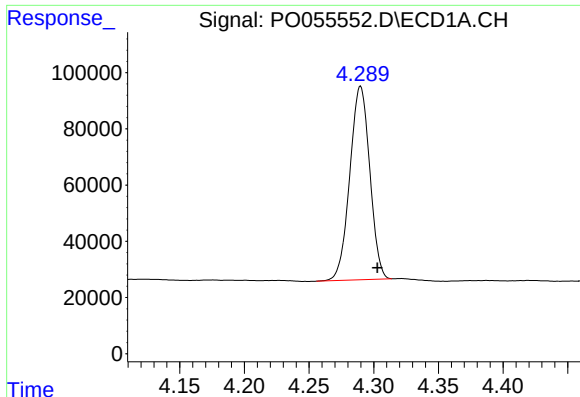


#1 Tetrachloro-m-xylene

R.T.: 4.289 min
Delta R.T.: -0.014 min
Response: 740232
Conc: 21.33 ng/ml m

Instrument :
ECD_O
ClientSampleId :
FK-EF-01-007-ABCD


Manual Integrations
APPROVED

mohammad
4/25/2019 8:36:52 AM

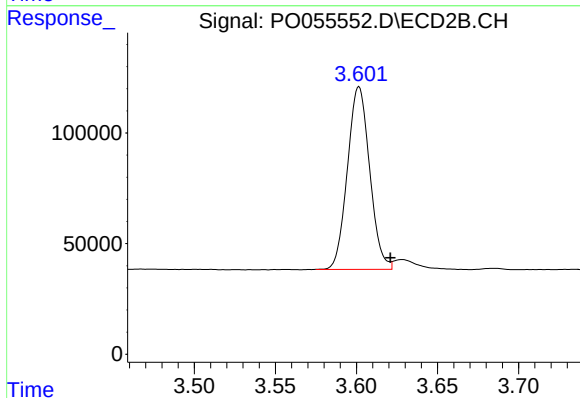


#1 Tetrachloro-m-xylene

R.T.: 3.601 min
Delta R.T.: -0.020 min
Response: 789268
Conc: 24.73 ng/ml m

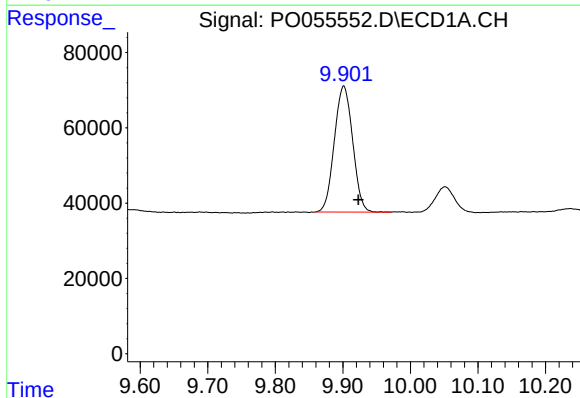

#2 Decachlorobiphenyl

R.T.: 9.901 min
Delta R.T.: -0.022 min
Response: 631024
Conc: 12.80 ng/ml

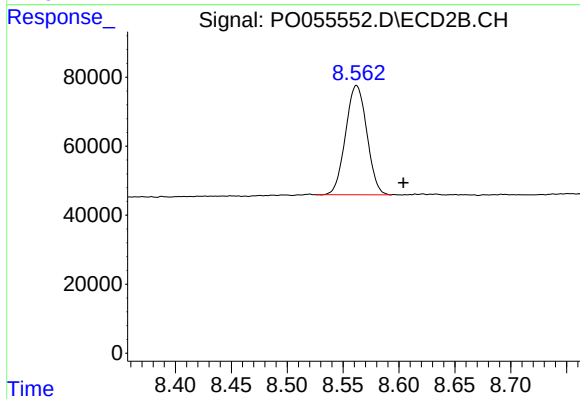

#2 Decachlorobiphenyl

R.T.: 8.562 min
Delta R.T.: -0.042 min
Response: 419359
Conc: 13.17 ng/ml