

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042321\
 Data File : P0077188.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Apr 2021 17:45
 Operator : DD\AJ
 Sample : M2091-18 20X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 01:36:17 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 09:50:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.898	3.892	123473	51100	1.168	0.971
2)	SA Decachlor...	10.867	0.000	91463	0	0.881	N.D. #
Target Compounds							
20)	L4 AR-1242-5	7.202	0.000	52966	0	22.907	N.D. #
24)	L5 AR-1248-4	7.148	0.000	130890	0	32.387	N.D. #
25)	L5 AR-1248-5	7.202	0.000	52966	0	12.965	N.D. #
26)	L6 AR-1254-1	7.148f	0.000	130890	0	31.830	N.D. #
31)	L7 AR-1260-1	7.900	0.000	14749	0	2.726	N.D. #
32)	L7 AR-1260-2	8.167	6.920	91003	60791	14.412	17.052
34)	L7 AR-1260-4	8.772	0.000	38206	0	7.898	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042321\
Data File : P0077188.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Apr 2021 17:45
Operator : DD\AJ
Sample : M2091-18 20X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 01:36:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 09:50:22 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

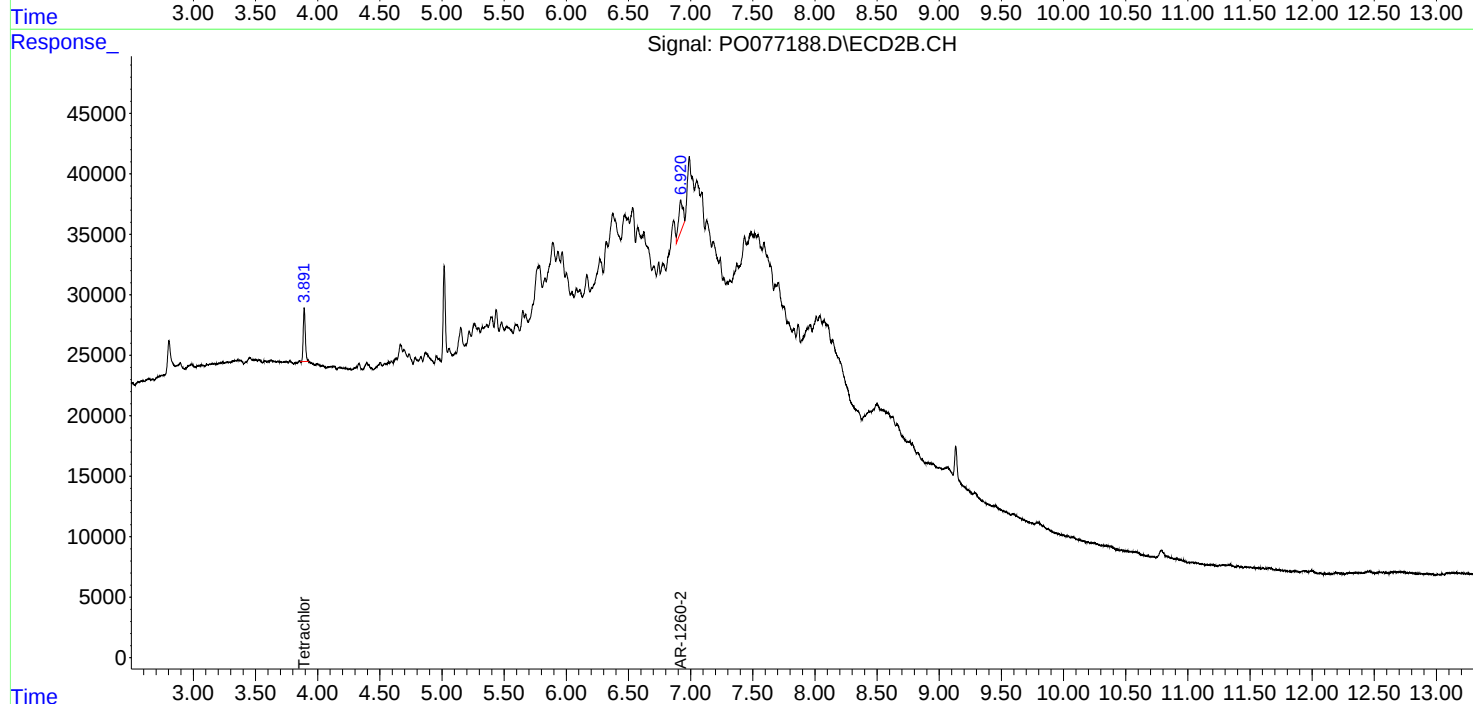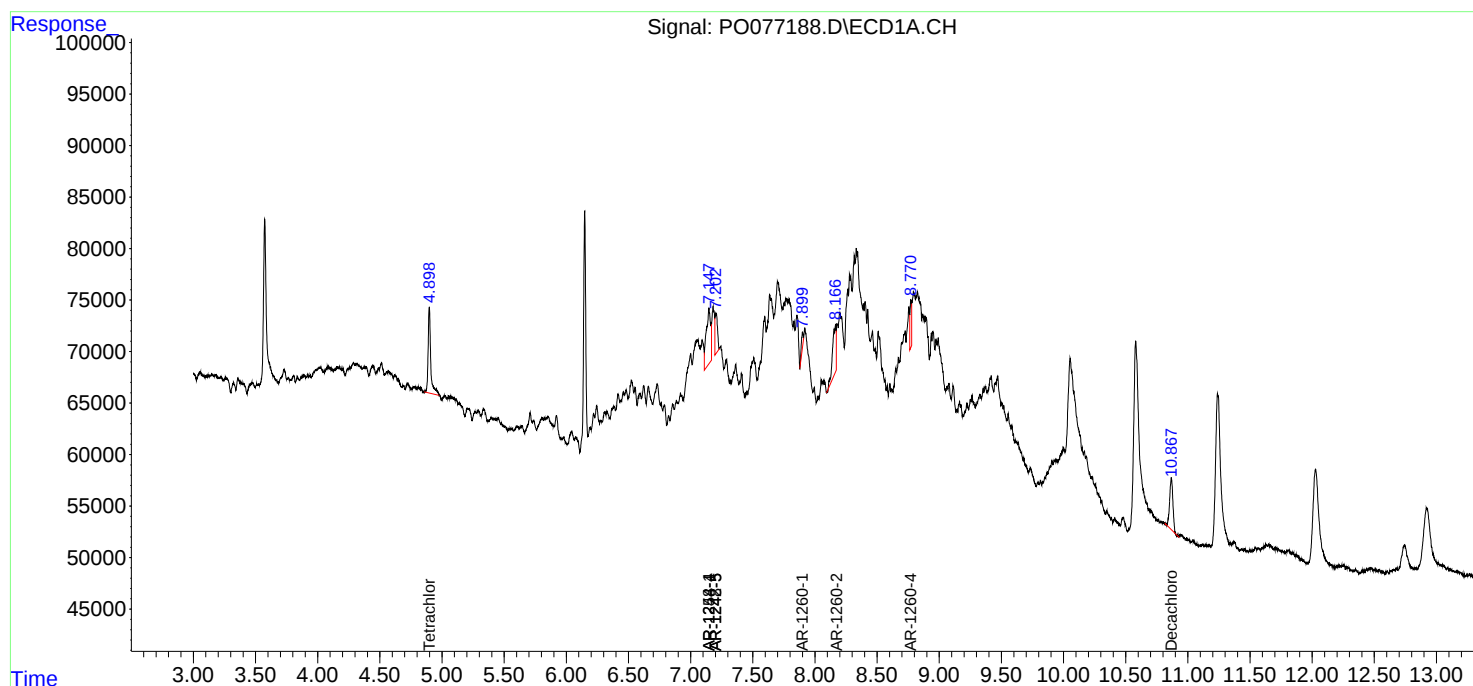


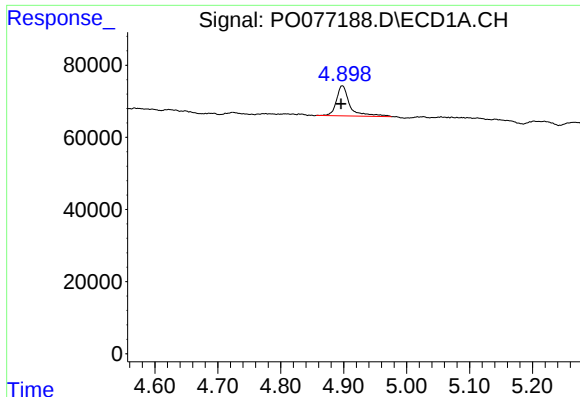

#1 Tetrachloro-m-xylene


R.T.: 4.898 min
Delta R.T.: 0.002 min
Response: 123473
Conc: 1.17 ng/ml

Instrument :
ECD_O
ClientSampleId :

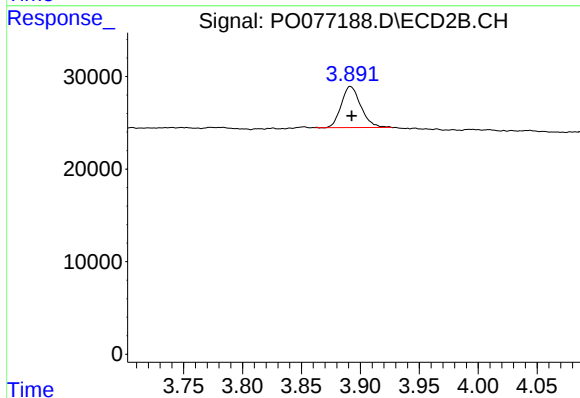


#1 Tetrachloro-m-xylene

R.T.: 3.892 min
Delta R.T.: -0.001 min
Response: 51100
Conc: 0.97 ng/ml

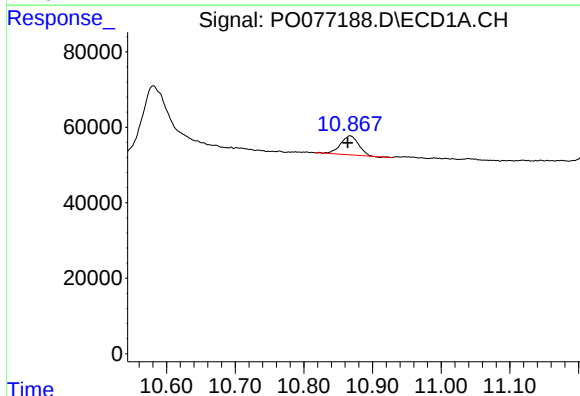


#2 Decachlorobiphenyl

R.T.: 10.867 min
Delta R.T.: 0.004 min
Response: 91463
Conc: 0.88 ng/ml

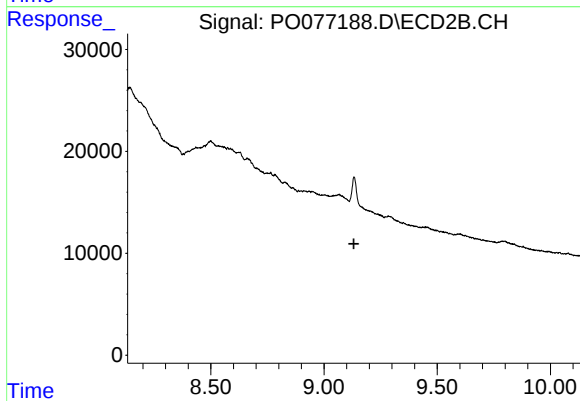

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 9.132 min
Response: 0
Conc: N.D.

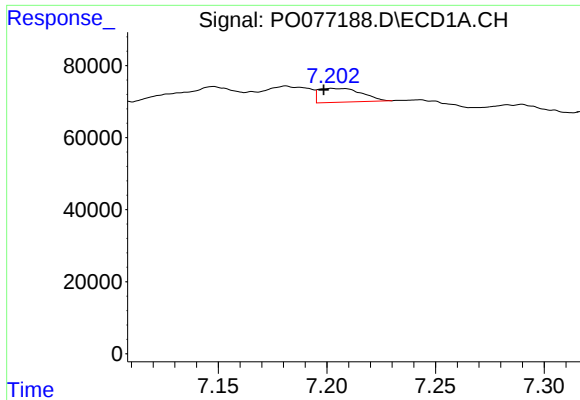

#20 AR-1242-5


R.T.: 7.202 min
Delta R.T.: 0.004 min
Response: 52966
Conc: 22.91 ng/ml

Instrument :
ECD_O
ClientSampleId :

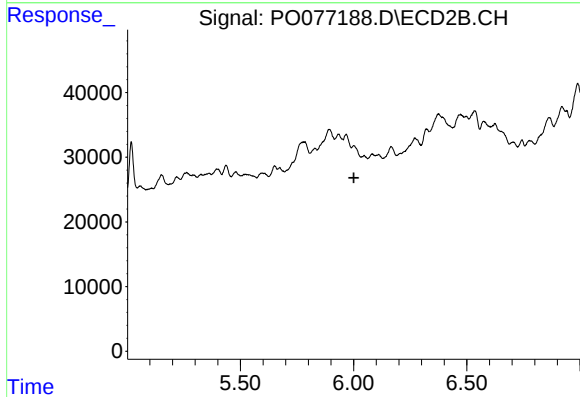


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 6.001 min
Response: 0
Conc: N.D.

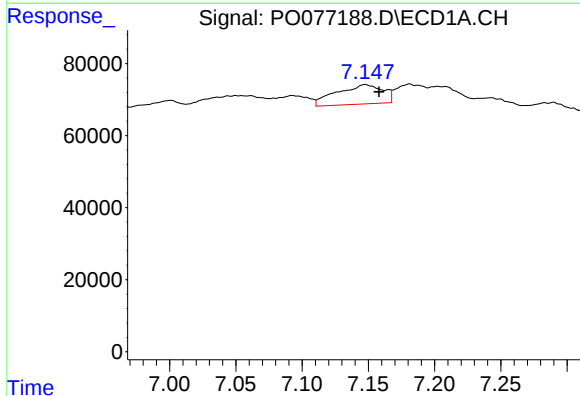


#24 AR-1248-4

R.T.: 7.148 min
Delta R.T.: -0.011 min
Response: 130890
Conc: 32.39 ng/ml

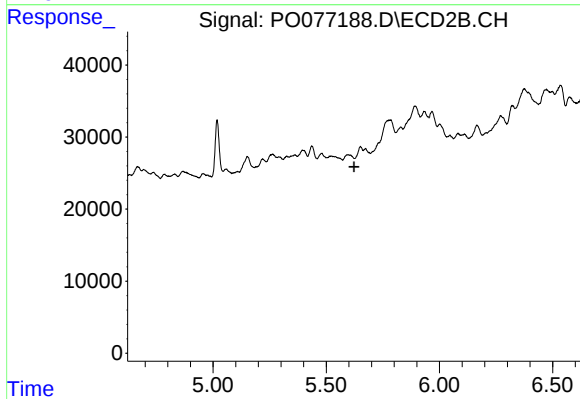

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.622 min
Response: 0
Conc: N.D.

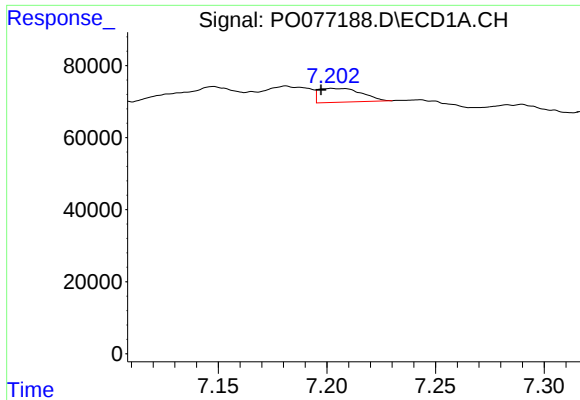

#25 AR-1248-5


R.T.: 7.202 min
Delta R.T.: 0.005 min
Response: 52966
Conc: 12.96 ng/ml

Instrument :
ECD_O
ClientSampleId :

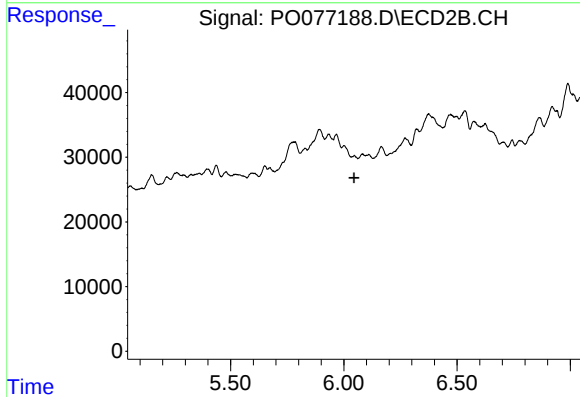


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 6.045 min
Response: 0
Conc: N.D.

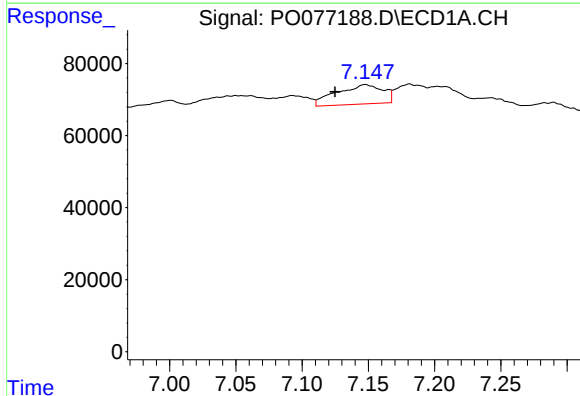


#26 AR-1254-1

R.T.: 7.148 min
Delta R.T.: 0.023 min
Response: 130890
Conc: 31.83 ng/ml

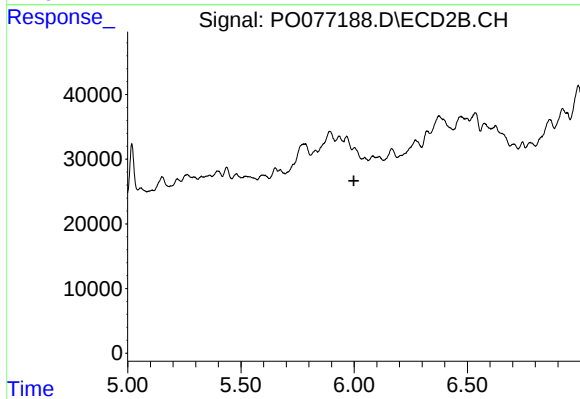

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 5.999 min
Response: 0
Conc: N.D.

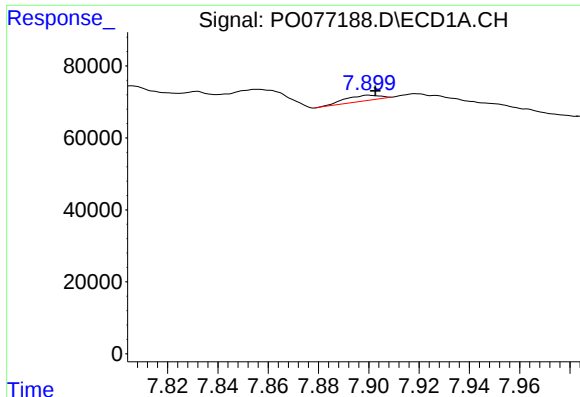

#31 AR-1260-1


R.T.: 7.900 min
Delta R.T.: -0.003 min
Response: 14749
Conc: 2.73 ng/ml

Instrument :
ECD_O
ClientSampleId :

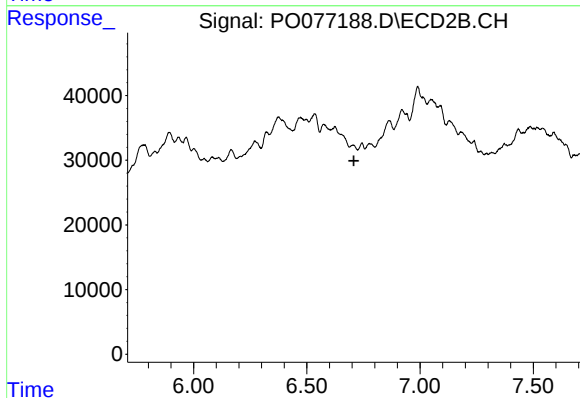


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 6.708 min
Response: 0
Conc: N.D.

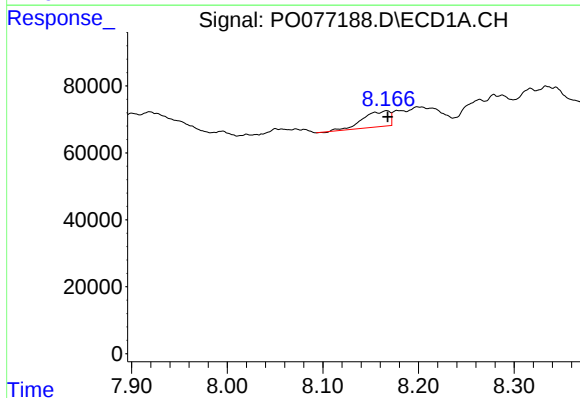


#32 AR-1260-2

R.T.: 8.167 min
Delta R.T.: -0.001 min
Response: 91003
Conc: 14.41 ng/ml

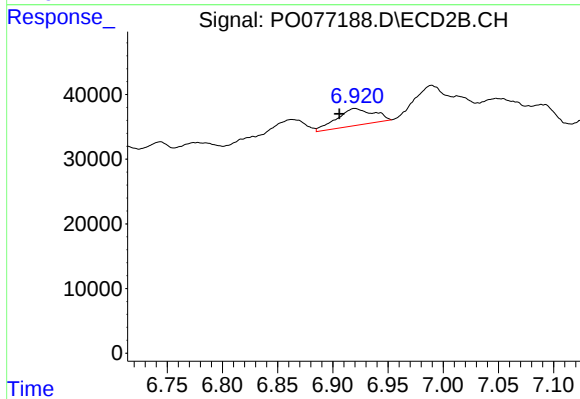

#32 AR-1260-2


R.T.: 6.920 min
Delta R.T.: 0.014 min
Response: 60791
Conc: 17.05 ng/ml

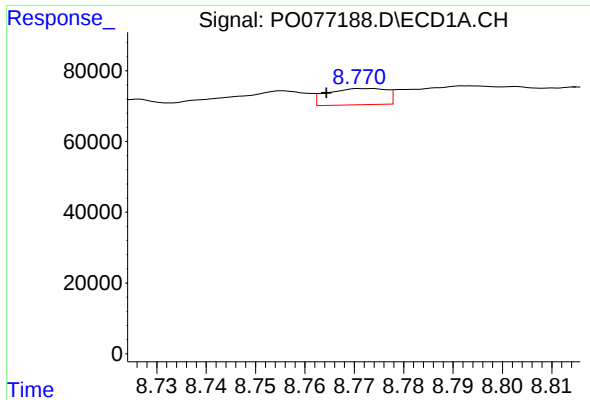

#34 AR-1260-4

R.T.: 8.772 min
Delta R.T.: 0.008 min
Response: 38206
Conc: 7.90 ng/ml

Instrument :
ECD_O
ClientSampleId :

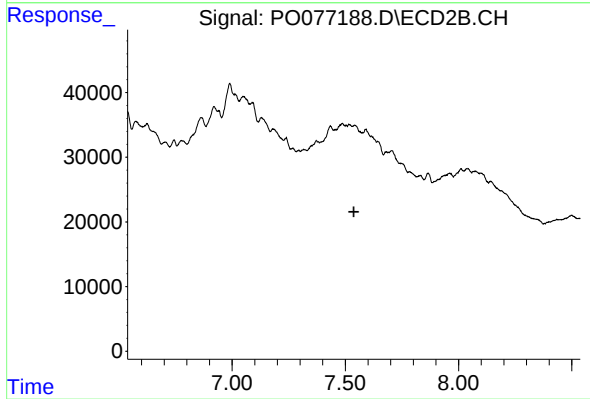

#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.537 min
Response: 0
Conc: N.D.