

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042321\
 Data File : P0077184.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Apr 2021 16:36
 Operator : DD\AJ
 Sample : M2091-04 20X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC248170L0Z-END-2-2

Manual Integrations
 APPROVED

Ankita
 4/23/2021 4:46:56 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 01:35:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 09:50:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.894	3.889	119373	44947	1.130m	0.854m
2) SA Decachlor...	10.860	9.128	142696	39003	1.374	1.034m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042321\
Data File : P0077184.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Apr 2021 16:36
Operator : DD\AJ
Sample : M2091-04 20X
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BC248170L0Z-END-2-2


Manual Integrations
APPROVED

Ankita
4/23/2021 4:46:56 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 01:35:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 09:50:22 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

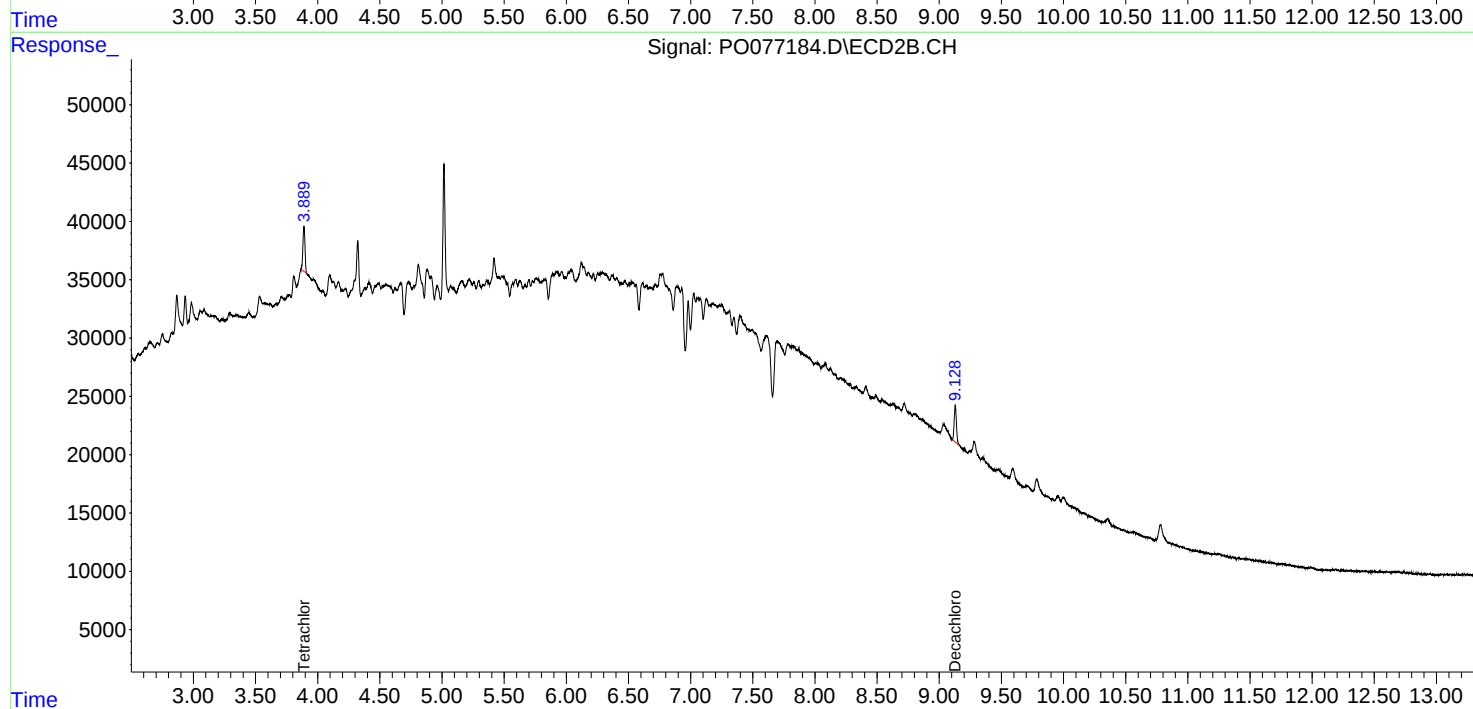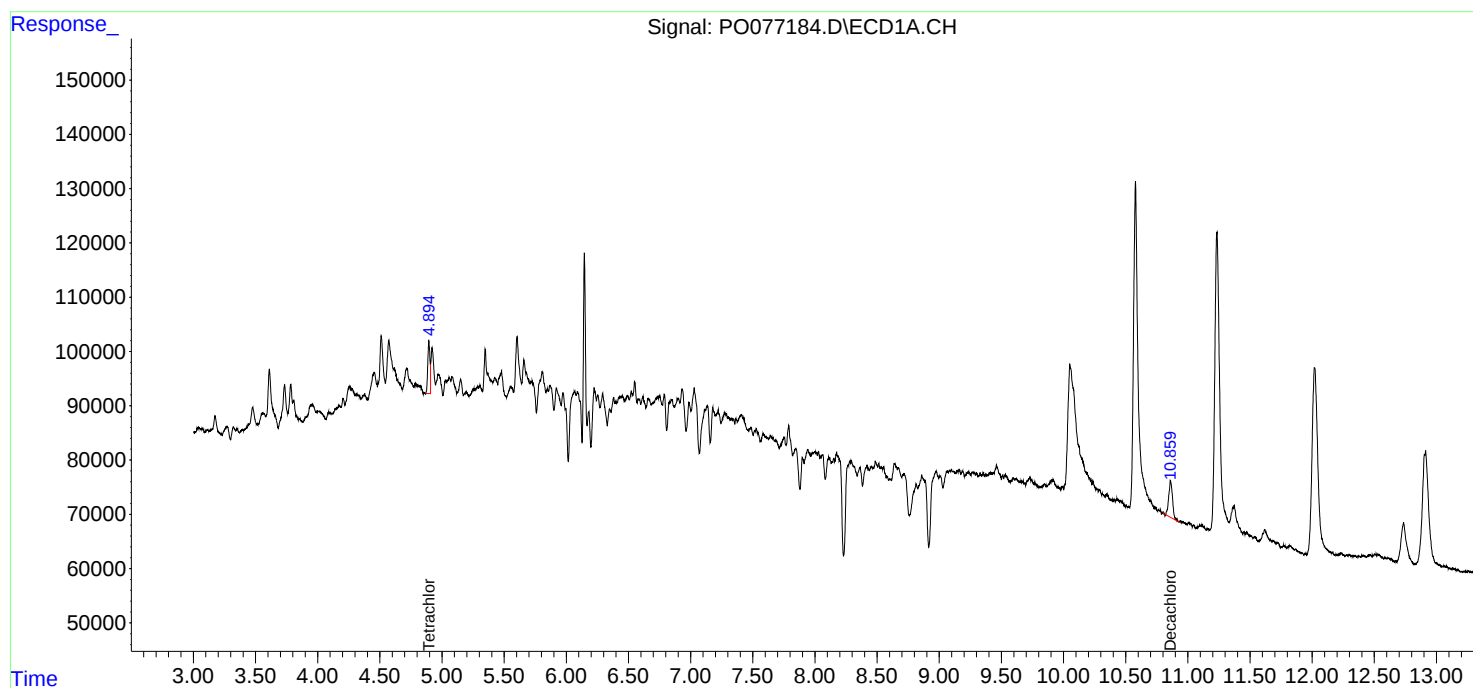

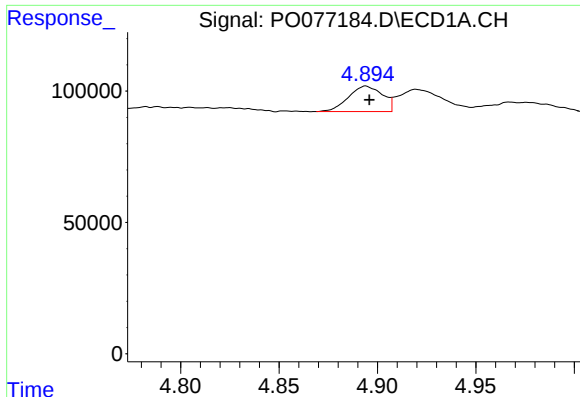


#1 Tetrachloro-m-xylene

R.T.: 4.894 min
Delta R.T.: -0.002 min
Response: 119373
Conc: 1.13 ng/ml m

Instrument :
ECD_O
ClientSampleId :
BC248170L0Z-END-2-2


Manual Integrations
APPROVED

Ankita
4/23/2021 4:46:56 PM

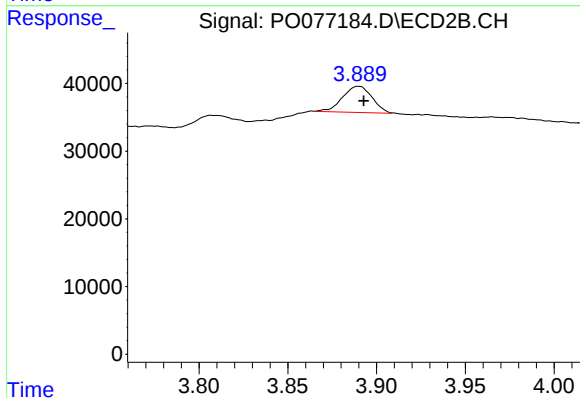


#1 Tetrachloro-m-xylene

R.T.: 3.889 min
Delta R.T.: -0.004 min
Response: 44947
Conc: 0.85 ng/ml m

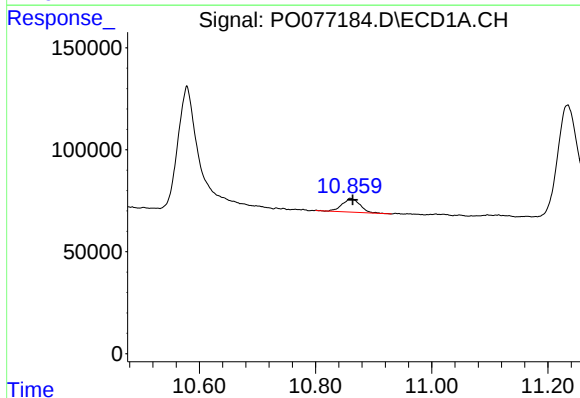

#2 Decachlorobiphenyl

R.T.: 10.860 min
Delta R.T.: -0.004 min
Response: 142696
Conc: 1.37 ng/ml

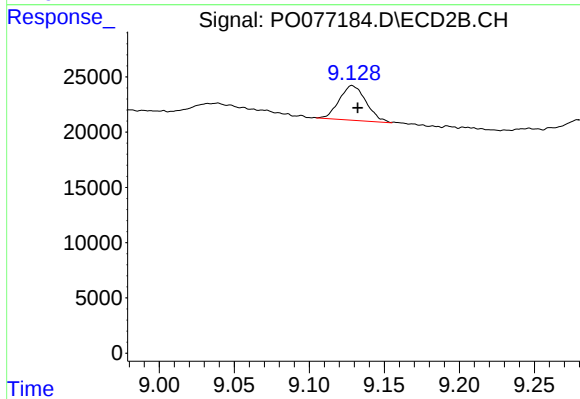

#2 Decachlorobiphenyl

R.T.: 9.128 min
Delta R.T.: -0.004 min
Response: 39003
Conc: 1.03 ng/ml m