

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042321\
 Data File : P0077192.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Apr 2021 19:10
 Operator : DD\AJ
 Sample : M2102-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 RO-124037

Manual Integrations
 APPROVED

Ankita
 4/23/2021 4:47:04 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 01:37:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 09:50:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.896	3.891	1825511	1176954	17.274	22.371 #
2) SA Decachlor...	10.863	9.129	1192400	482129	11.485	12.777
Target Compounds						
31) L7 AR-1260-1	7.903	6.706	67664	51561	12.506	17.272 #
32) L7 AR-1260-2	8.168	6.903	246614	57948	39.056	16.255m#
33) L7 AR-1260-3	8.534	7.055	82221	49024	20.143	14.909m#
34) L7 AR-1260-4	8.764	7.535	80410	45964	16.622	19.515
35) L7 AR-1260-5	9.085	7.783	153458	117504	16.502	21.889m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042321\
Data File : P0077192.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Apr 2021 19:10
Operator : DD\AJ
Sample : M2102-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
RO-124037


Manual Integrations
APPROVED

Ankita
4/23/2021 4:47:04 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 01:37:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 09:50:22 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

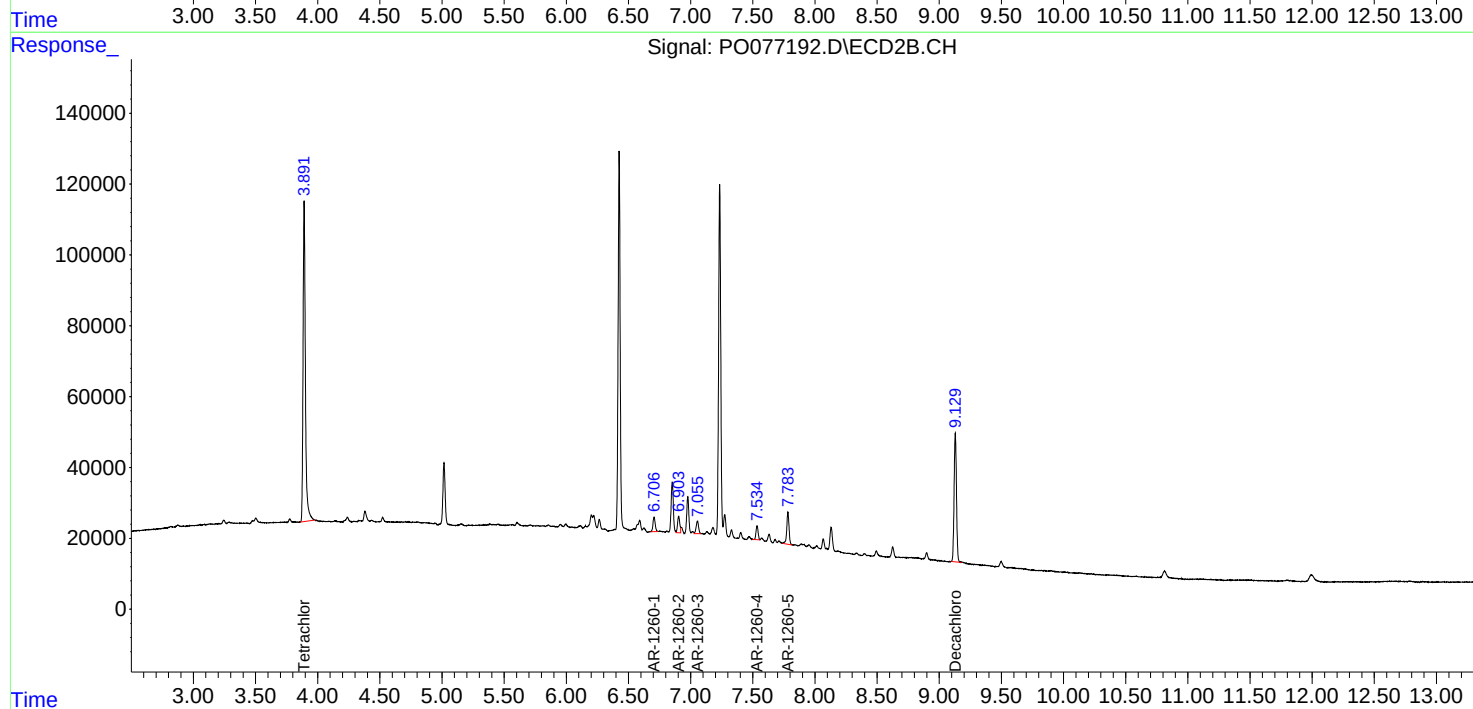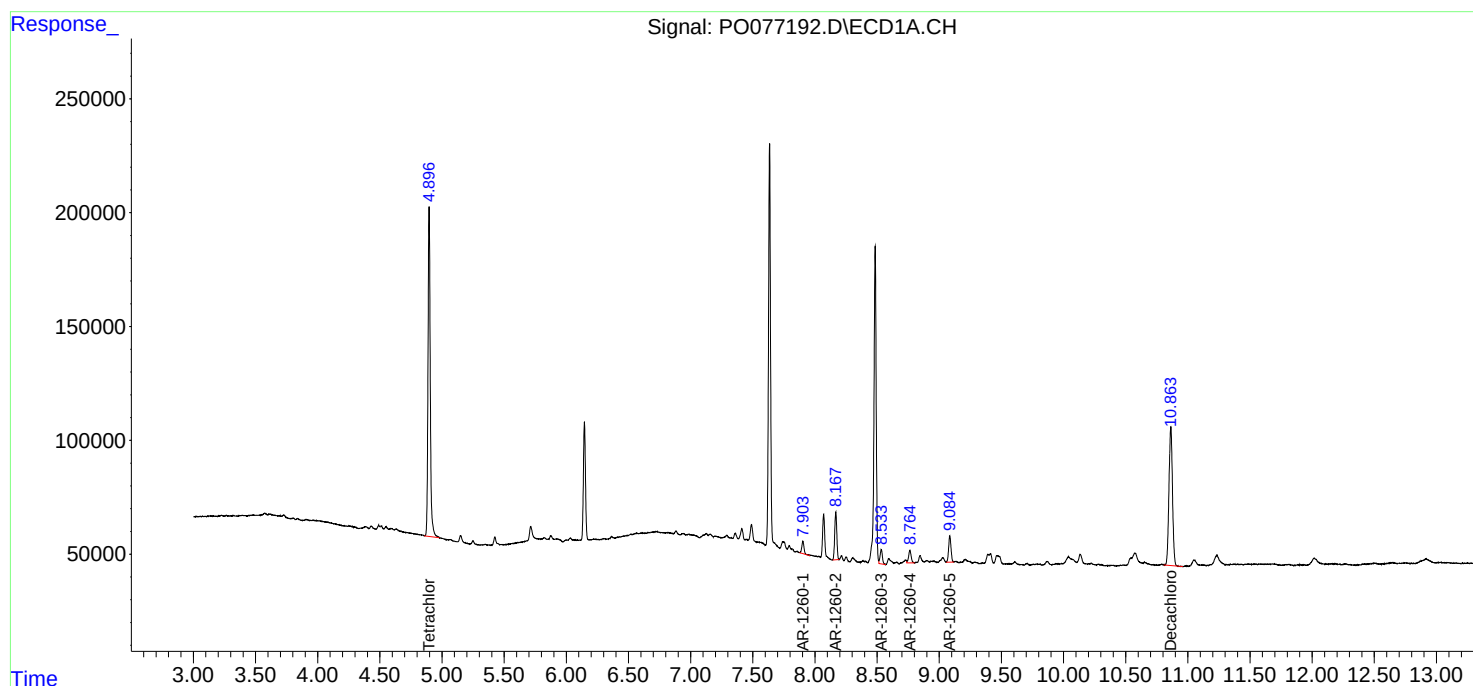

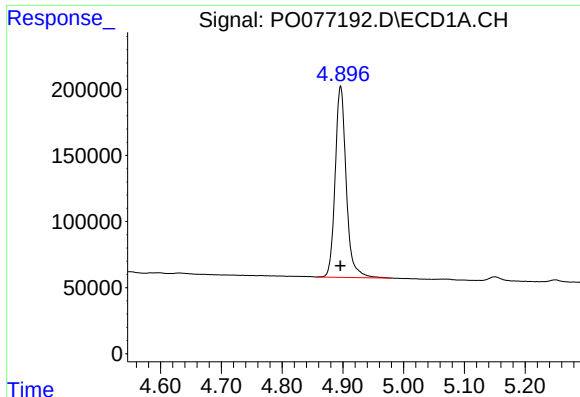


#1 Tetrachloro-m-xylene

R.T.: 4.896 min
Delta R.T.: 0.000 min
Response: 1825511
Conc: 17.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
RO-124037


Manual Integrations
APPROVED

Ankita
4/23/2021 4:47:04 PM

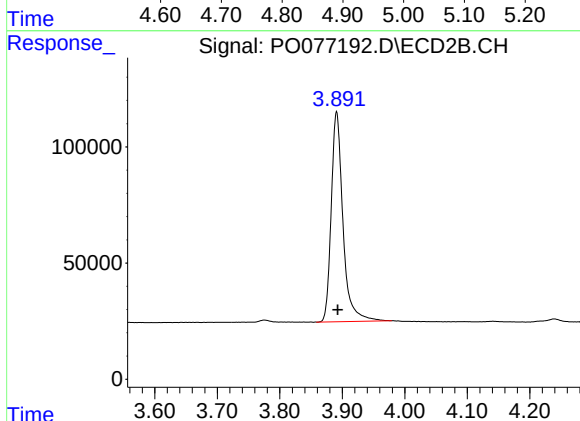


#1 Tetrachloro-m-xylene

R.T.: 3.891 min
Delta R.T.: -0.002 min
Response: 1176954
Conc: 22.37 ng/ml

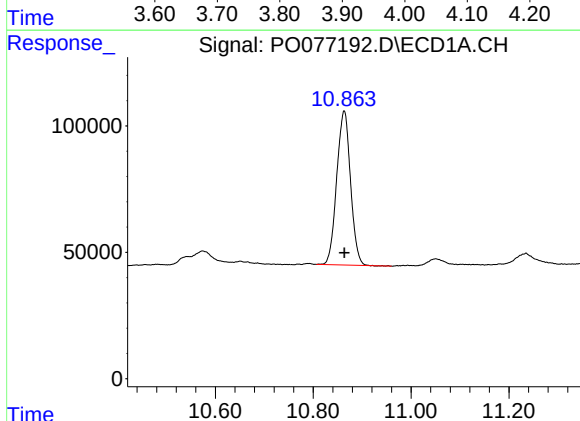


#2 Decachlorobiphenyl

R.T.: 10.863 min
Delta R.T.: 0.000 min
Response: 1192400
Conc: 11.48 ng/ml

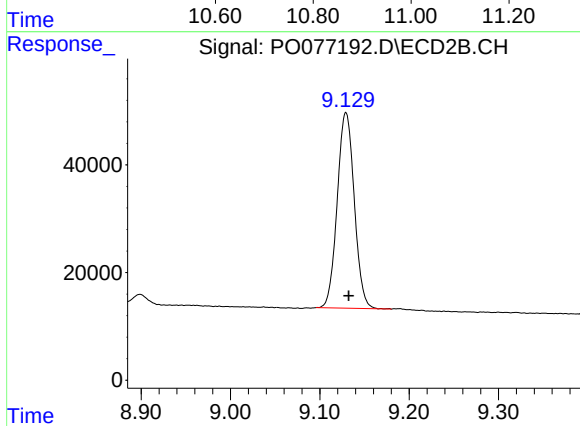

#2 Decachlorobiphenyl

R.T.: 9.129 min
Delta R.T.: -0.003 min
Response: 482129
Conc: 12.78 ng/ml

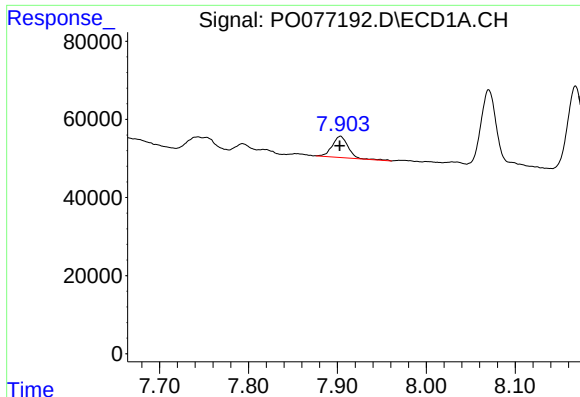


#31 AR-1260-1

R.T.: 7.903 min
Delta R.T.: 0.000 min
Response: 67664
Conc: 12.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
RO-124037


Manual Integrations
APPROVED

Ankita
4/23/2021 4:47:04 PM

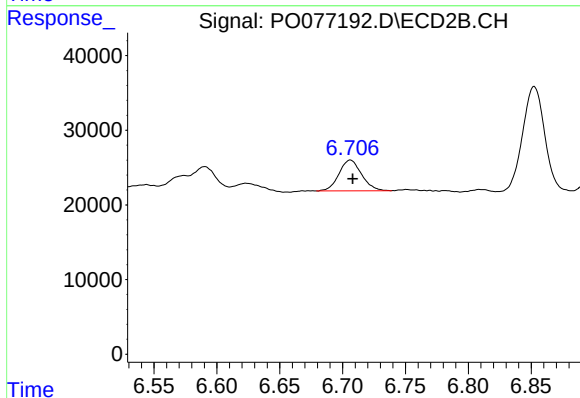


#31 AR-1260-1

R.T.: 6.706 min
Delta R.T.: -0.002 min
Response: 51561
Conc: 17.27 ng/ml

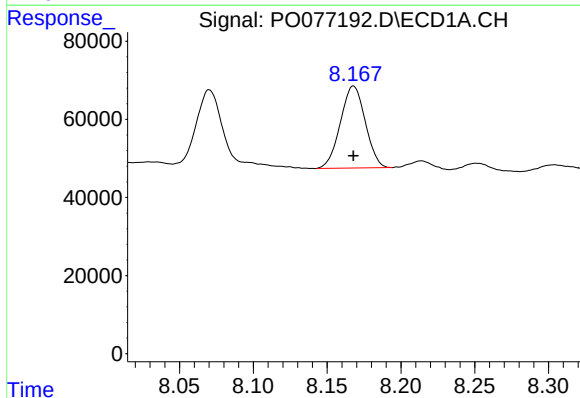


#32 AR-1260-2

R.T.: 8.168 min
Delta R.T.: 0.000 min
Response: 246614
Conc: 39.06 ng/ml

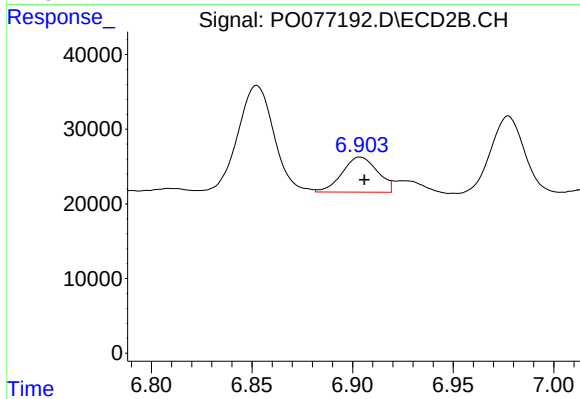

#32 AR-1260-2

R.T.: 6.903 min
Delta R.T.: -0.003 min
Response: 57948
Conc: 16.25 ng/ml m

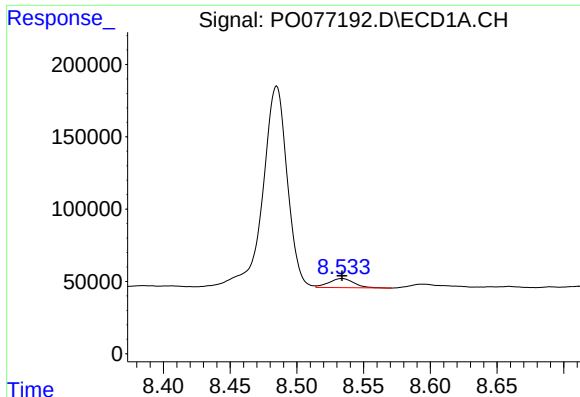


#33 AR-1260-3

R.T.: 8.534 min
Delta R.T.: 0.000 min
Response: 82221
Conc: 20.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
RO-124037


Manual Integrations
APPROVED

Ankita
4/23/2021 4:47:04 PM

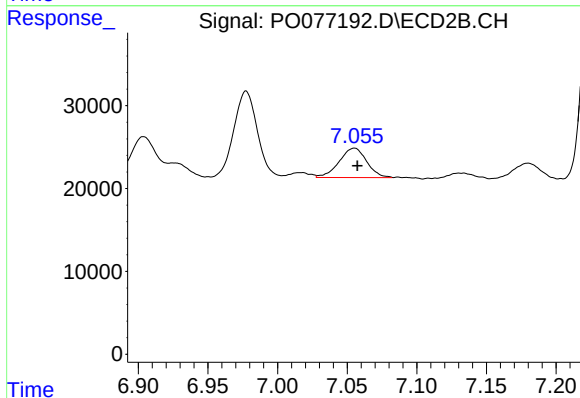


#33 AR-1260-3

R.T.: 7.055 min
Delta R.T.: -0.002 min
Response: 49024
Conc: 14.91 ng/ml m

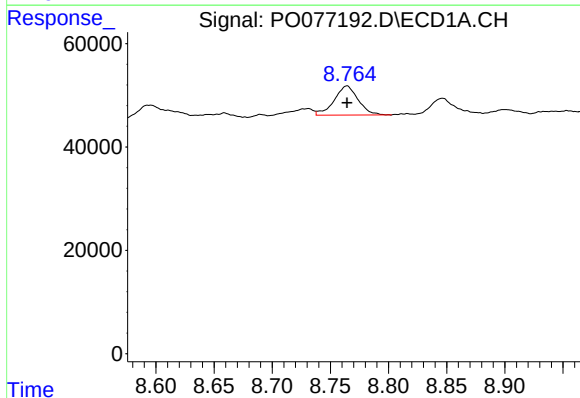


#34 AR-1260-4

R.T.: 8.764 min
Delta R.T.: 0.000 min
Response: 80410
Conc: 16.62 ng/ml

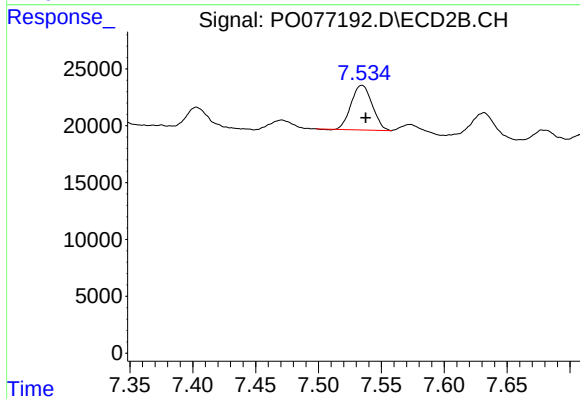

#34 AR-1260-4

R.T.: 7.535 min
Delta R.T.: -0.003 min
Response: 45964
Conc: 19.52 ng/ml

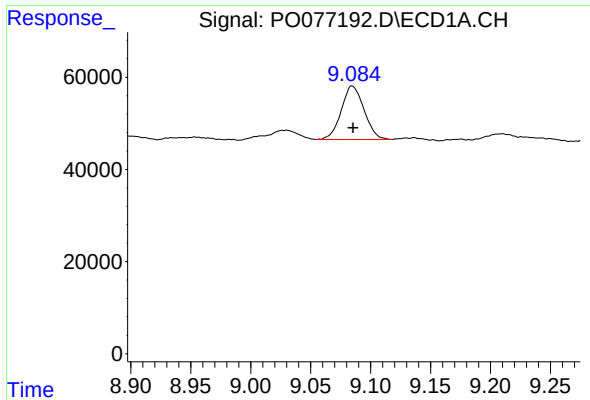


#35 AR-1260-5

R.T.: 9.085 min
Delta R.T.: 0.000 min
Response: 153458
Conc: 16.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
RO-124037

Manual Integrations
APPROVED

Ankita
4/23/2021 4:47:04 PM

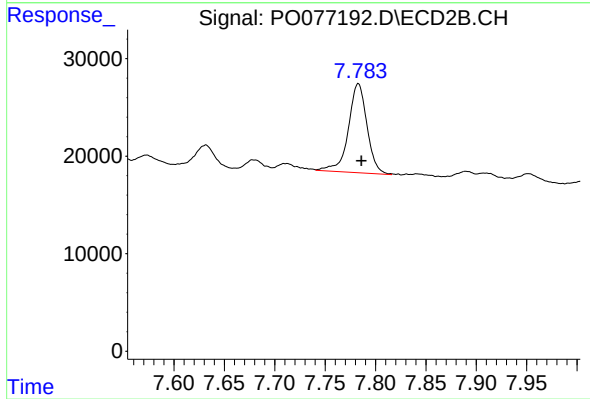

#35 AR-1260-5

R.T.: 7.783 min
Delta R.T.: -0.003 min
Response: 117504
Conc: 21.89 ng/ml m