

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042321\
 Data File : P0077199.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Apr 2021 22:19
 Operator : DD\AJ
 Sample : M2099-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-1

Manual Integrations
 APPROVED

Ankita
 4/23/2021 4:46:32 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 01:39:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 09:50:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.894	3.889	2060435	924344	19.497	17.569
2) SA Decachlor...	10.860	9.129	1737801	616521	16.738	16.339
Target Compounds						
31) L7 AR-1260-1	7.903	6.705	463577	324667	85.678	108.754 #
32) L7 AR-1260-2	8.167	6.903	859009	389232	136.040	109.181
33) L7 AR-1260-3	8.533	7.055	563792	336321	138.123	102.278 #
34) L7 AR-1260-4	8.763	7.534	671965	325908	138.905	138.372
35) L7 AR-1260-5	9.085	7.784	1237258	736829	133.051	137.261

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042321\
Data File : P0077199.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Apr 2021 22:19
Operator : DD\AJ
Sample : M2099-01
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
TP-1


Manual Integrations
APPROVED

Ankita
4/23/2021 4:46:32 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 01:39:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 09:50:22 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

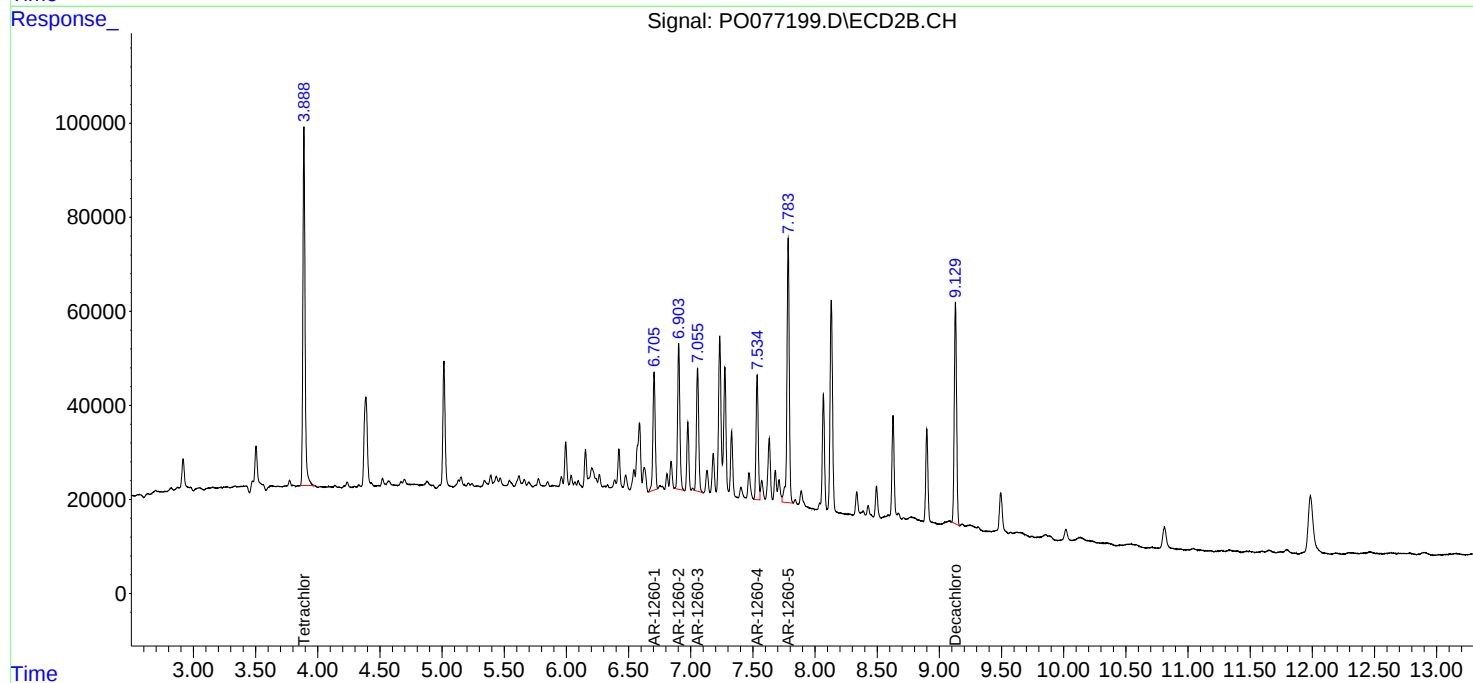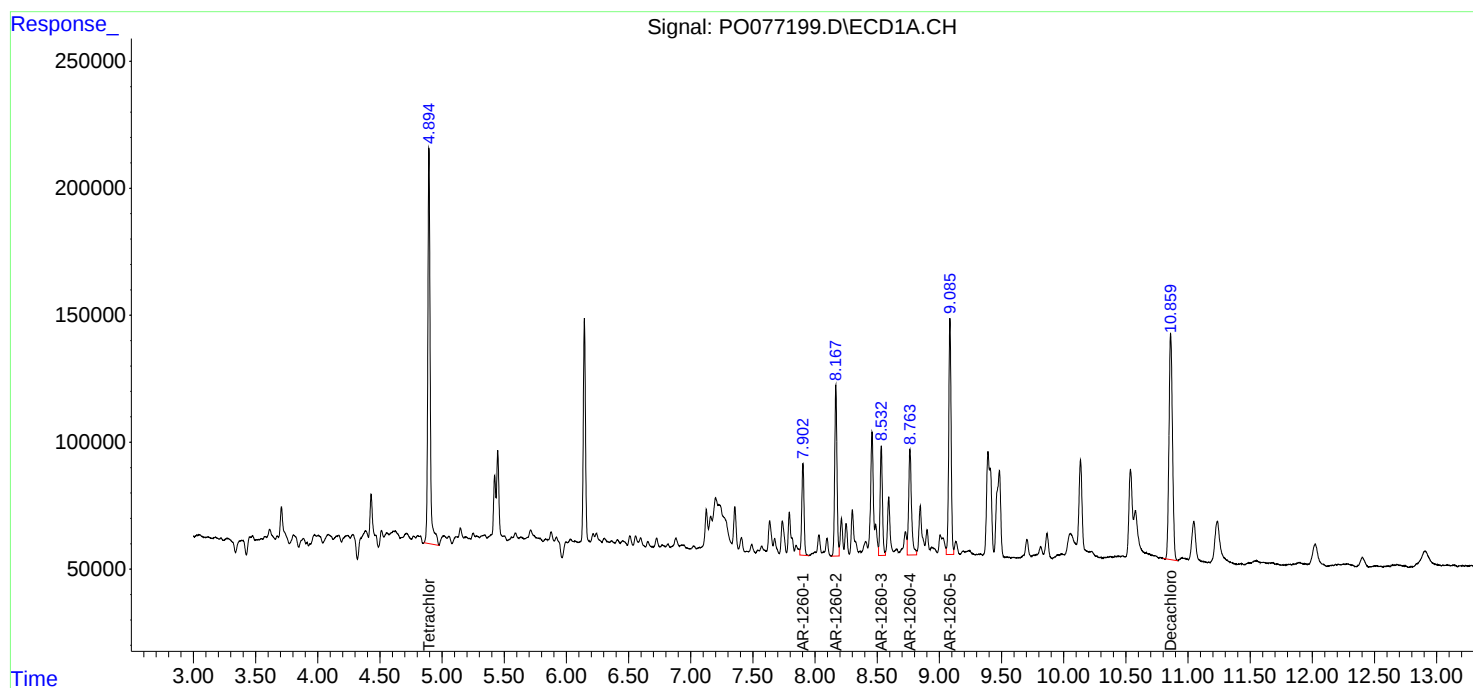

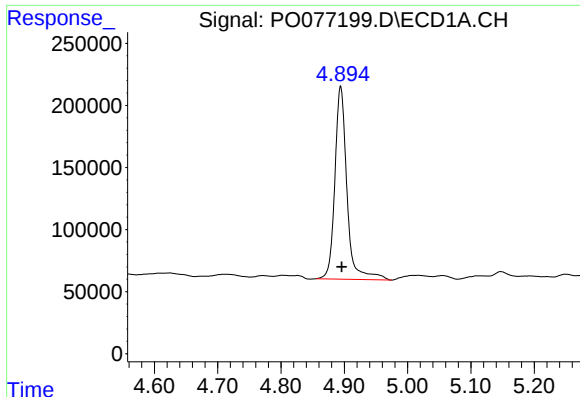


#1 Tetrachloro-m-xylene

R.T.: 4.894 min
Delta R.T.: -0.002 min
Response: 2060435
Conc: 19.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-1


Manual Integrations
APPROVED

Ankita
4/23/2021 4:46:32 PM

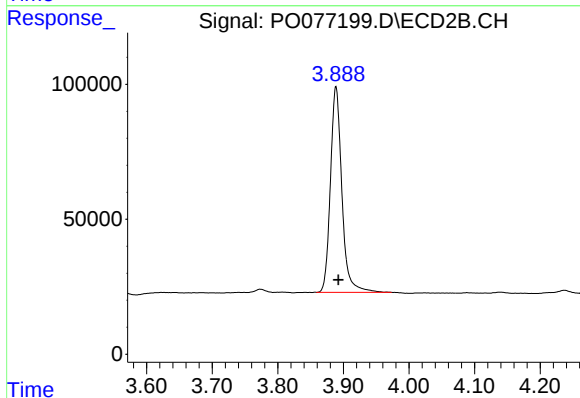


#1 Tetrachloro-m-xylene

R.T.: 3.889 min
Delta R.T.: -0.004 min
Response: 924344
Conc: 17.57 ng/ml

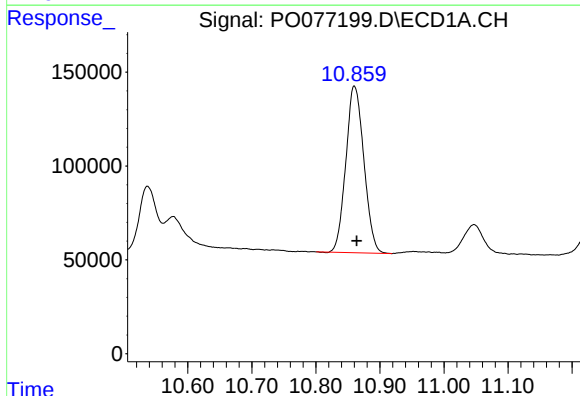


#2 Decachlorobiphenyl

R.T.: 10.860 min
Delta R.T.: -0.004 min
Response: 1737801
Conc: 16.74 ng/ml

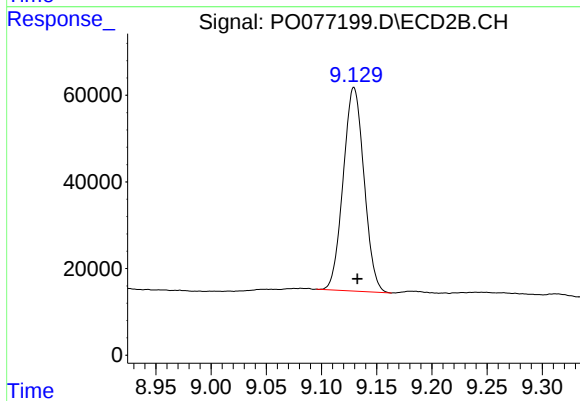

#2 Decachlorobiphenyl

R.T.: 9.129 min
Delta R.T.: -0.003 min
Response: 616521
Conc: 16.34 ng/ml

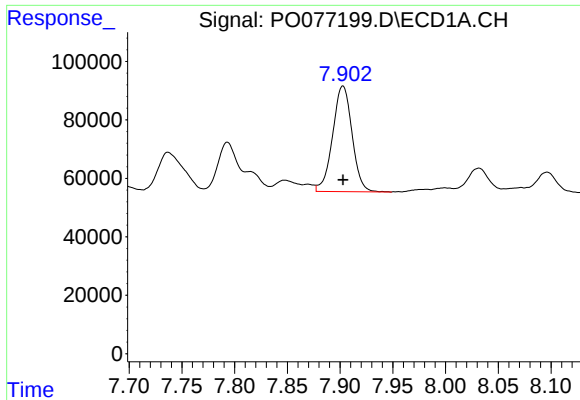


#31 AR-1260-1

R.T.: 7.903 min
Delta R.T.: 0.000 min
Response: 463577
Conc: 85.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-1


Manual Integrations
APPROVED

Ankita
4/23/2021 4:46:32 PM

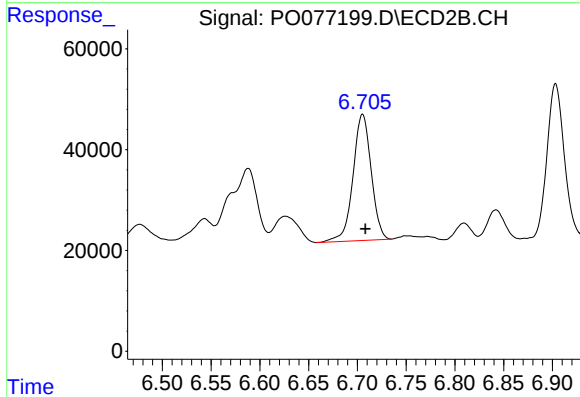


#31 AR-1260-1

R.T.: 6.705 min
Delta R.T.: -0.003 min
Response: 324667
Conc: 108.75 ng/ml

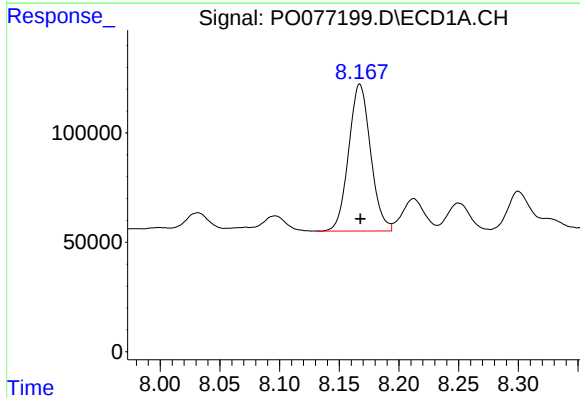


#32 AR-1260-2

R.T.: 8.167 min
Delta R.T.: 0.000 min
Response: 859009
Conc: 136.04 ng/ml

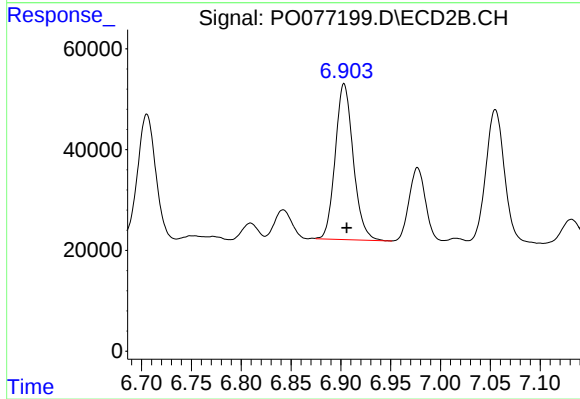

#32 AR-1260-2

R.T.: 6.903 min
Delta R.T.: -0.003 min
Response: 389232
Conc: 109.18 ng/ml

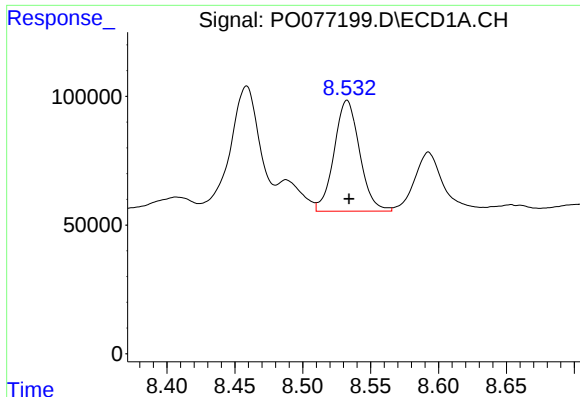


#33 AR-1260-3

R.T.: 8.533 min
Delta R.T.: -0.001 min
Response: 563792
Conc: 138.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-1


Manual Integrations
APPROVED

Ankita
4/23/2021 4:46:32 PM

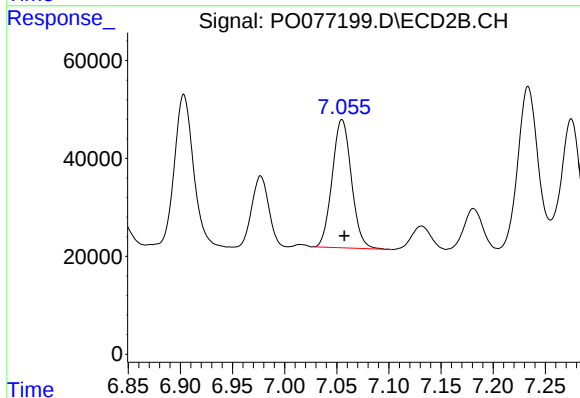


#33 AR-1260-3

R.T.: 7.055 min
Delta R.T.: -0.002 min
Response: 336321
Conc: 102.28 ng/ml

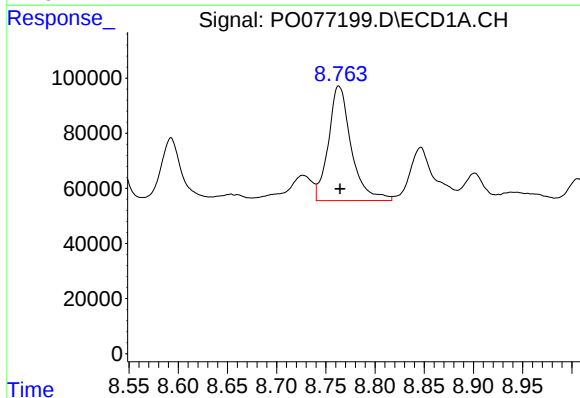


#34 AR-1260-4

R.T.: 8.763 min
Delta R.T.: -0.001 min
Response: 671965
Conc: 138.90 ng/ml

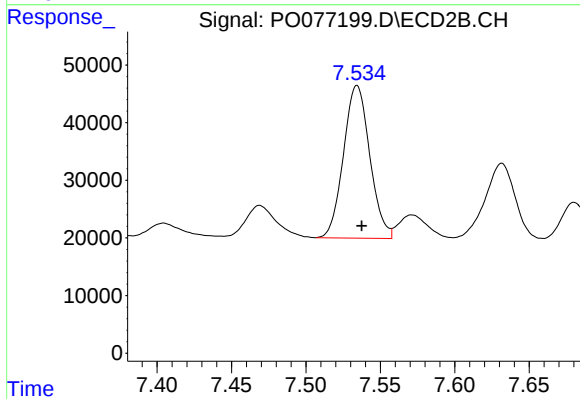

#34 AR-1260-4

R.T.: 7.534 min
Delta R.T.: -0.003 min
Response: 325908
Conc: 138.37 ng/ml

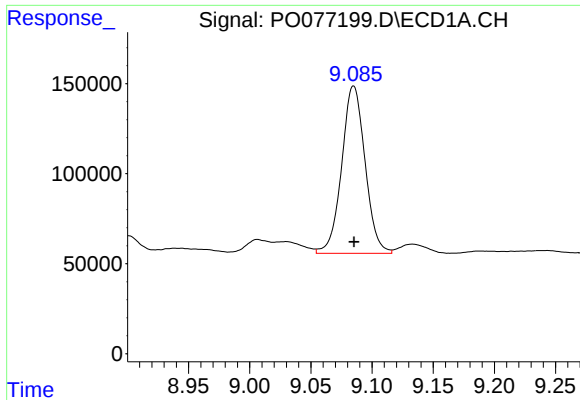


#35 AR-1260-5

R.T.: 9.085 min
Delta R.T.: 0.000 min
Response: 1237258
Conc: 133.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-1

Manual Integrations
APPROVED

Ankita
4/23/2021 4:46:32 PM

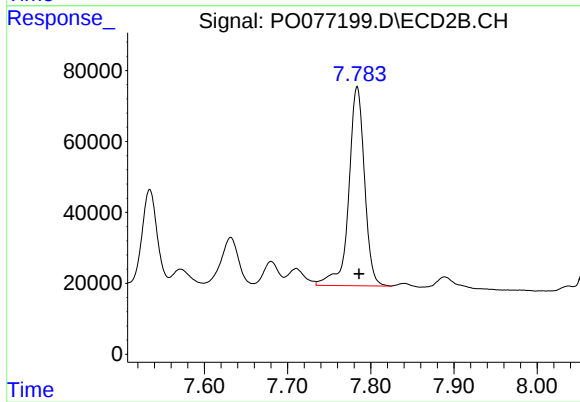

#35 AR-1260-5

R.T.: 7.784 min
Delta R.T.: -0.002 min
Response: 736829
Conc: 137.26 ng/ml