

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042321\
 Data File : P0077200.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Apr 2021 22:36
 Operator : DD\AJ
 Sample : M2099-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-2

Manual Integrations
 APPROVED

Ankita
 4/23/2021 4:46:34 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 01:39:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 09:50:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.895	3.889	2363238	1239244	22.362	23.555
2) SA Decachlor...	10.861	9.128	2255184	780887	21.721	20.695
Target Compounds						
31) L7 AR-1260-1	7.902	6.705	938098	605694	173.380	202.889
32) L7 AR-1260-2	8.167	6.903	1467066	770086	232.337	216.012
33) L7 AR-1260-3	8.532	7.054	970537	623113	237.771	189.494
34) L7 AR-1260-4	8.762	7.534	1075202	570325	222.260	242.145
35) L7 AR-1260-5	9.084	7.783	2238126	1343492	240.681	250.274

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042321\
Data File : P0077200.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Apr 2021 22:36
Operator : DD\AJ
Sample : M2099-03
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
TP-2


Manual Integrations
APPROVED

Ankita
4/23/2021 4:46:34 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 01:39:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 09:50:22 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

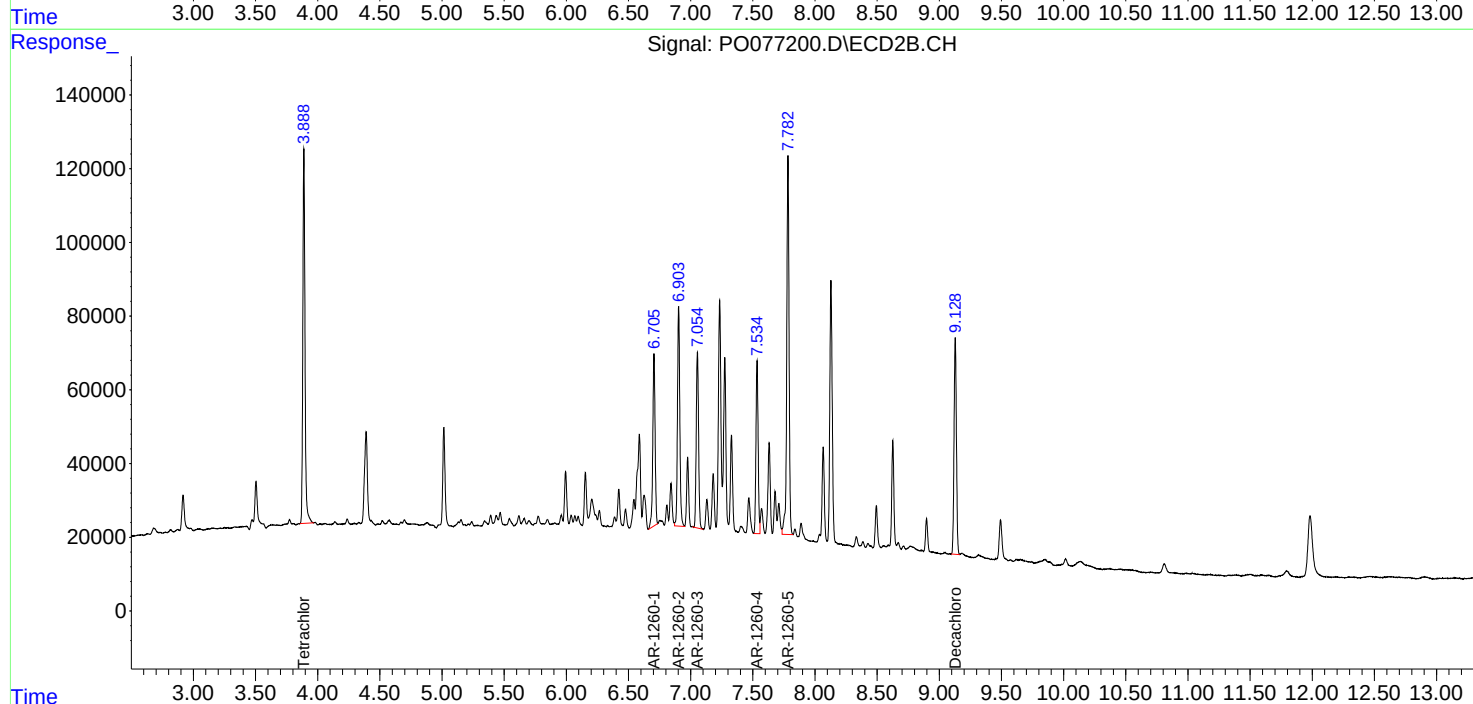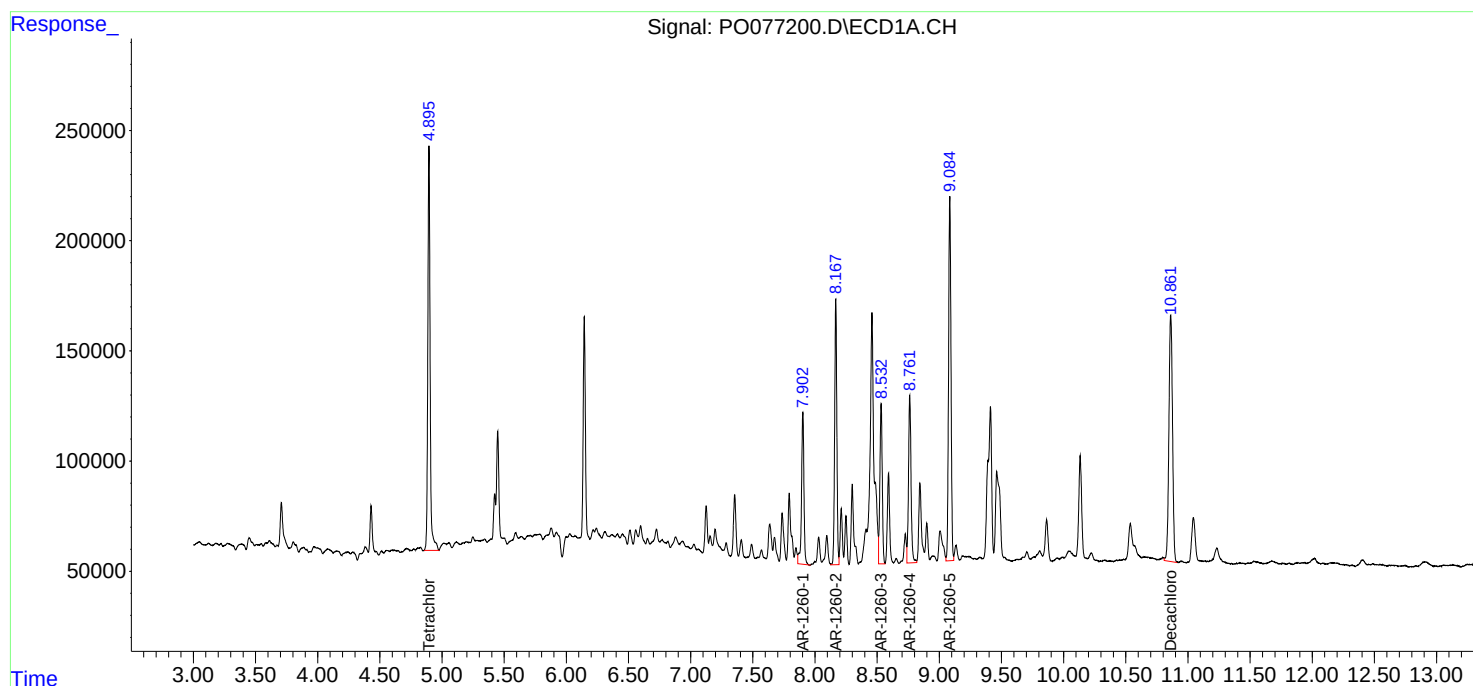

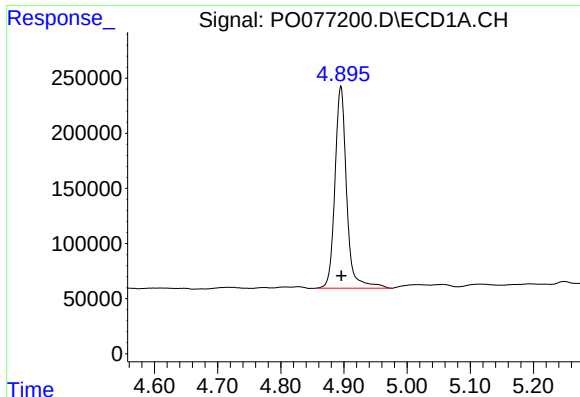


#1 Tetrachloro-m-xylene

R.T.: 4.895 min
Delta R.T.: 0.000 min
Response: 2363238
Conc: 22.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-2


Manual Integrations
APPROVED

Ankita
4/23/2021 4:46:34 PM

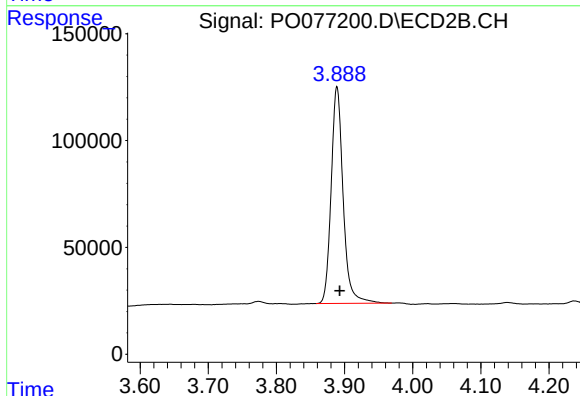


#1 Tetrachloro-m-xylene

R.T.: 3.889 min
Delta R.T.: -0.004 min
Response: 1239244
Conc: 23.55 ng/ml

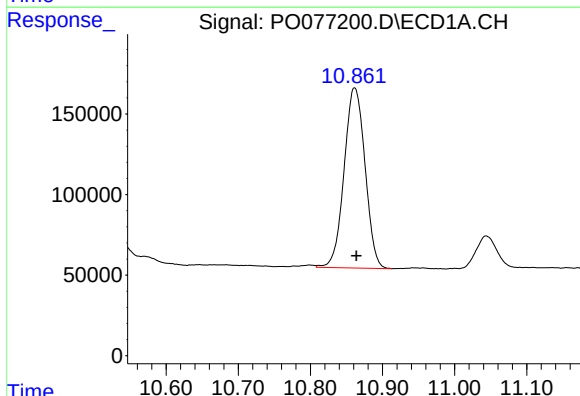


#2 Decachlorobiphenyl

R.T.: 10.861 min
Delta R.T.: -0.002 min
Response: 2255184
Conc: 21.72 ng/ml

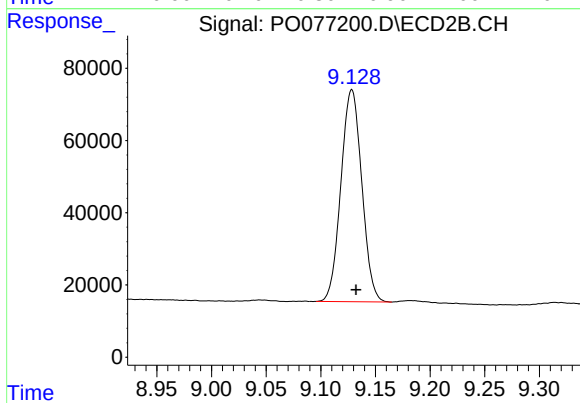

#2 Decachlorobiphenyl

R.T.: 9.128 min
Delta R.T.: -0.004 min
Response: 780887
Conc: 20.69 ng/ml

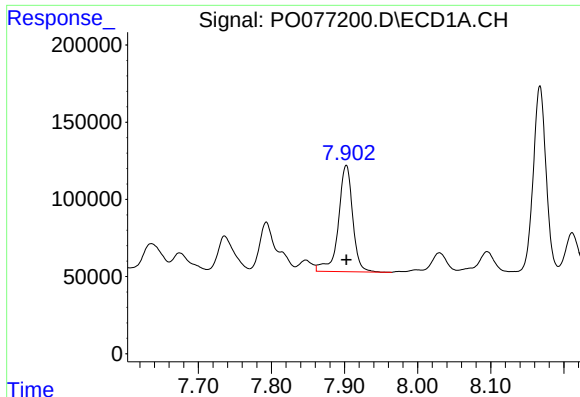


#31 AR-1260-1

R.T.: 7.902 min
Delta R.T.: 0.000 min
Response: 938098
Conc: 173.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-2


Manual Integrations
APPROVED

Ankita
4/23/2021 4:46:34 PM

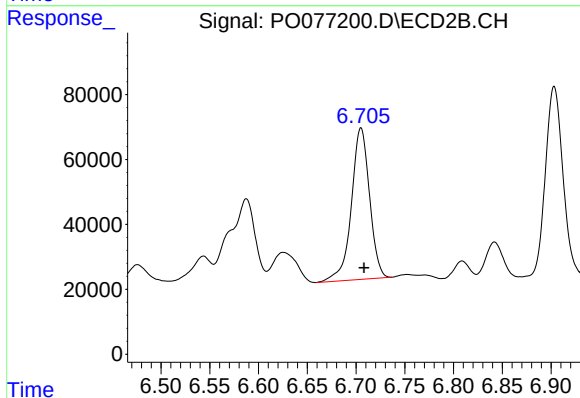


#31 AR-1260-1

R.T.: 6.705 min
Delta R.T.: -0.003 min
Response: 605694
Conc: 202.89 ng/ml

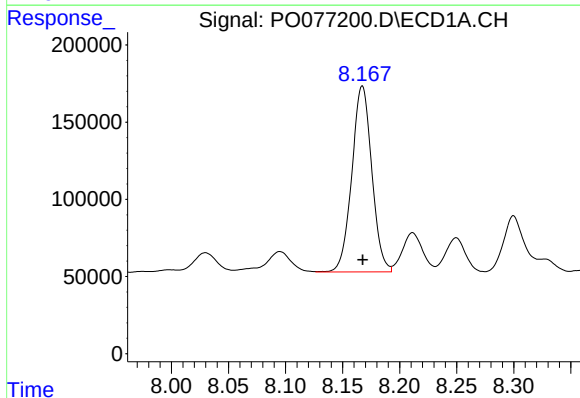


#32 AR-1260-2

R.T.: 8.167 min
Delta R.T.: 0.000 min
Response: 1467066
Conc: 232.34 ng/ml

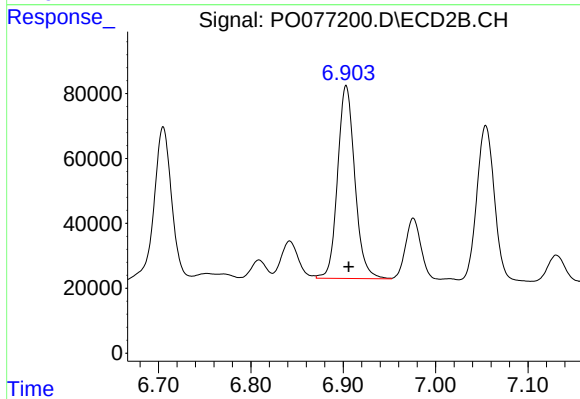

#32 AR-1260-2

R.T.: 6.903 min
Delta R.T.: -0.003 min
Response: 770086
Conc: 216.01 ng/ml

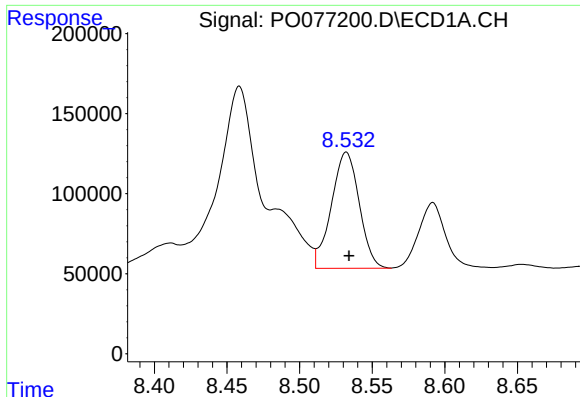


#33 AR-1260-3

R.T.: 8.532 min
Delta R.T.: -0.002 min
Response: 970537
Conc: 237.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-2


Manual Integrations
APPROVED

Ankita
4/23/2021 4:46:34 PM

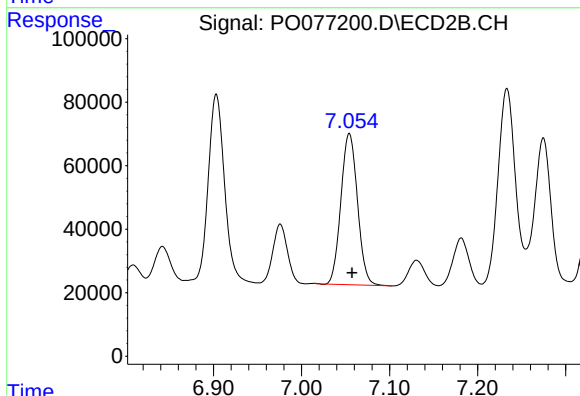


#33 AR-1260-3

R.T.: 7.054 min
Delta R.T.: -0.003 min
Response: 623113
Conc: 189.49 ng/ml

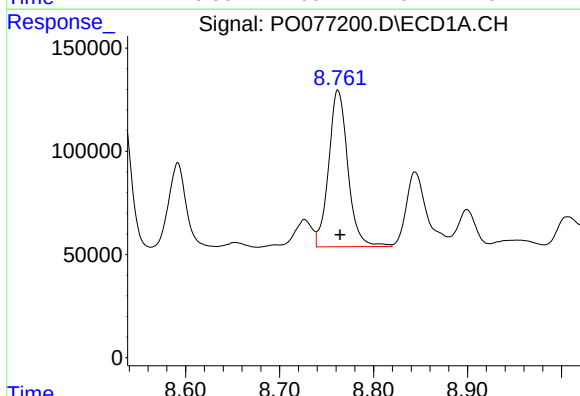


#34 AR-1260-4

R.T.: 8.762 min
Delta R.T.: -0.002 min
Response: 1075202
Conc: 222.26 ng/ml

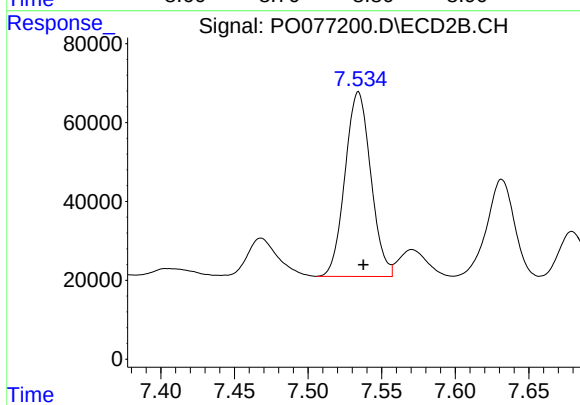

#34 AR-1260-4

R.T.: 7.534 min
Delta R.T.: -0.003 min
Response: 570325
Conc: 242.14 ng/ml

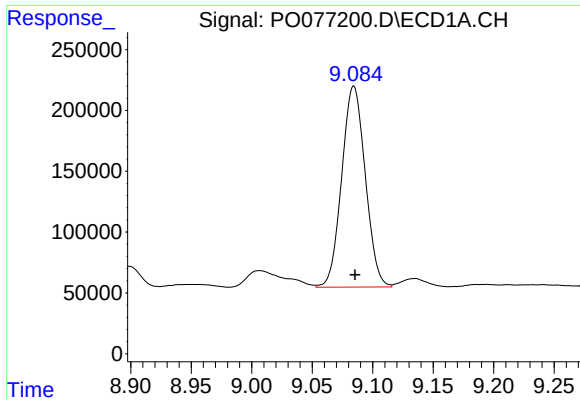


#35 AR-1260-5

R.T.: 9.084 min
Delta R.T.: -0.001 min
Response: 2238126
Conc: 240.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-2

Manual Integrations
APPROVED

Ankita
4/23/2021 4:46:34 PM

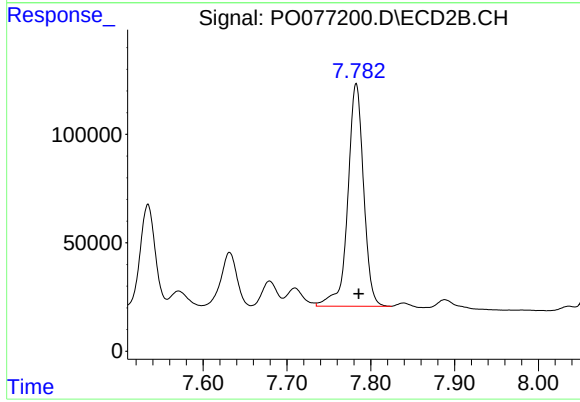

#35 AR-1260-5

R.T.: 7.783 min
Delta R.T.: -0.003 min
Response: 1343492
Conc: 250.27 ng/ml