

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042321\
 Data File : P0077201.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Apr 2021 22:53
 Operator : DD\AJ
 Sample : M2099-05
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-3

Manual Integrations
 APPROVED

Ankita
 4/23/2021 4:46:36 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 01:40:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 09:50:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.895	3.890	1718583	937515	16.262	17.820
2) SA Decachlor...	10.861	9.128	1585652	572265	15.273	15.166
Target Compounds						
31) L7 AR-1260-1	7.902	6.705	712537	456435	131.691	152.892
32) L7 AR-1260-2	8.167	6.903	1116741	595037	176.857	166.910
33) L7 AR-1260-3	8.532	7.054	690599	487991	169.189	148.402
34) L7 AR-1260-4	8.763	7.534	709996	388924	146.767	165.127
35) L7 AR-1260-5	9.085	7.783	1502317	917891	161.555	170.990

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042321\
Data File : P0077201.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Apr 2021 22:53
Operator : DD\AJ
Sample : M2099-05
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
TP-3


Manual Integrations
APPROVED

Ankita
4/23/2021 4:46:36 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 01:40:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 09:50:22 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

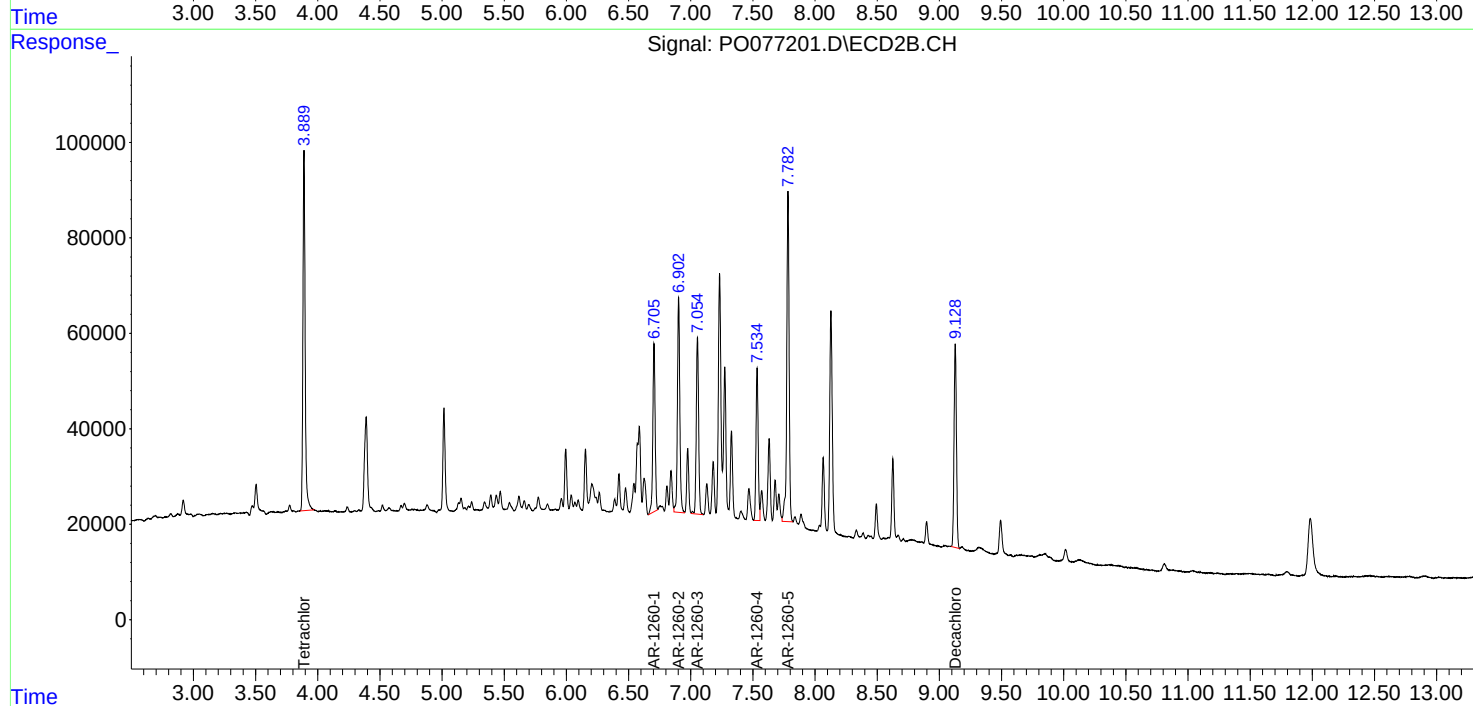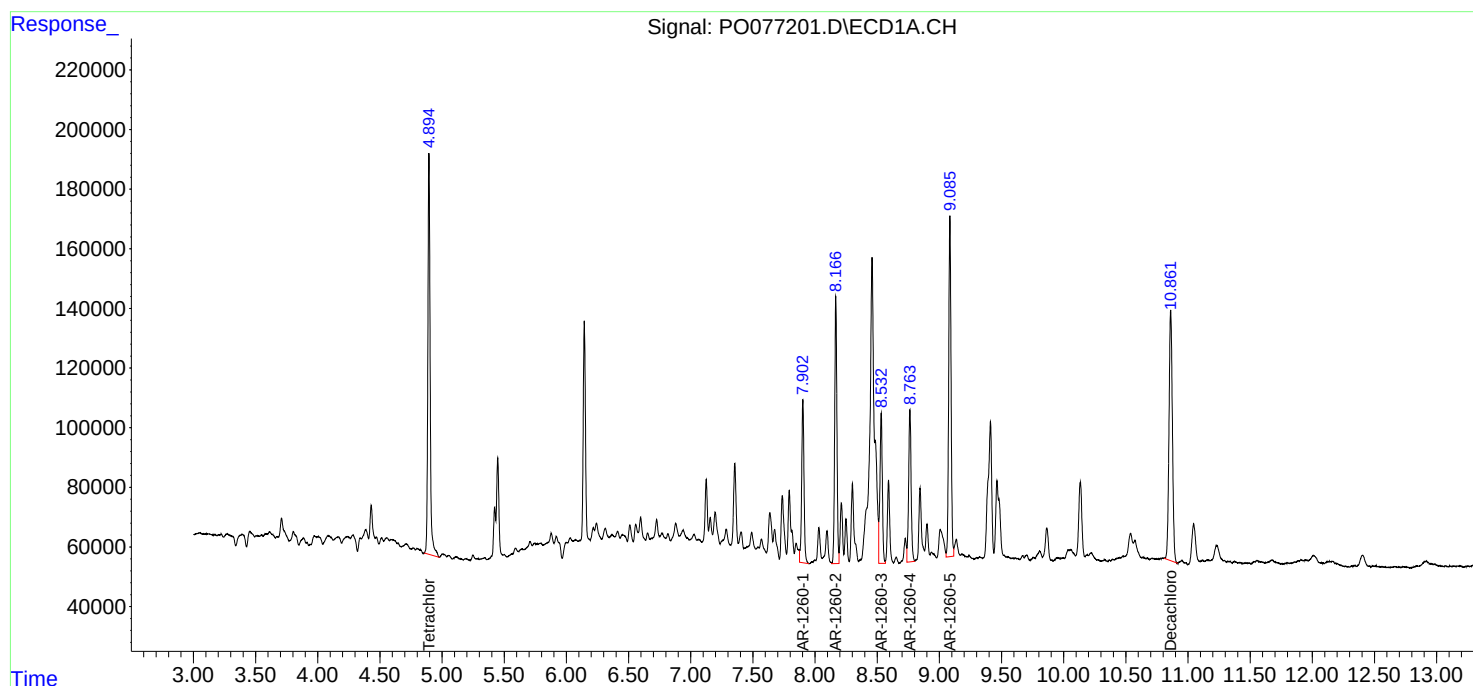

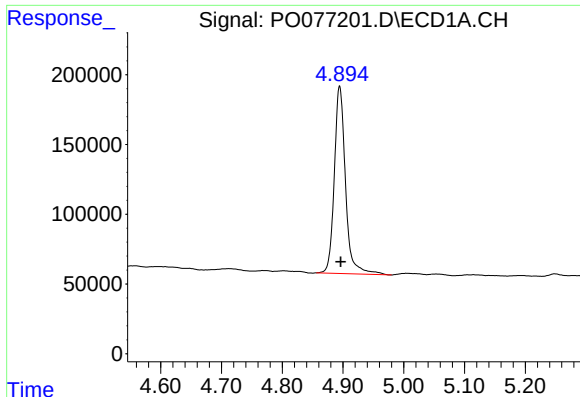


#1 Tetrachloro-m-xylene

R.T.: 4.895 min
Delta R.T.: -0.001 min
Response: 1718583
Conc: 16.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-3


Manual Integrations
APPROVED

Ankita
4/23/2021 4:46:36 PM

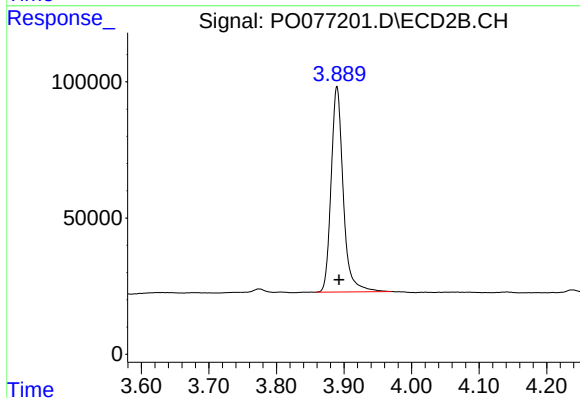


#1 Tetrachloro-m-xylene

R.T.: 3.890 min
Delta R.T.: -0.003 min
Response: 937515
Conc: 17.82 ng/ml

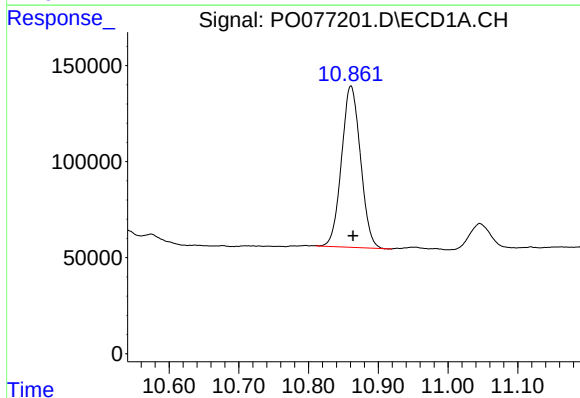


#2 Decachlorobiphenyl

R.T.: 10.861 min
Delta R.T.: -0.003 min
Response: 1585652
Conc: 15.27 ng/ml

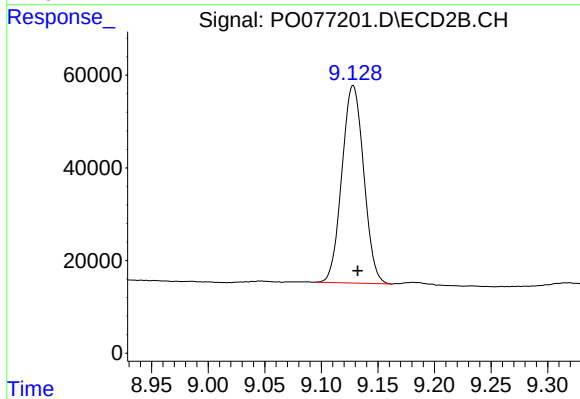

#2 Decachlorobiphenyl

R.T.: 9.128 min
Delta R.T.: -0.004 min
Response: 572265
Conc: 15.17 ng/ml

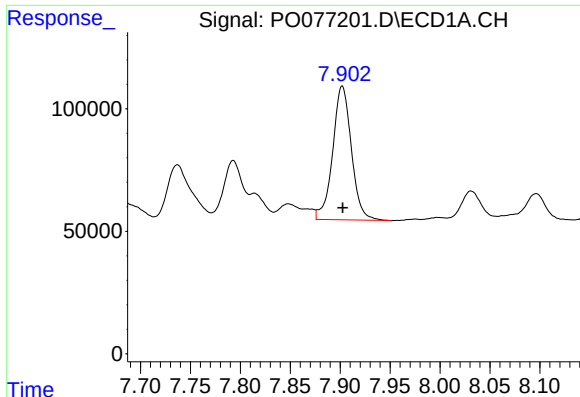


#31 AR-1260-1

R.T.: 7.902 min
Delta R.T.: 0.000 min
Response: 712537
Conc: 131.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-3


Manual Integrations
APPROVED

Ankita
4/23/2021 4:46:36 PM

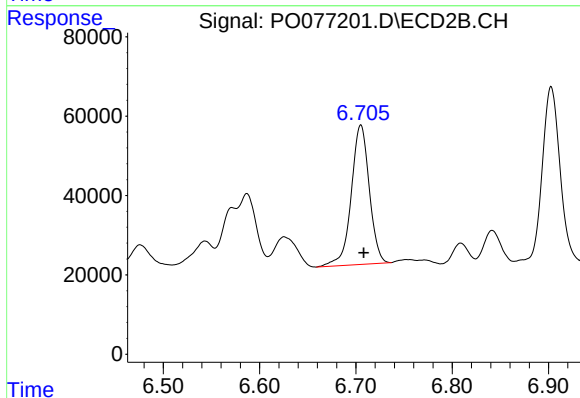


#31 AR-1260-1

R.T.: 6.705 min
Delta R.T.: -0.003 min
Response: 456435
Conc: 152.89 ng/ml

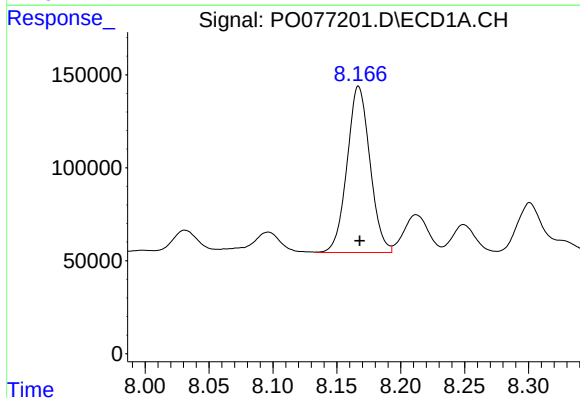


#32 AR-1260-2

R.T.: 8.167 min
Delta R.T.: 0.000 min
Response: 1116741
Conc: 176.86 ng/ml

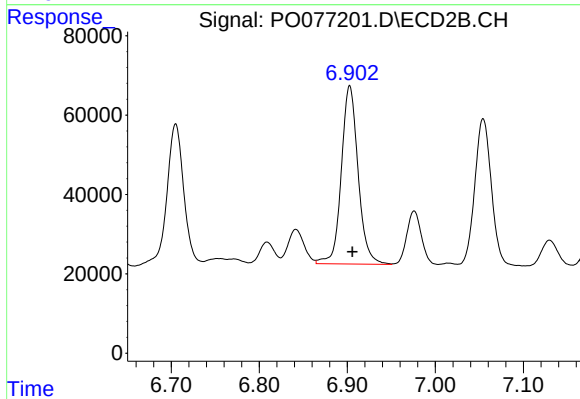

#32 AR-1260-2

R.T.: 6.903 min
Delta R.T.: -0.003 min
Response: 595037
Conc: 166.91 ng/ml

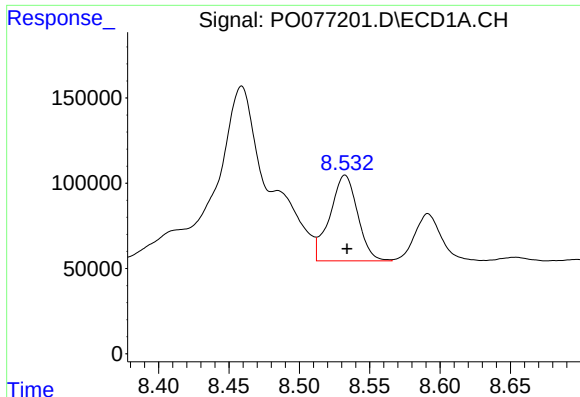


#33 AR-1260-3

R.T.: 8.532 min
Delta R.T.: -0.002 min
Response: 690599
Conc: 169.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-3


Manual Integrations
APPROVED

Ankita
4/23/2021 4:46:36 PM

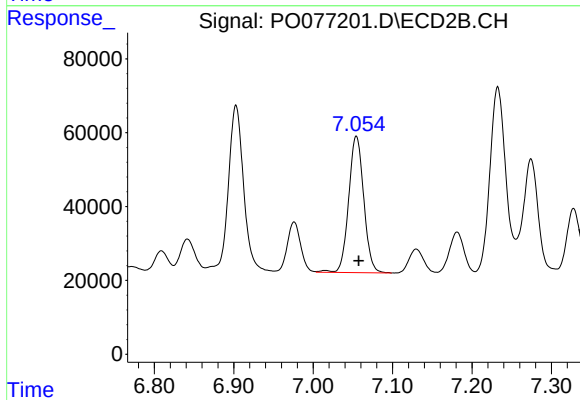


#33 AR-1260-3

R.T.: 7.054 min
Delta R.T.: -0.003 min
Response: 487991
Conc: 148.40 ng/ml

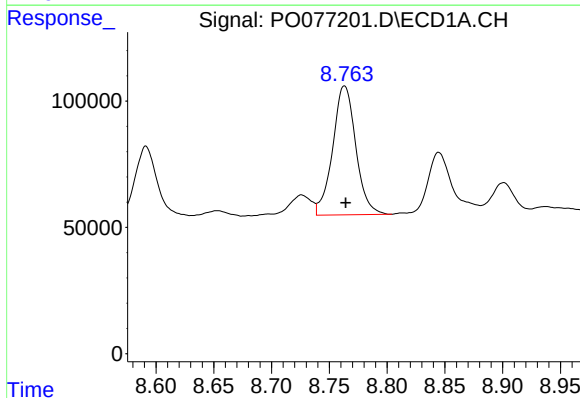


#34 AR-1260-4

R.T.: 8.763 min
Delta R.T.: -0.001 min
Response: 709996
Conc: 146.77 ng/ml

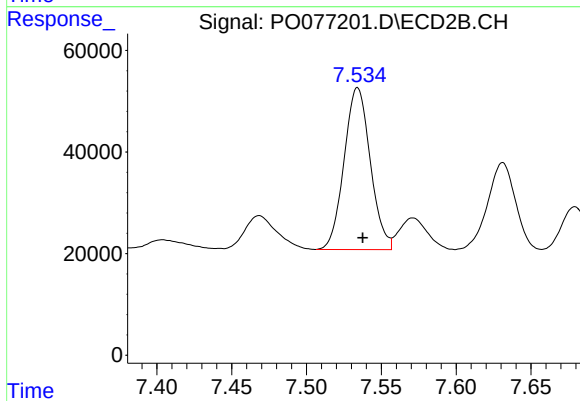

#34 AR-1260-4

R.T.: 7.534 min
Delta R.T.: -0.003 min
Response: 388924
Conc: 165.13 ng/ml

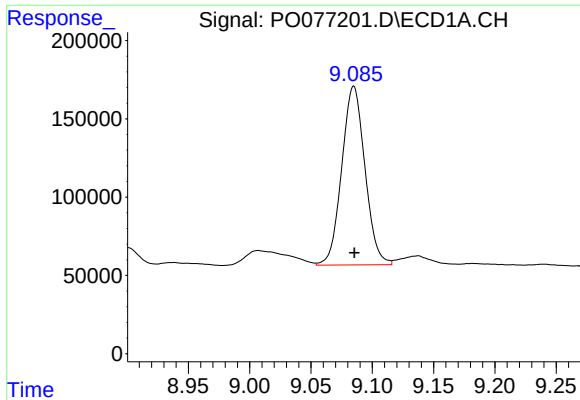


#35 AR-1260-5

R.T.: 9.085 min
Delta R.T.: 0.000 min
Response: 1502317
Conc: 161.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-3

Manual Integrations
APPROVED

Ankita
4/23/2021 4:46:36 PM

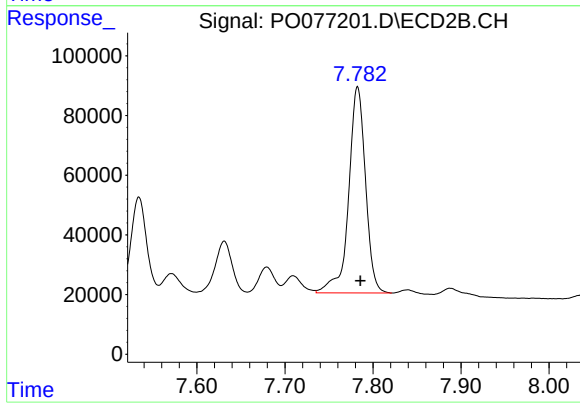

#35 AR-1260-5

R.T.: 7.783 min
Delta R.T.: -0.003 min
Response: 917891
Conc: 170.99 ng/ml