

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042321\
 Data File : P0077202.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Apr 2021 23:11
 Operator : DD\AJ
 Sample : M2099-07
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-4

Manual Integrations
 APPROVED

Ankita
 4/23/2021 4:46:37 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 01:40:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 09:50:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.895	3.889	2128096	1003932	20.137	19.082
2) SA Decachlor...	10.861	9.129	1533797	547282	14.773	14.504
Target Compounds						
31) L7 AR-1260-1	7.903	6.705	214613	144823	39.665	48.512m
32) L7 AR-1260-2	8.169	6.904	538835	186620	85.335	52.348 #
33) L7 AR-1260-3	8.533	7.054	271463	146388	66.505	44.518 #
34) L7 AR-1260-4	8.764	7.535	220911	112983	45.666	47.969
35) L7 AR-1260-5	9.086	7.783	410745	305814	44.170	56.969 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042321\
Data File : P0077202.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Apr 2021 23:11
Operator : DD\AJ
Sample : M2099-07
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
TP-4


Manual Integrations
APPROVED

Ankita
4/23/2021 4:46:37 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 01:40:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 09:50:22 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

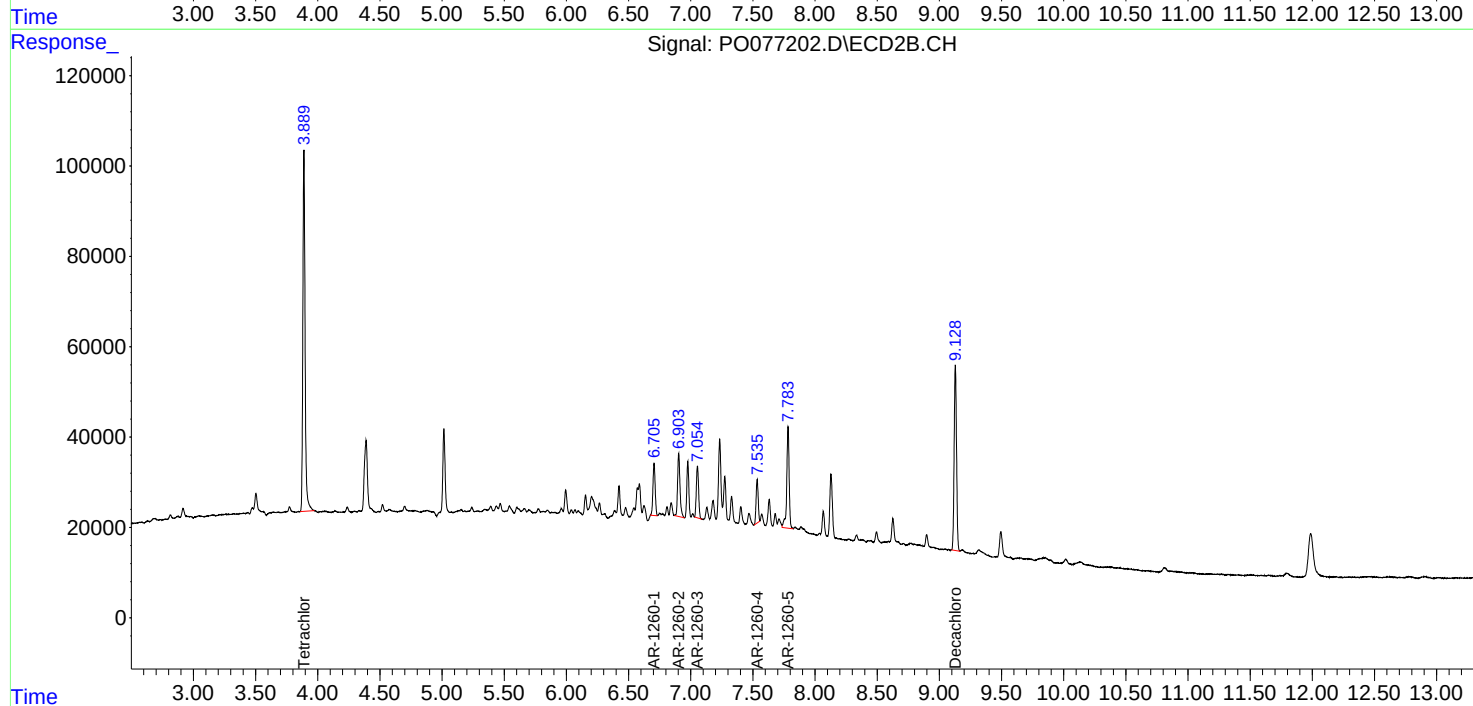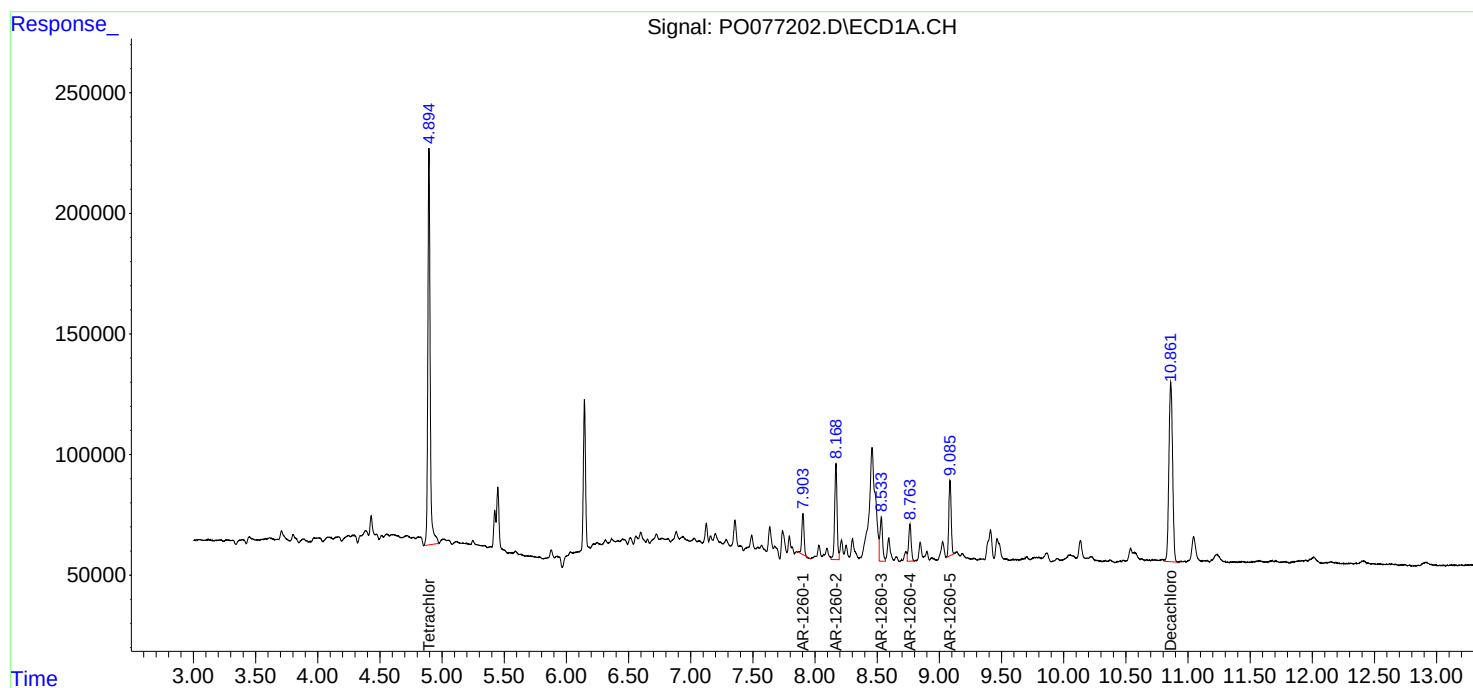

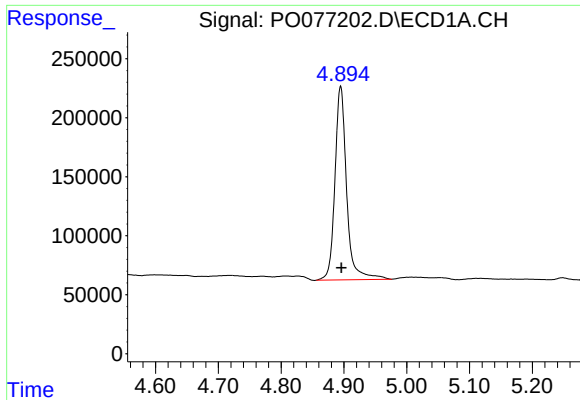


#1 Tetrachloro-m-xylene

R.T.: 4.895 min
Delta R.T.: -0.001 min
Response: 2128096
Conc: 20.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-4


Manual Integrations
APPROVED

Ankita
4/23/2021 4:46:37 PM

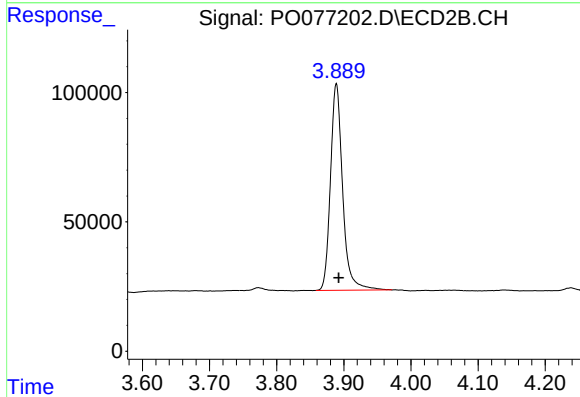


#1 Tetrachloro-m-xylene

R.T.: 3.889 min
Delta R.T.: -0.004 min
Response: 1003932
Conc: 19.08 ng/ml

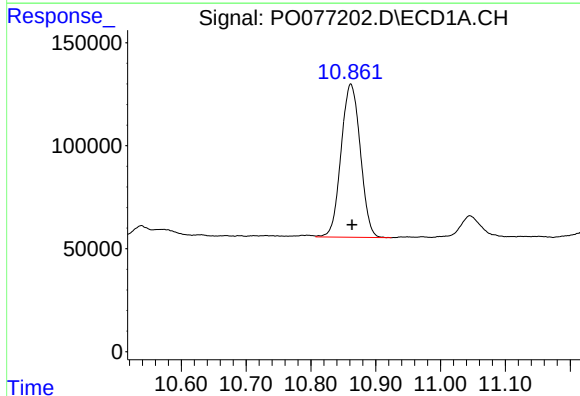


#2 Decachlorobiphenyl

R.T.: 10.861 min
Delta R.T.: -0.002 min
Response: 1533797
Conc: 14.77 ng/ml

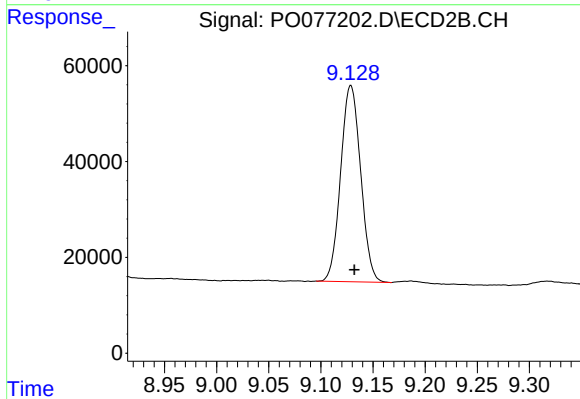

#2 Decachlorobiphenyl

R.T.: 9.129 min
Delta R.T.: -0.004 min
Response: 547282
Conc: 14.50 ng/ml

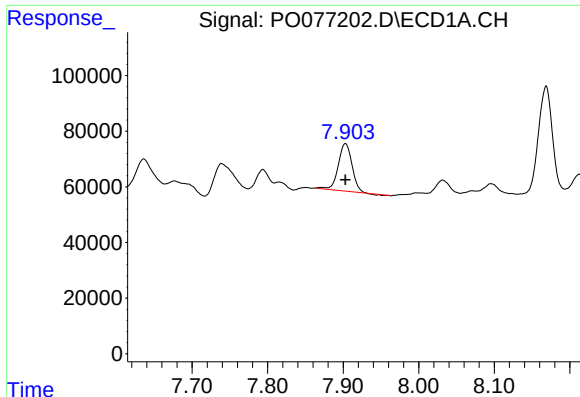


#31 AR-1260-1

R.T.: 7.903 min
Delta R.T.: 0.000 min
Response: 214613
Conc: 39.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-4


Manual Integrations
APPROVED

Ankita
4/23/2021 4:46:37 PM

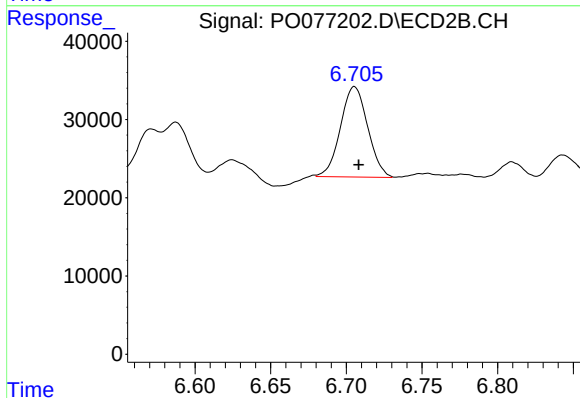


#31 AR-1260-1

R.T.: 6.705 min
Delta R.T.: -0.003 min
Response: 144823
Conc: 48.51 ng/ml m

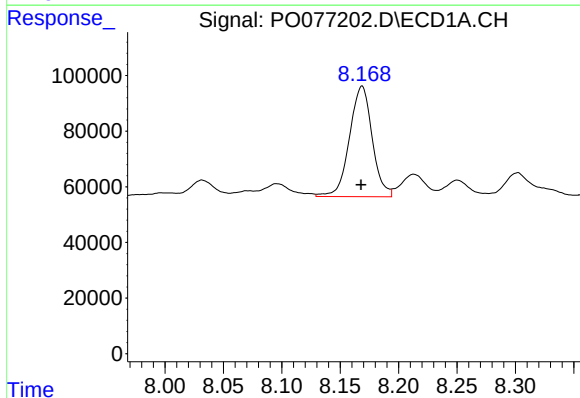


#32 AR-1260-2

R.T.: 8.169 min
Delta R.T.: 0.000 min
Response: 538835
Conc: 85.33 ng/ml

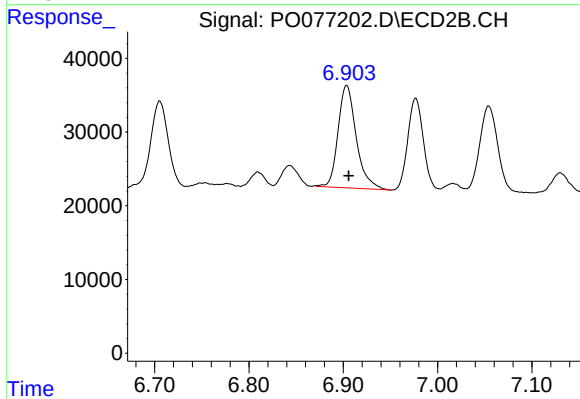

#32 AR-1260-2

R.T.: 6.904 min
Delta R.T.: -0.002 min
Response: 186620
Conc: 52.35 ng/ml

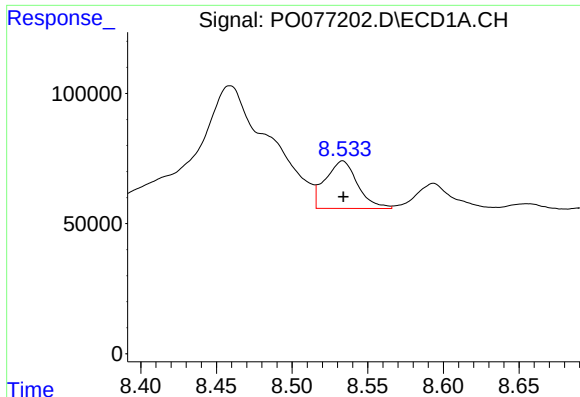


#33 AR-1260-3

R.T.: 8.533 min
Delta R.T.: 0.000 min
Response: 271463
Conc: 66.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-4


Manual Integrations
APPROVED

Ankita
4/23/2021 4:46:37 PM

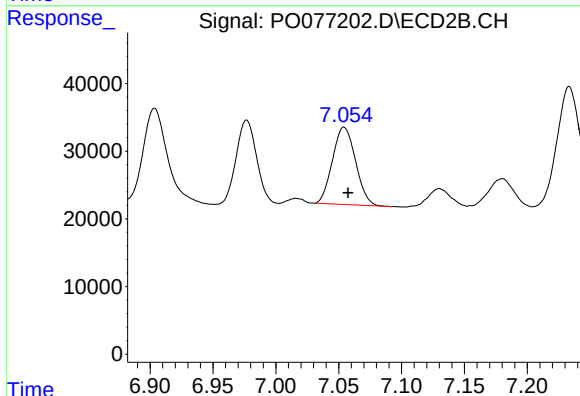


#33 AR-1260-3

R.T.: 7.054 min
Delta R.T.: -0.003 min
Response: 146388
Conc: 44.52 ng/ml

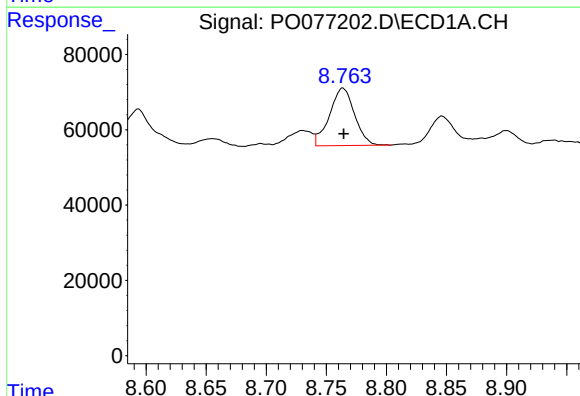


#34 AR-1260-4

R.T.: 8.764 min
Delta R.T.: 0.000 min
Response: 220911
Conc: 45.67 ng/ml

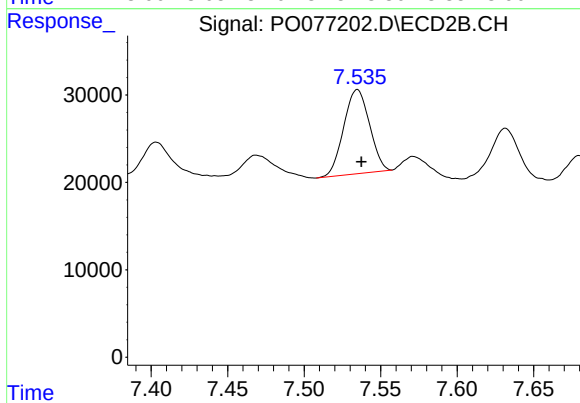

#34 AR-1260-4

R.T.: 7.535 min
Delta R.T.: -0.003 min
Response: 112983
Conc: 47.97 ng/ml

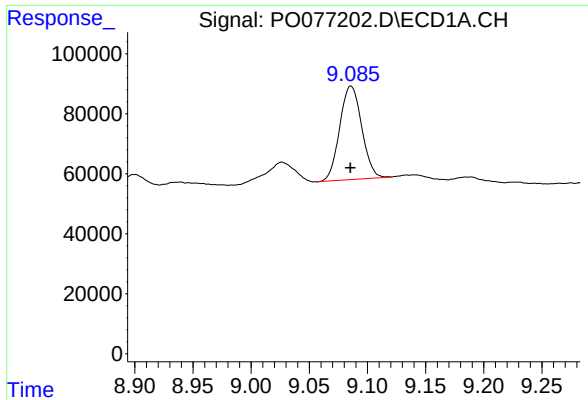


#35 AR-1260-5

R.T.: 9.086 min
Delta R.T.: 0.000 min
Response: 410745
Conc: 44.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-4

Manual Integrations
APPROVED

Ankita
4/23/2021 4:46:37 PM

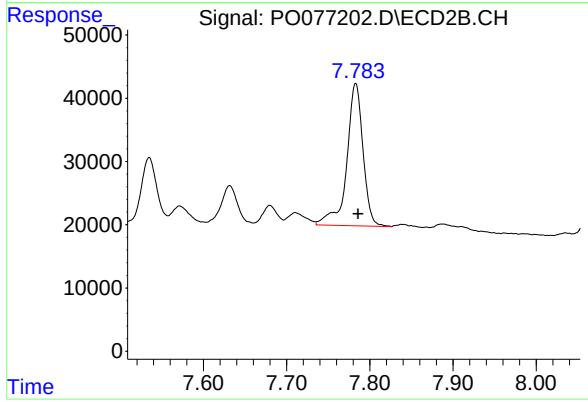

#35 AR-1260-5

R.T.: 7.783 min
Delta R.T.: -0.003 min
Response: 305814
Conc: 56.97 ng/ml