

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042321\
 Data File : P0077203.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Apr 2021 23:28
 Operator : DD\AJ
 Sample : M2099-09
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-5

Manual Integrations
 APPROVED

Ankita
 4/23/2021 4:46:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 01:41:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 09:50:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.896	3.891	2198422	1047440	20.802	19.909
2) SA Decachlor...	10.864	9.130	1876618	669567	18.075	17.745
Target Compounds						
31) L7 AR-1260-1	7.904	6.706	252772	137645	46.717m	46.107m
32) L7 AR-1260-2	8.168	6.904	464781	192926	73.607m	54.116 #
33) L7 AR-1260-3	8.534	7.056	363156	191612	88.969	58.271 #
34) L7 AR-1260-4	8.764	7.535	327831	144939	67.767	61.537
35) L7 AR-1260-5	9.086	7.783	476900	340927	51.284	63.510

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042321\
Data File : P0077203.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Apr 2021 23:28
Operator : DD\AJ
Sample : M2099-09
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
TP-5


Manual Integrations
APPROVED

Ankita
4/23/2021 4:46:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 01:41:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 09:50:22 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

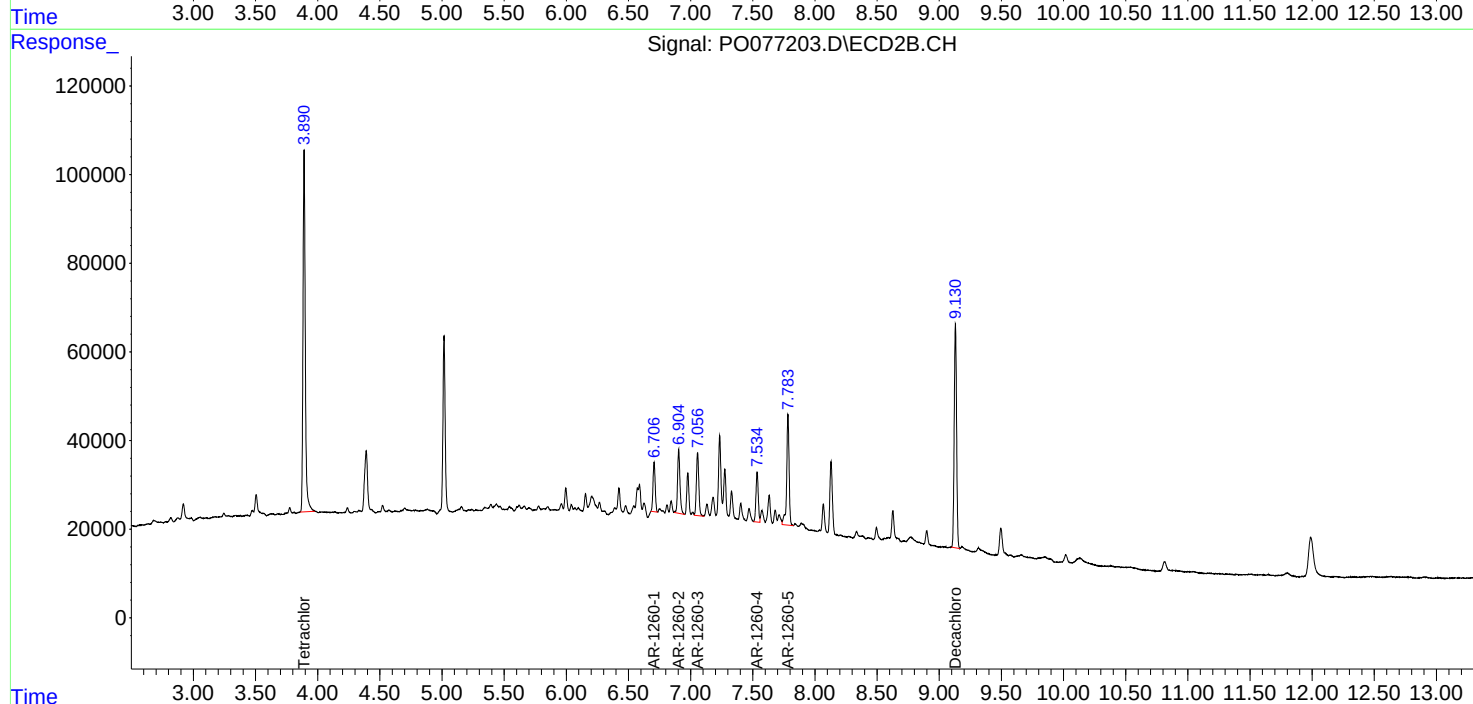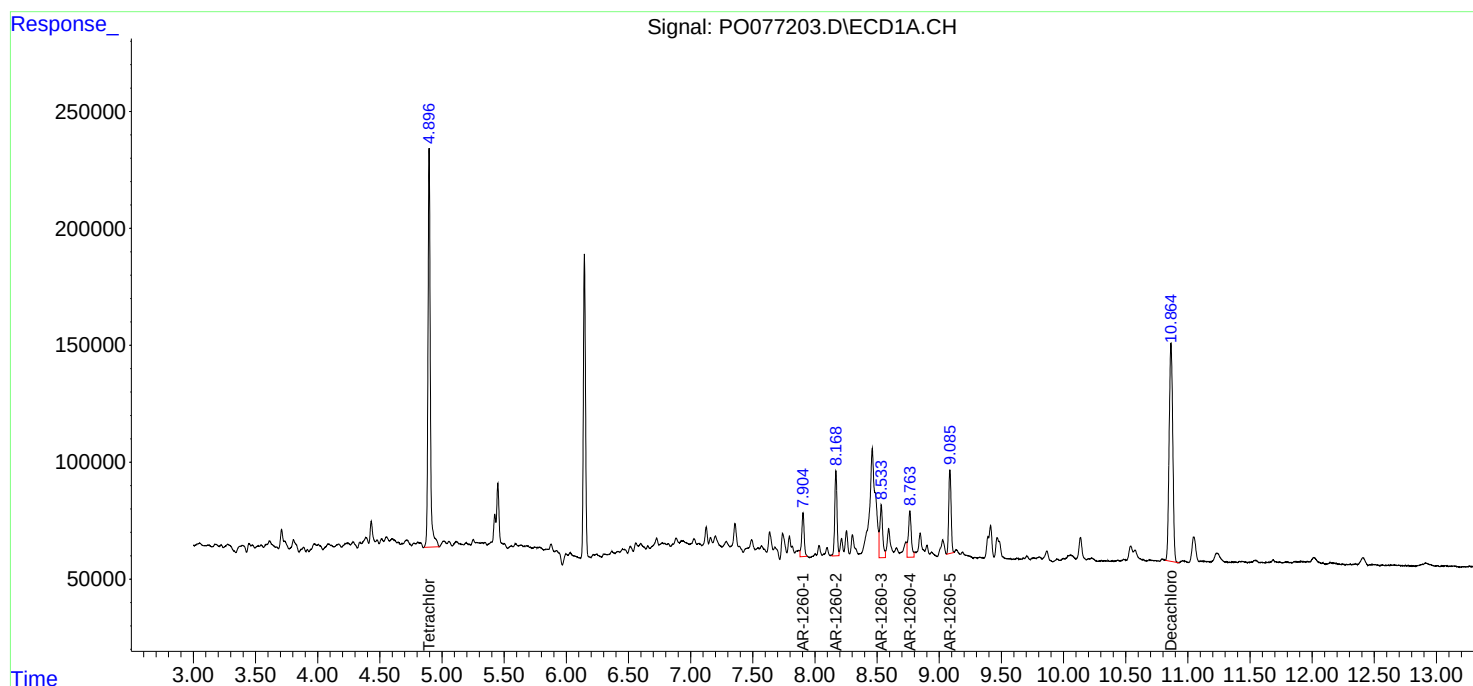

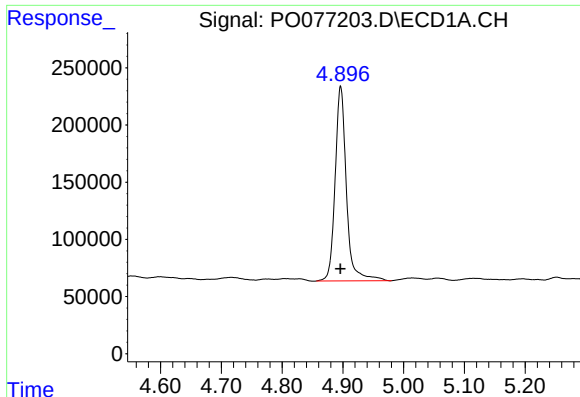


#1 Tetrachloro-m-xylene

R.T.: 4.896 min
Delta R.T.: 0.000 min
Response: 2198422
Conc: 20.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-5


Manual Integrations
APPROVED

Ankita
4/23/2021 4:46:40 PM

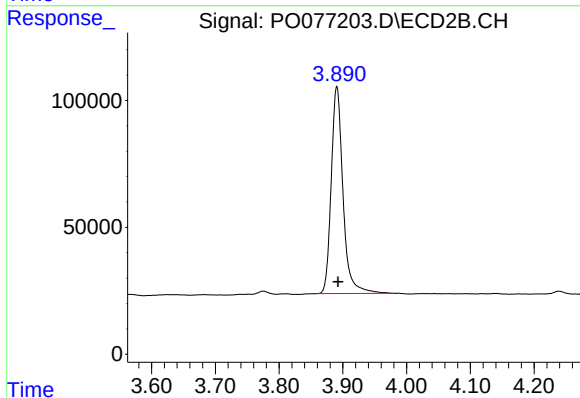


#1 Tetrachloro-m-xylene

R.T.: 3.891 min
Delta R.T.: -0.002 min
Response: 1047440
Conc: 19.91 ng/ml

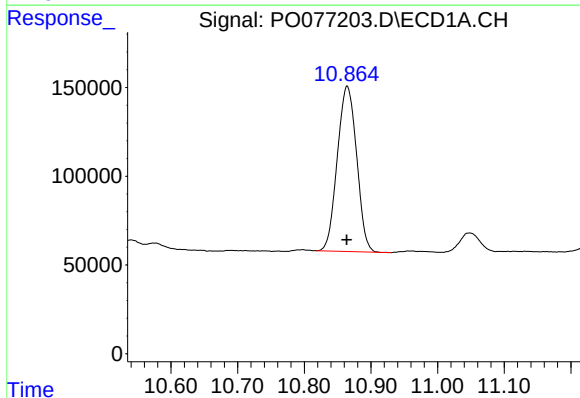


#2 Decachlorobiphenyl

R.T.: 10.864 min
Delta R.T.: 0.000 min
Response: 1876618
Conc: 18.08 ng/ml

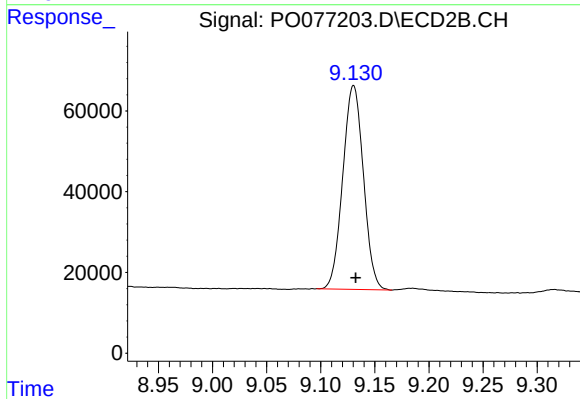

#2 Decachlorobiphenyl

R.T.: 9.130 min
Delta R.T.: -0.002 min
Response: 669567
Conc: 17.74 ng/ml

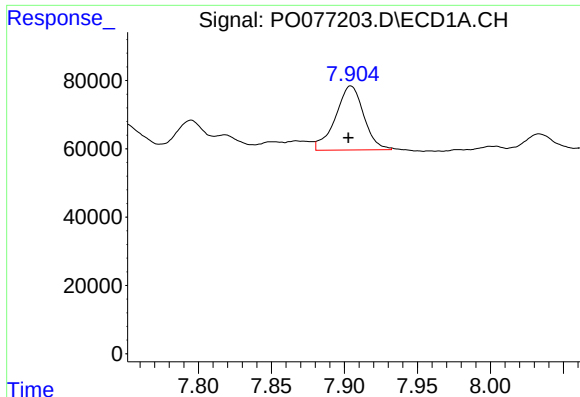


#31 AR-1260-1

R.T.: 7.904 min
Delta R.T.: 0.001 min
Response: 252772
Conc: 46.72 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-5


Manual Integrations
APPROVED

Ankita
4/23/2021 4:46:40 PM

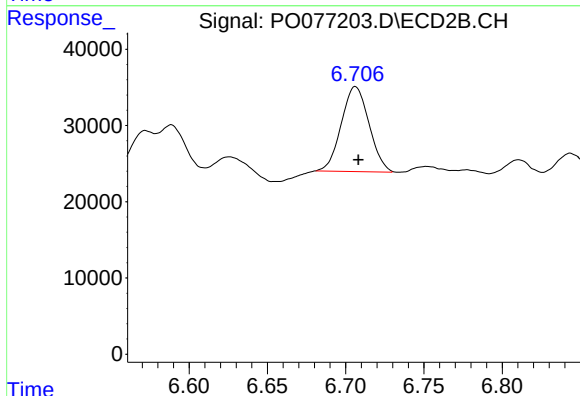


#31 AR-1260-1

R.T.: 6.706 min
Delta R.T.: -0.002 min
Response: 137645
Conc: 46.11 ng/ml m

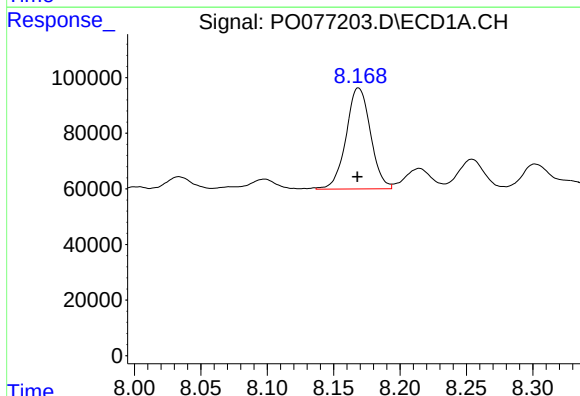


#32 AR-1260-2

R.T.: 8.168 min
Delta R.T.: 0.000 min
Response: 464781
Conc: 73.61 ng/ml m

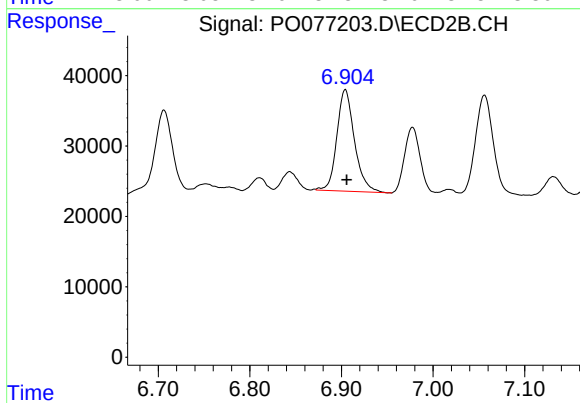

#32 AR-1260-2

R.T.: 6.904 min
Delta R.T.: -0.002 min
Response: 192926
Conc: 54.12 ng/ml

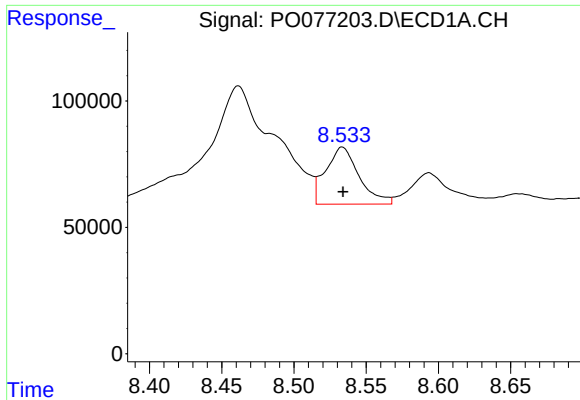


#33 AR-1260-3

R.T.: 8.534 min
Delta R.T.: 0.000 min
Response: 363156
Conc: 88.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-5


Manual Integrations
APPROVED

Ankita
4/23/2021 4:46:40 PM

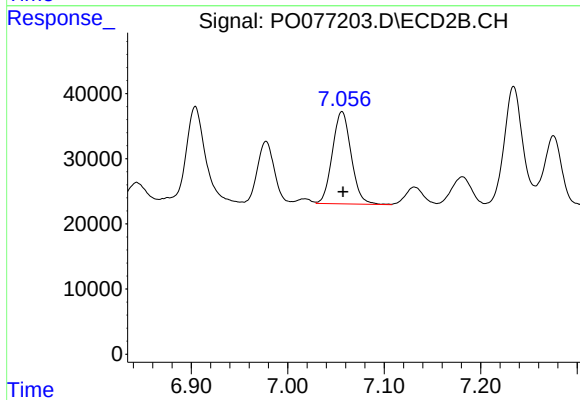


#33 AR-1260-3

R.T.: 7.056 min
Delta R.T.: -0.001 min
Response: 191612
Conc: 58.27 ng/ml

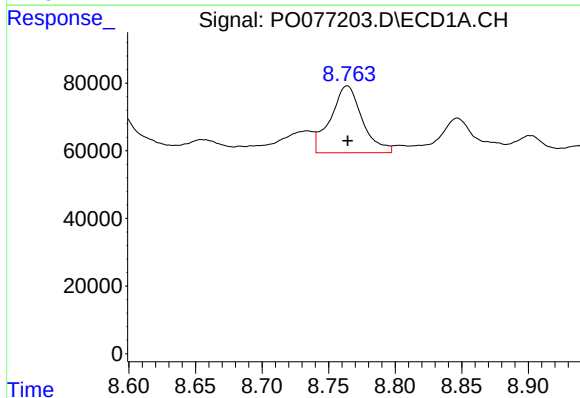


#34 AR-1260-4

R.T.: 8.764 min
Delta R.T.: 0.000 min
Response: 327831
Conc: 67.77 ng/ml

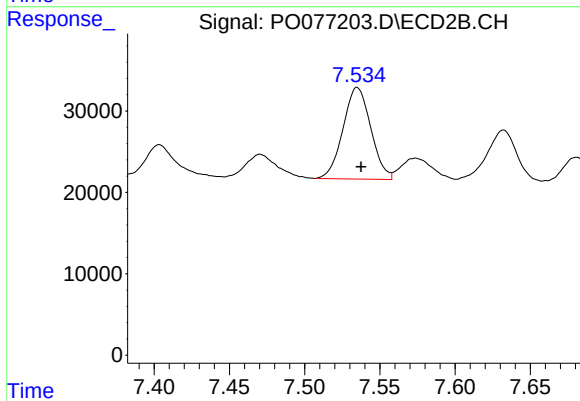

#34 AR-1260-4

R.T.: 7.535 min
Delta R.T.: -0.003 min
Response: 144939
Conc: 61.54 ng/ml

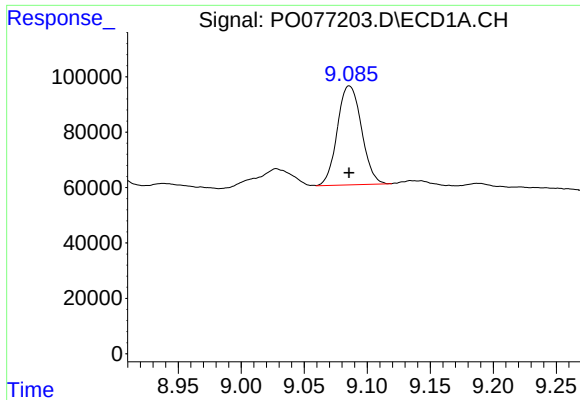


#35 AR-1260-5

R.T.: 9.086 min
Delta R.T.: 0.000 min
Response: 476900
Conc: 51.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-5

Manual Integrations
APPROVED

Ankita
4/23/2021 4:46:40 PM

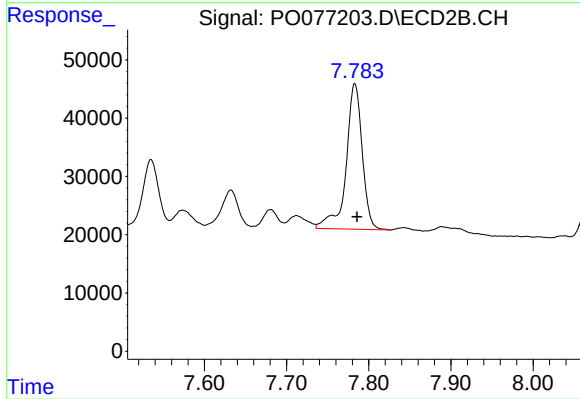

#35 AR-1260-5

R.T.: 7.783 min
Delta R.T.: -0.003 min
Response: 340927
Conc: 63.51 ng/ml