

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042321\
 Data File : P0077204.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Apr 2021 23:45
 Operator : DD\AJ
 Sample : M2101-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 31042-43

Manual Integrations
 APPROVED

Ankita
 4/23/2021 4:46:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 01:41:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 09:50:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.895	3.890	2054650	1005097	19.442	19.104
2) SA Decachlor...	10.860	9.128	969663	356322	9.340m	9.443

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042321\
Data File : P0077204.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Apr 2021 23:45
Operator : DD\AJ
Sample : M2101-01
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
31042-43


Manual Integrations
APPROVED

Ankita
4/23/2021 4:46:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 01:41:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 09:50:22 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

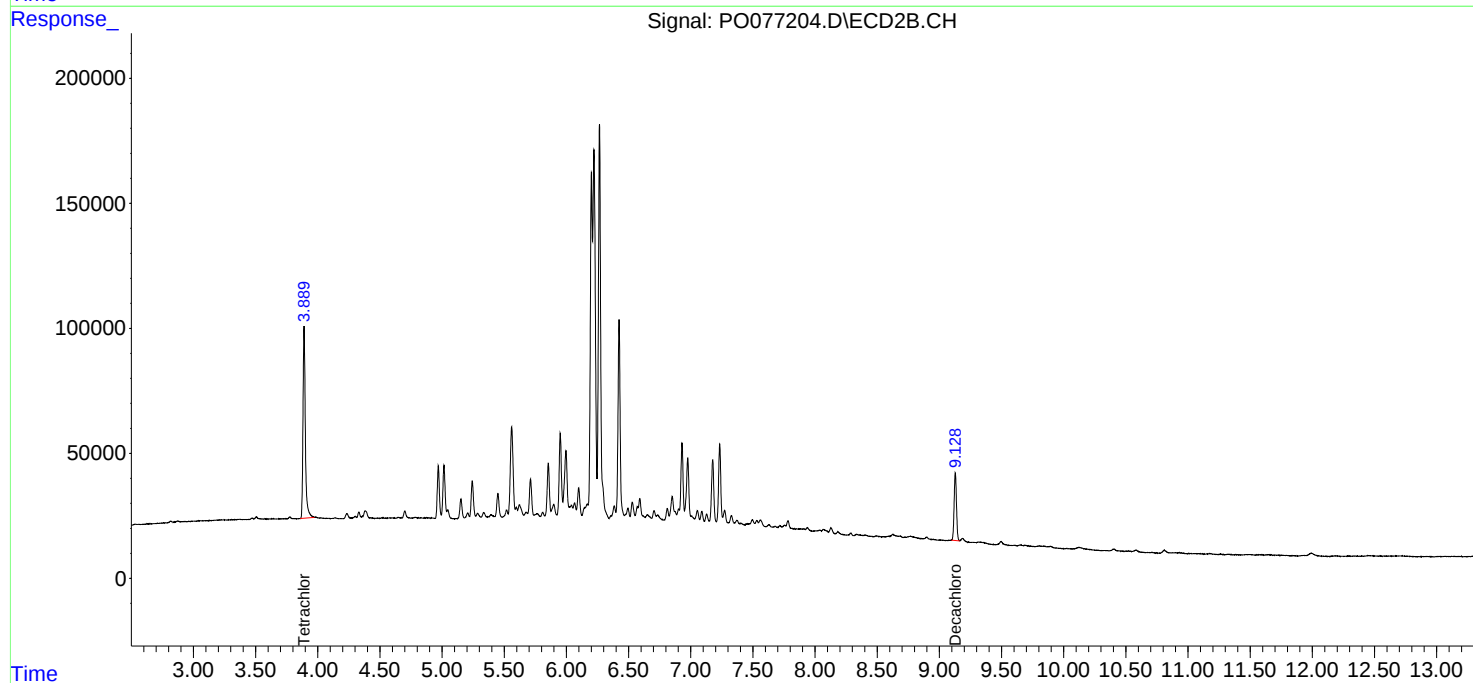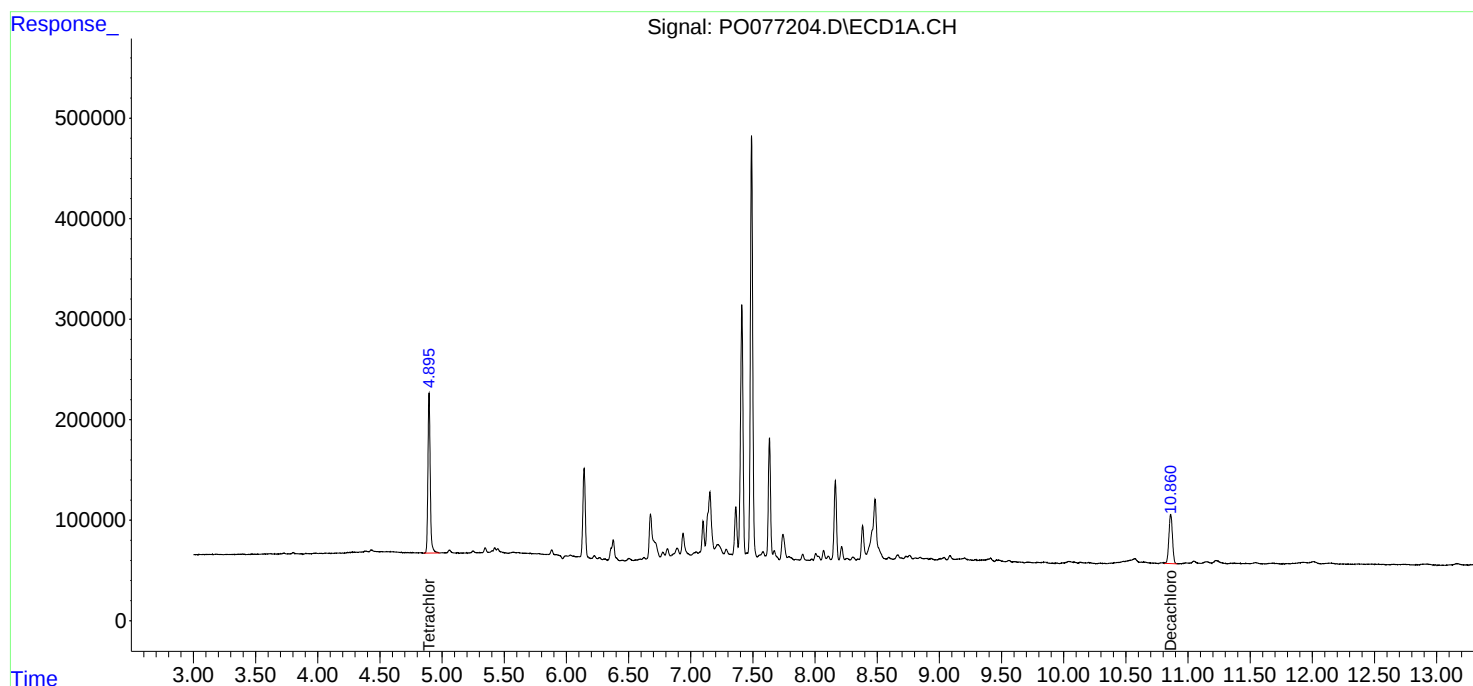

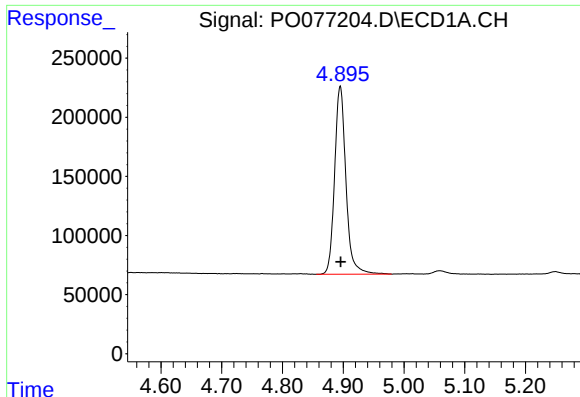


#1 Tetrachloro-m-xylene

R.T.: 4.895 min
Delta R.T.: 0.000 min
Response: 2054650
Conc: 19.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
31042-43


Manual Integrations
APPROVED

Ankita
4/23/2021 4:46:42 PM

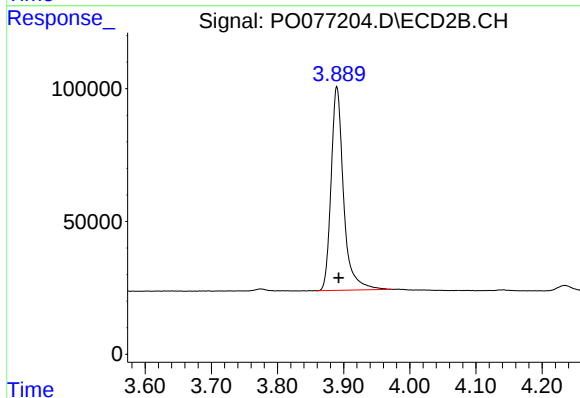


#1 Tetrachloro-m-xylene

R.T.: 3.890 min
Delta R.T.: -0.003 min
Response: 1005097
Conc: 19.10 ng/ml

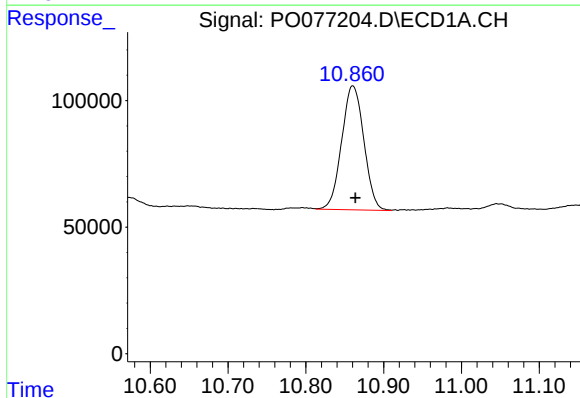

#2 Decachlorobiphenyl

R.T.: 10.860 min
Delta R.T.: -0.004 min
Response: 969663
Conc: 9.34 ng/ml m

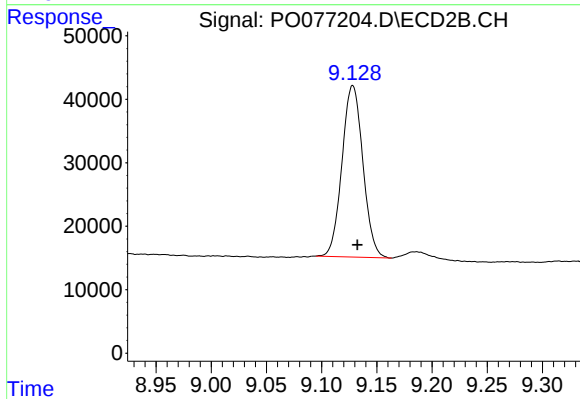

#2 Decachlorobiphenyl

R.T.: 9.128 min
Delta R.T.: -0.004 min
Response: 356322
Conc: 9.44 ng/ml