

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042324\
Data File : P0103058.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Apr 2024 15:49
Operator : YP/AJ
Sample : P2207-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
BUR-1291

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/24/2024
Supervised By :Ankita Jodhani 04/24/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 24 01:41:29 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042224.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 23 02:20:10 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.254	3.374	68363336	40870235	13.555m	14.768
2) SA Decachlor...	9.772	8.226	15788537	8743808	5.437	5.093

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO042324\
Data File : PO103058.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Apr 2024 15:49
Operator : YP/AJ
Sample : P2207-02
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BUR-1291


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/24/2024
Supervised By :Ankita Jodhani 04/24/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 24 01:41:29 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO042224.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 23 02:20:10 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

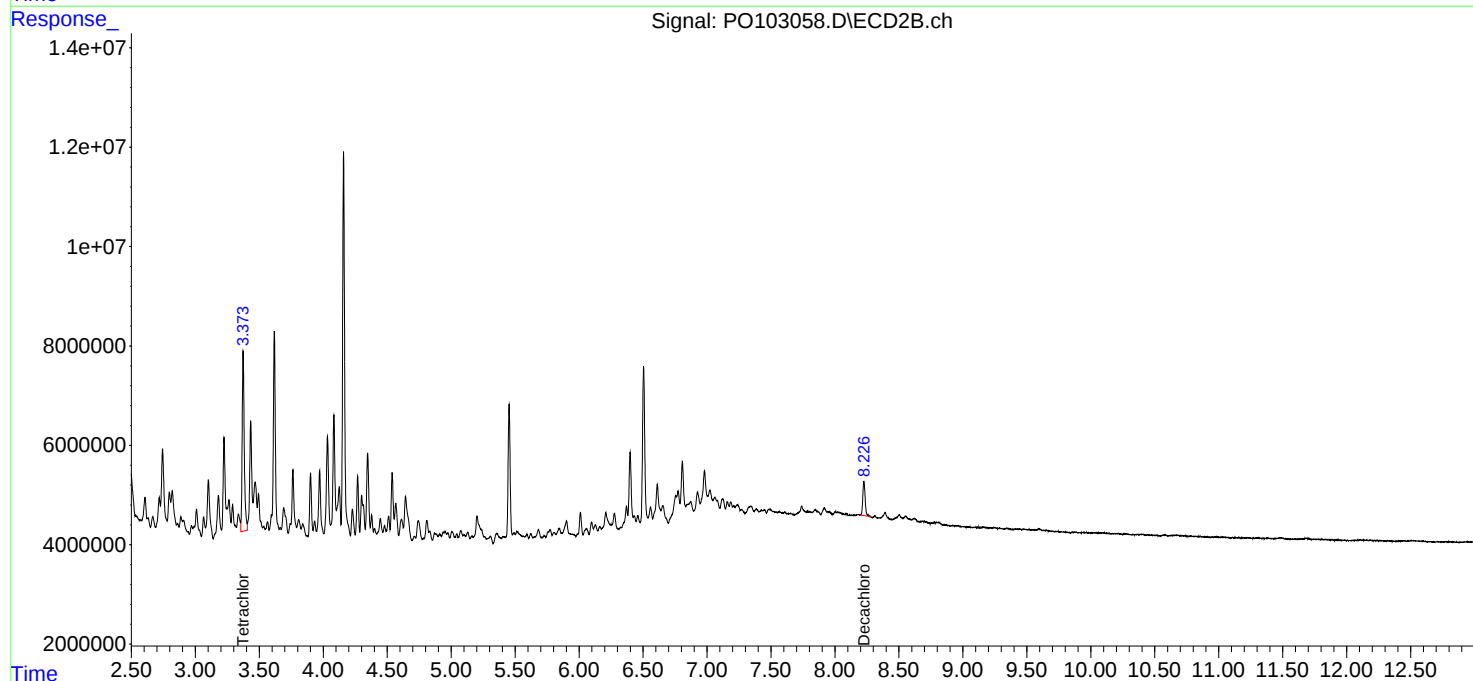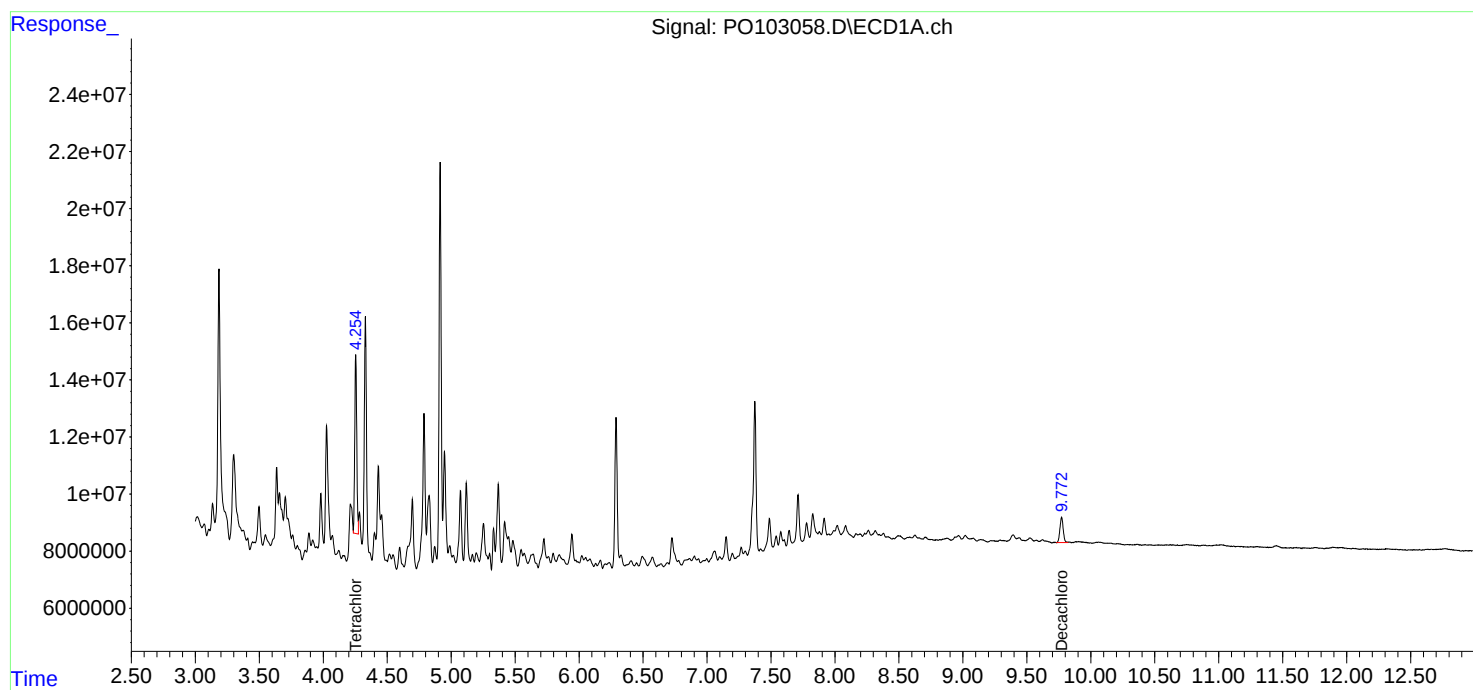

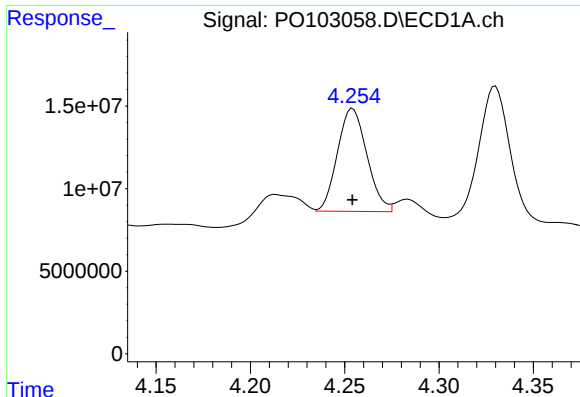


#1 Tetrachloro-m-xylene

R.T.: 4.254 min
Delta R.T.: 0.000 min
Response: 68363336
Conc: 13.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
BUR-1291


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/24/2024
Supervised By :Ankita Jodhani 04/24/2024

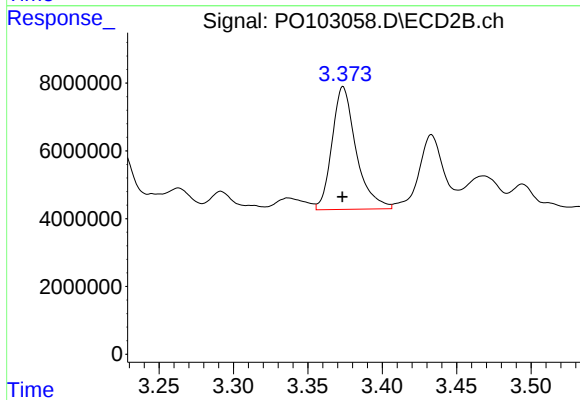


#1 Tetrachloro-m-xylene

R.T.: 3.374 min
Delta R.T.: 0.000 min
Response: 40870235
Conc: 14.77 ng/ml

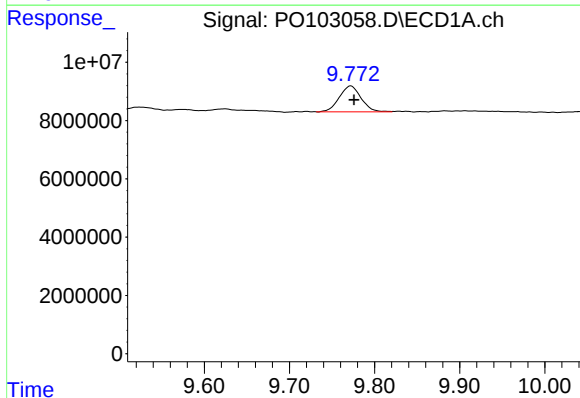

#2 Decachlorobiphenyl

R.T.: 9.772 min
Delta R.T.: -0.004 min
Response: 15788537
Conc: 5.44 ng/ml

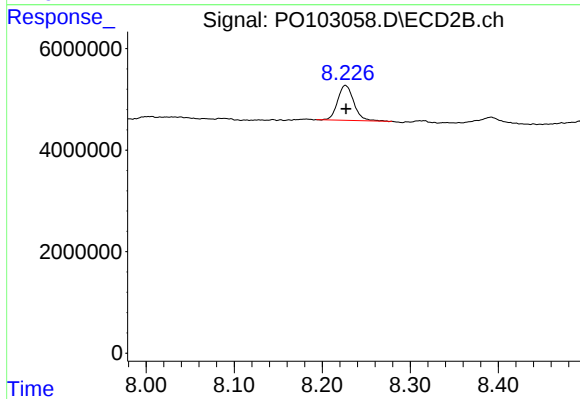

#2 Decachlorobiphenyl

R.T.: 8.226 min
Delta R.T.: 0.000 min
Response: 8743808
Conc: 5.09 ng/ml