

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042324\
 Data File : P0103060.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Apr 2024 16:23
 Operator : YP/AJ
 Sample : P2218-02
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 B-131-GW-02

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/24/2024
 Supervised By :Ankita Jodhani 04/24/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 24 01:42:08 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042224.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 23 02:20:10 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.254	3.373	75540256	37411921	14.978m	13.518m
2) SA Decachlor...	9.773	8.226	33009695	18350940	11.368	10.688

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO042324\
Data File : PO103060.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Apr 2024 16:23
Operator : YP/AJ
Sample : P2218-02
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
B-131-GW-02


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/24/2024
Supervised By :Ankita Jodhani 04/24/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 24 01:42:08 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO042224.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 23 02:20:10 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

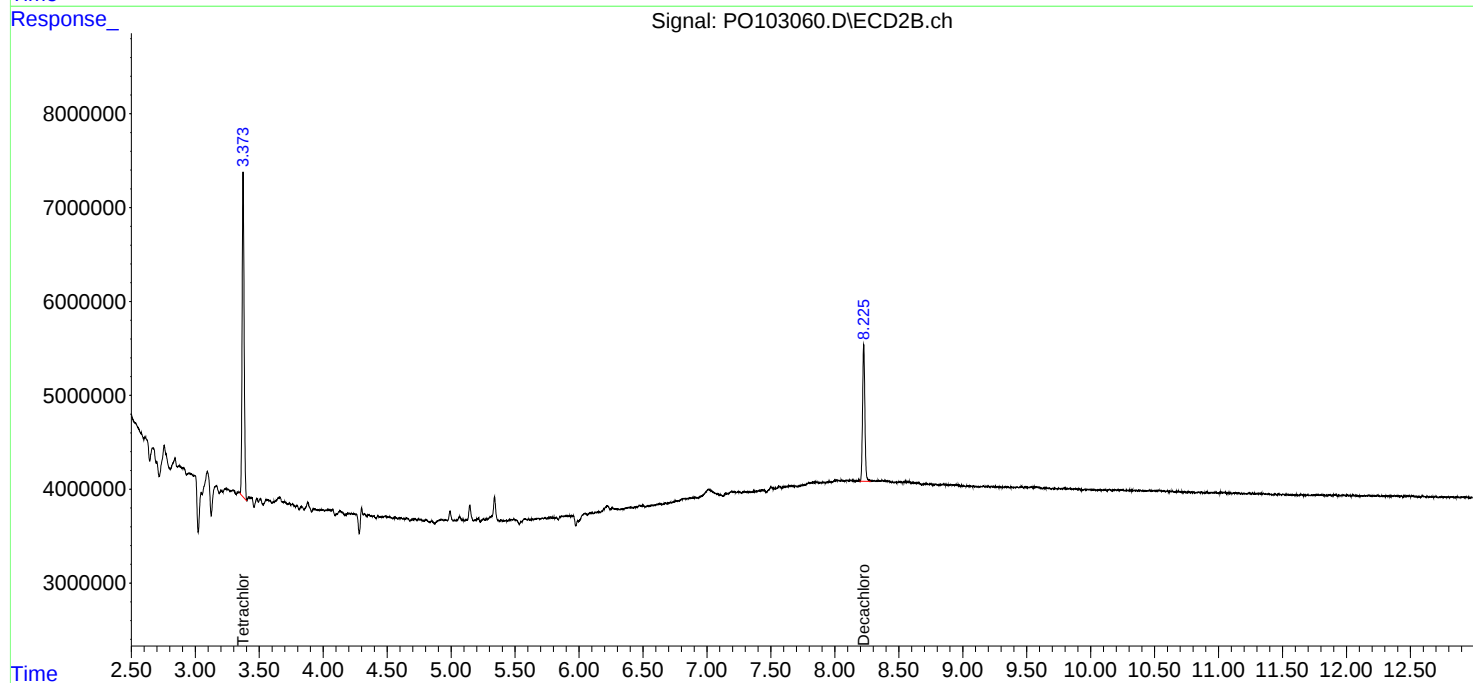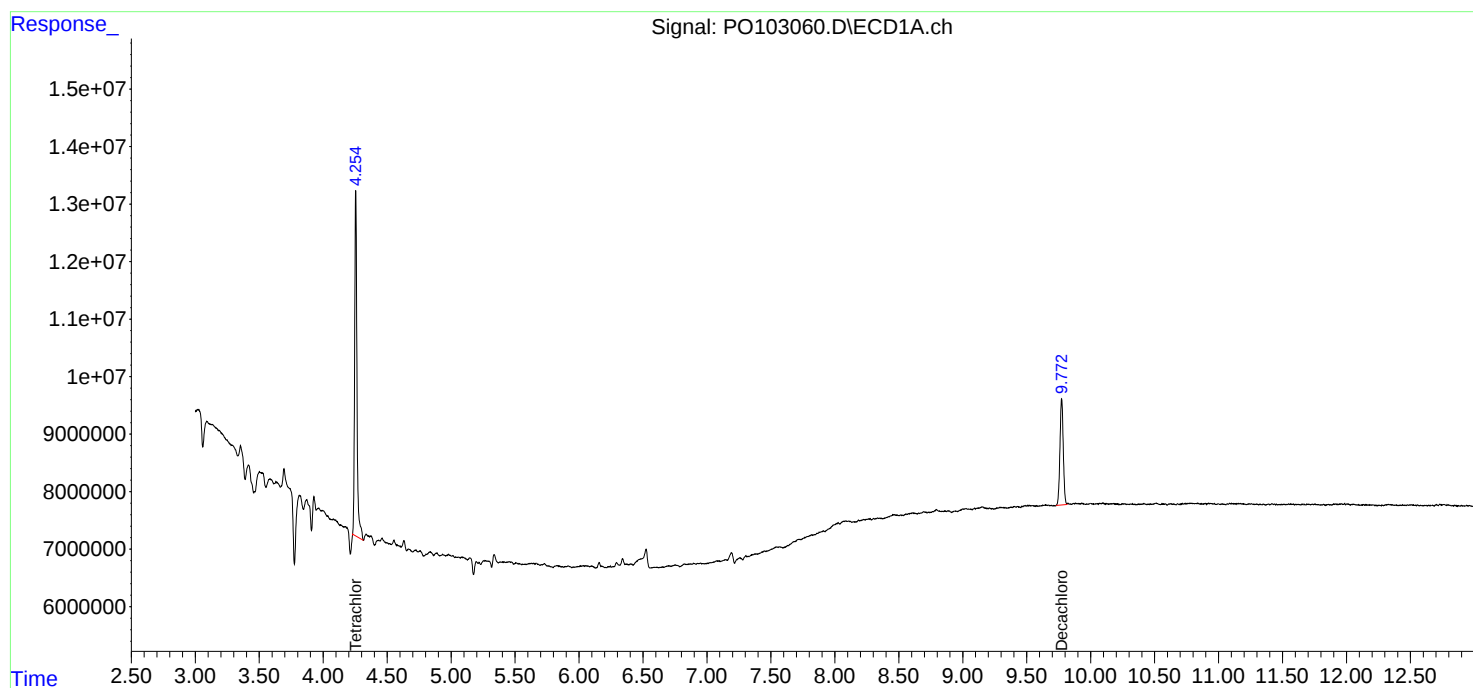

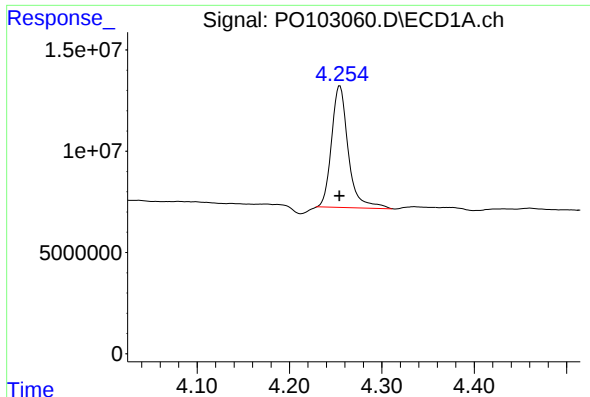


#1 Tetrachloro-m-xylene

R.T.: 4.254 min
Delta R.T.: 0.000 min
Response: 75540256
Conc: 14.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
B-131-GW-02


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/24/2024
Supervised By :Ankita Jodhani 04/24/2024

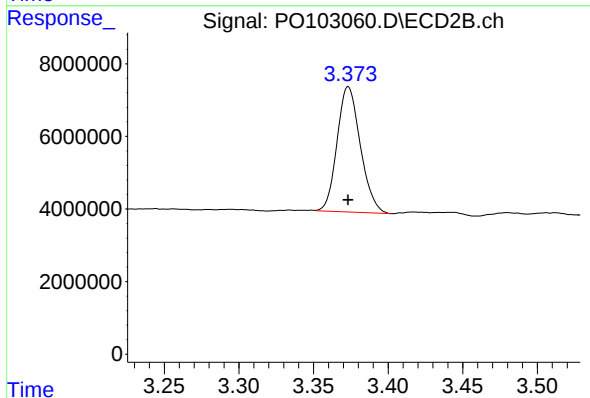


#1 Tetrachloro-m-xylene

R.T.: 3.373 min
Delta R.T.: 0.000 min
Response: 37411921
Conc: 13.52 ng/ml m

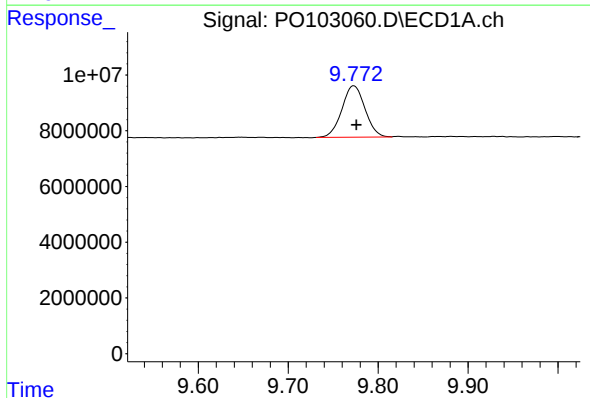

#2 Decachlorobiphenyl

R.T.: 9.773 min
Delta R.T.: -0.003 min
Response: 33009695
Conc: 11.37 ng/ml

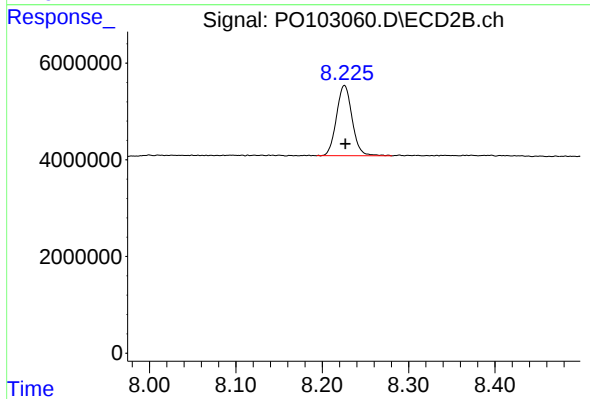

#2 Decachlorobiphenyl

R.T.: 8.226 min
Delta R.T.: -0.001 min
Response: 18350940
Conc: 10.69 ng/ml