

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042324\
 Data File : P0103104.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2024 06:25
 Operator : YP/AJ
 Sample : P2231-04
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PE-3(0-0.5)

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/24/2024
 Supervised By :Ankita Jodhani 04/24/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 24 06:45:29 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042224.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 23 02:20:10 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.252	3.370	102.6E6	50270820	20.352	18.164
2) SA Decachlor...	9.772	8.222	42736354	24225634	14.718m	14.110m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO042324\
Data File : PO103104.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2024 06:25
Operator : YP/AJ
Sample : P2231-04
Misc :
ALS Vial : 51 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PE-3(0-0.5)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/24/2024
Supervised By :Ankita Jodhani 04/24/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 24 06:45:29 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO042224.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 23 02:20:10 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

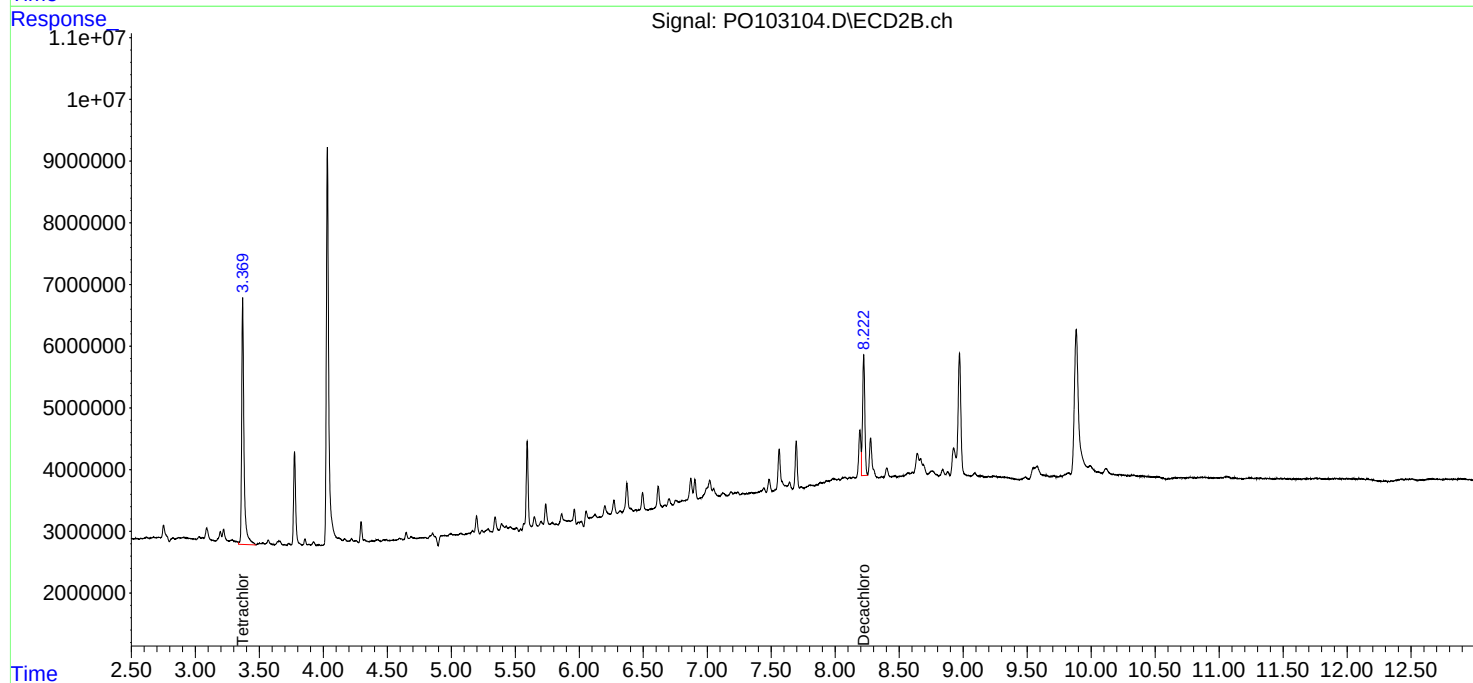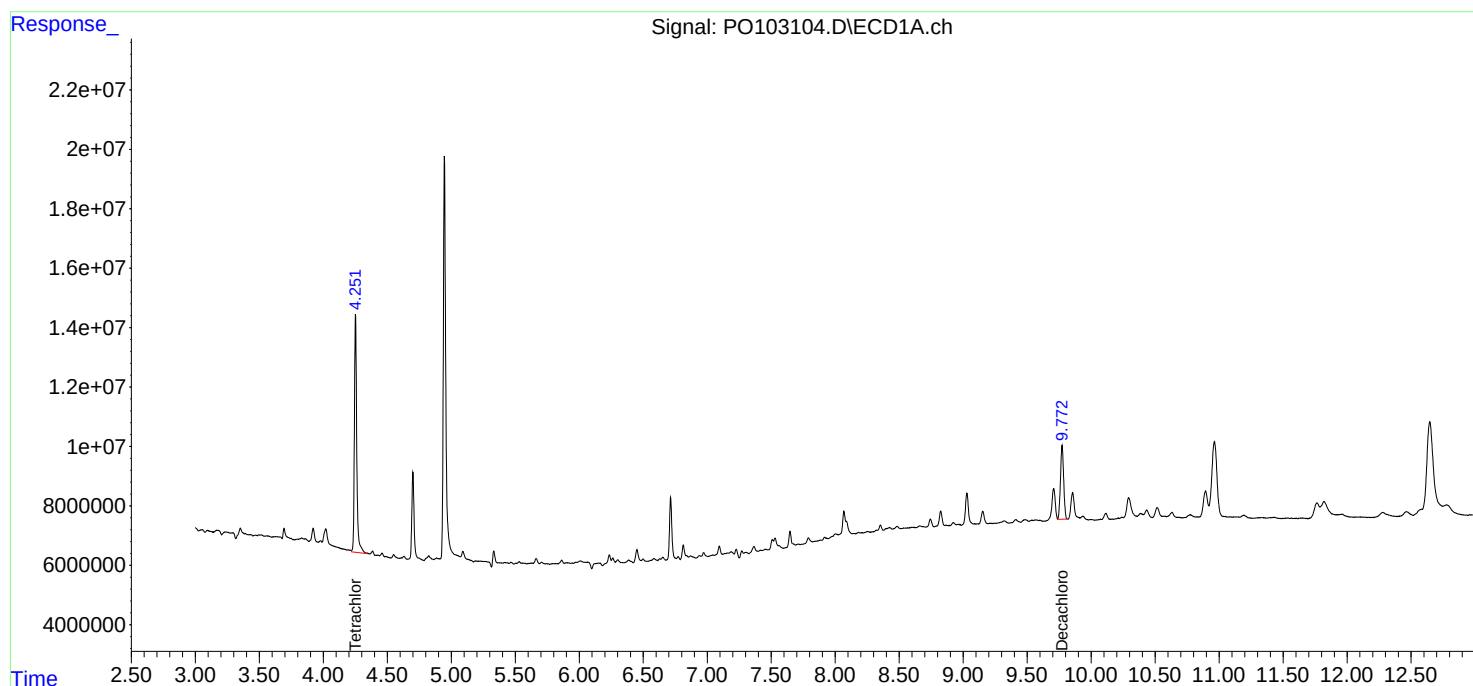

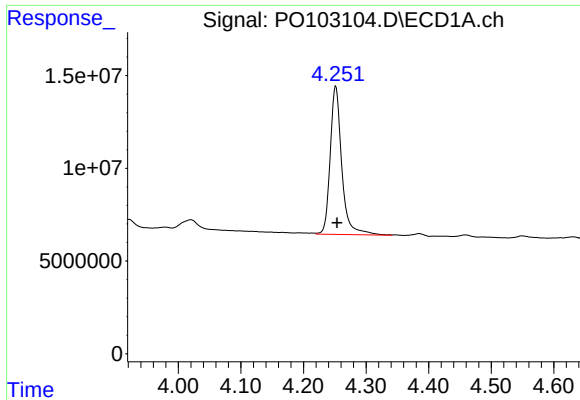


#1 Tetrachloro-m-xylene

R.T.: 4.252 min
Delta R.T.: -0.002 min
Response: 102643634
Conc: 20.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
PE-3(0-0.5)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/24/2024
Supervised By :Ankita Jodhani 04/24/2024

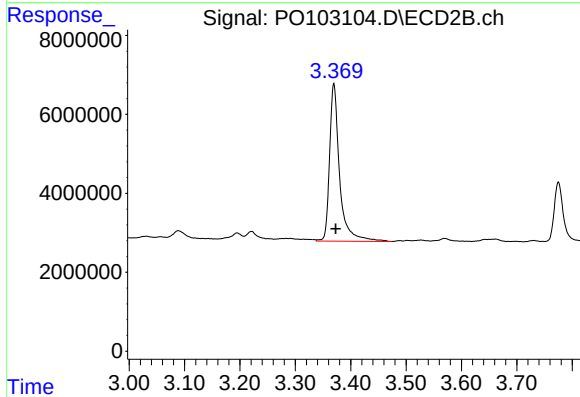


#1 Tetrachloro-m-xylene

R.T.: 3.370 min
Delta R.T.: -0.003 min
Response: 50270820
Conc: 18.16 ng/ml

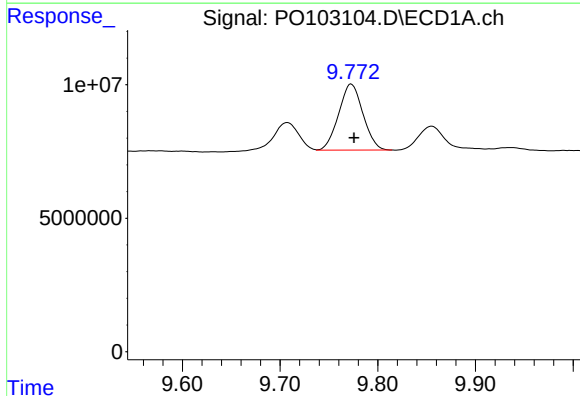

#2 Decachlorobiphenyl

R.T.: 9.772 min
Delta R.T.: -0.004 min
Response: 42736354
Conc: 14.72 ng/ml m

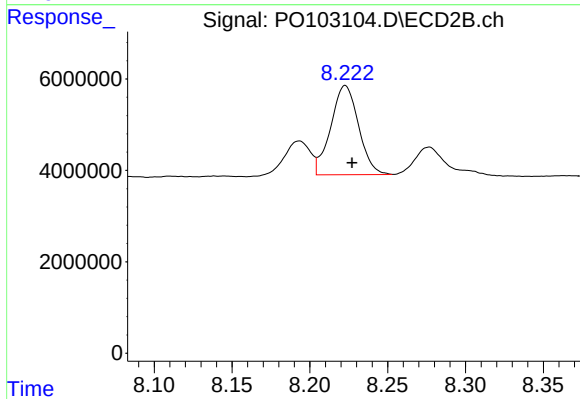

#2 Decachlorobiphenyl

R.T.: 8.222 min
Delta R.T.: -0.005 min
Response: 24225634
Conc: 14.11 ng/ml m