

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042521\
 Data File : P0077282.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Apr 2021 14:05
 Operator : DD\AJ
 Sample : M2136-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 02:19:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 09:50:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.897	3.891	1021285	566663	9.664	10.771
2) SA Decachlor...	10.862	9.124	415694	253598	4.004	6.721 #
Target Compounds						
20) L4 AR-1242-5	7.196	0.000	14689735	0	6353.013	N.D. #
24) L5 AR-1248-4	7.137f	0.000	262603	0	64.978	N.D. #
25) L5 AR-1248-5	7.196	0.000	14689735	0	3595.706	N.D. #
26) L6 AR-1254-1	7.137	0.000	262603	0	63.860	N.D. #
35) L7 AR-1260-5	9.100	0.000	521451	0	56.075	N.D. #
37) L8 AR-1262-2	9.100f	0.000	521451	0	44.890	N.D. #
38) L8 AR-1262-3	0.000	8.052f	0	59587	N.D.	24.650 #
41) L9 AR-1268-1	0.000	8.052f	0	59587	N.D.	8.451 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042521\
Data File : P0077282.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Apr 2021 14:05
Operator : DD\AJ
Sample : M2136-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 02:19:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 09:50:22 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

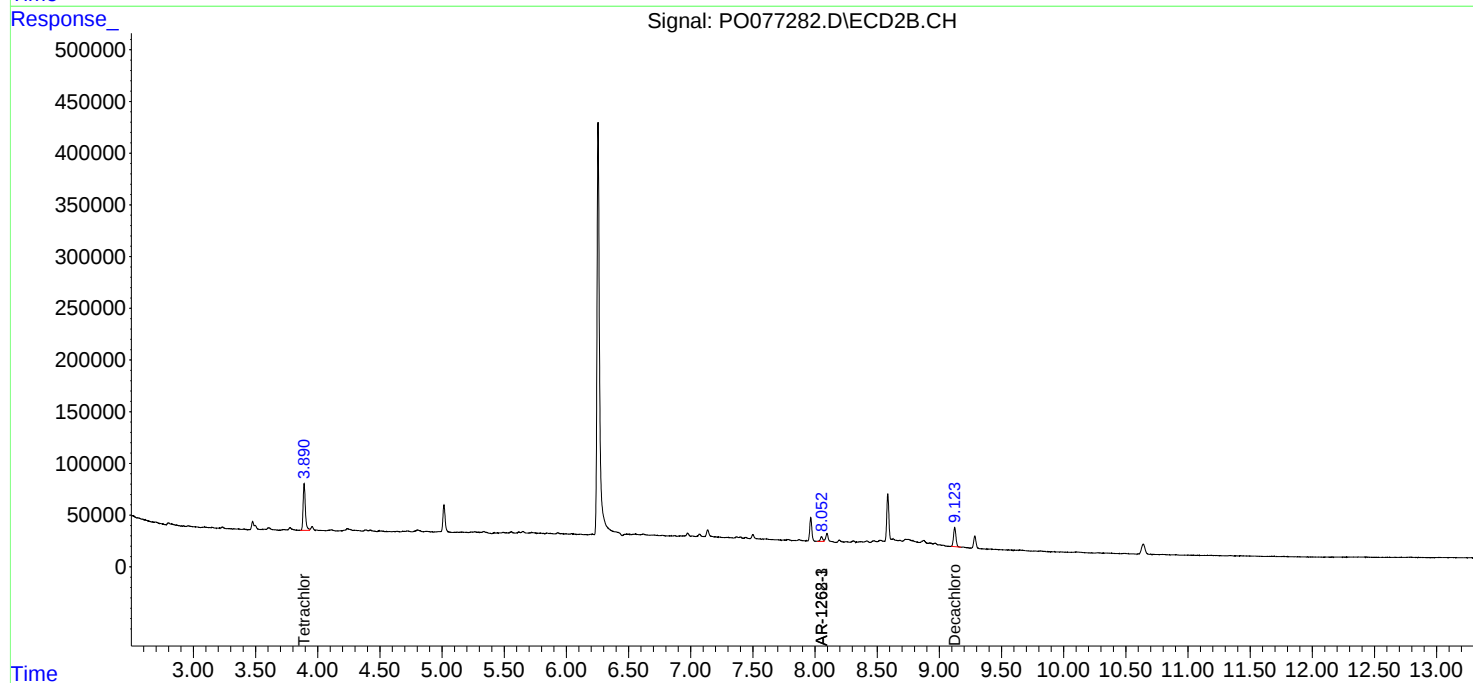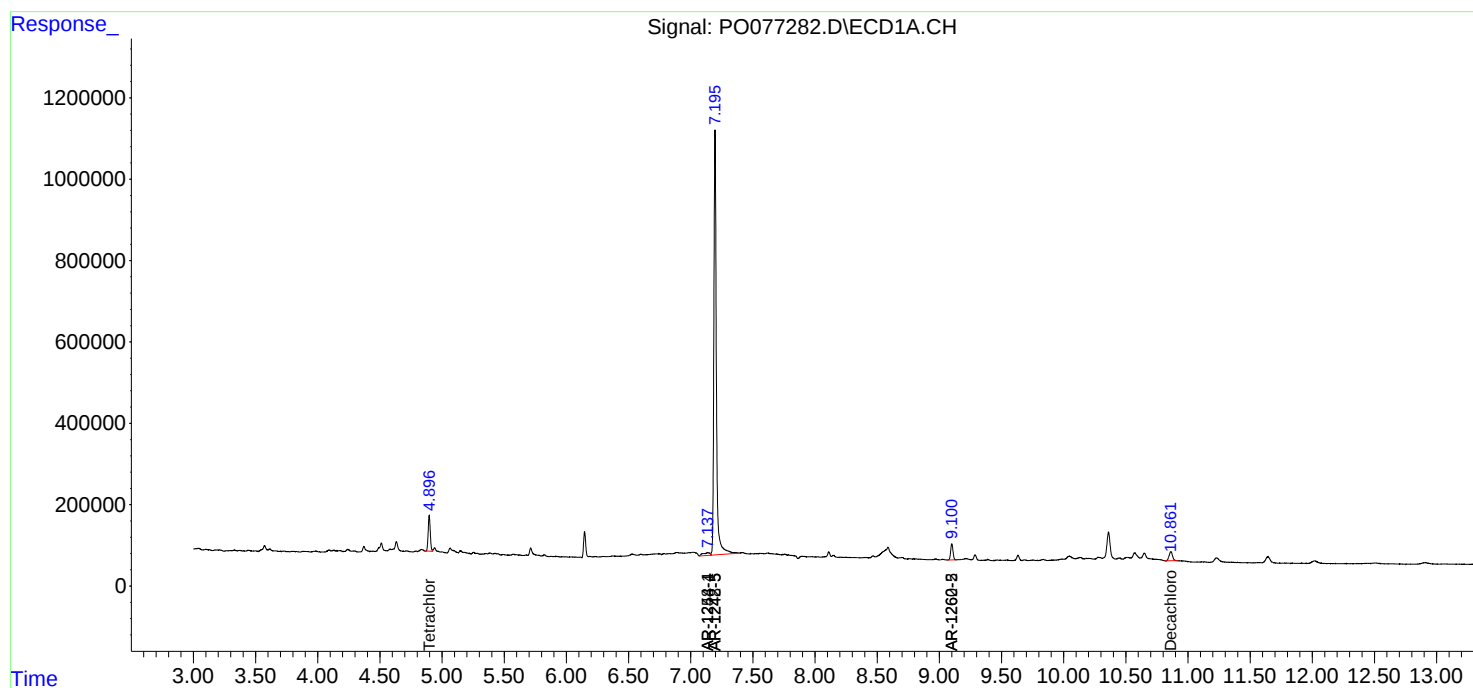


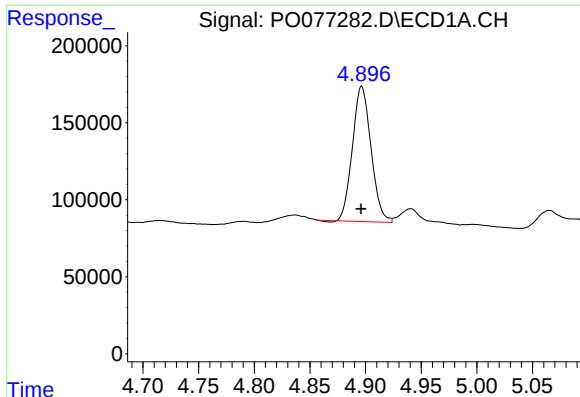

#1 Tetrachloro-m-xylene


R.T.: 4.897 min
Delta R.T.: 0.000 min
Response: 1021285
Conc: 9.66 ng/ml

Instrument :
ECD_O
ClientSampleId :

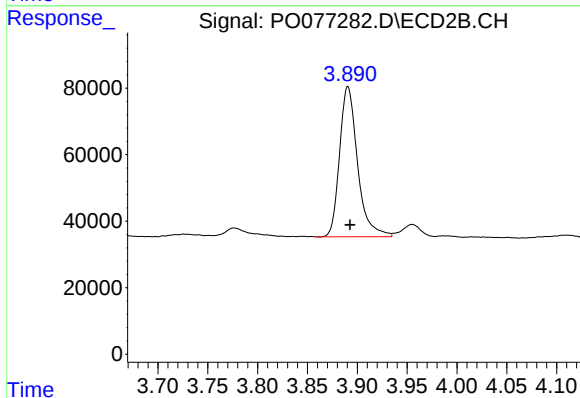


#1 Tetrachloro-m-xylene

R.T.: 3.891 min
Delta R.T.: -0.002 min
Response: 566663
Conc: 10.77 ng/ml

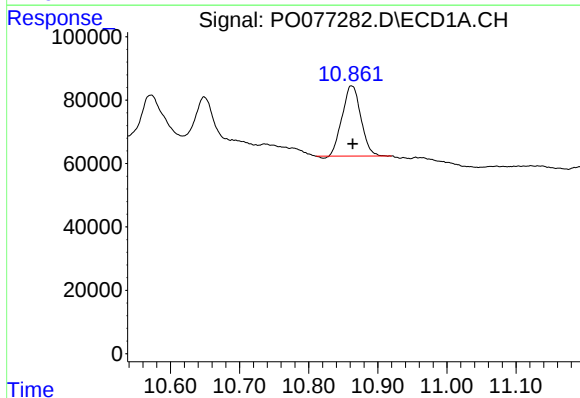


#2 Decachlorobiphenyl

R.T.: 10.862 min
Delta R.T.: -0.002 min
Response: 415694
Conc: 4.00 ng/ml

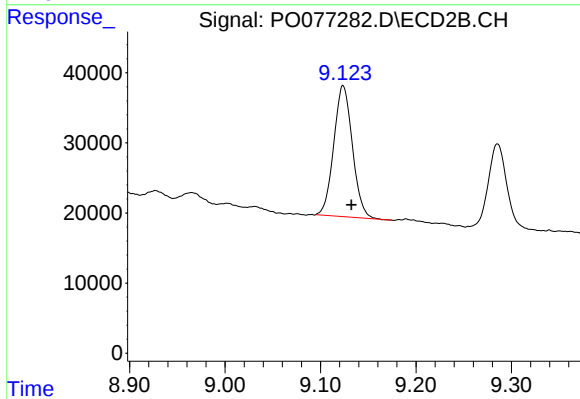

#2 Decachlorobiphenyl


R.T.: 9.124 min
Delta R.T.: -0.009 min
Response: 253598
Conc: 6.72 ng/ml

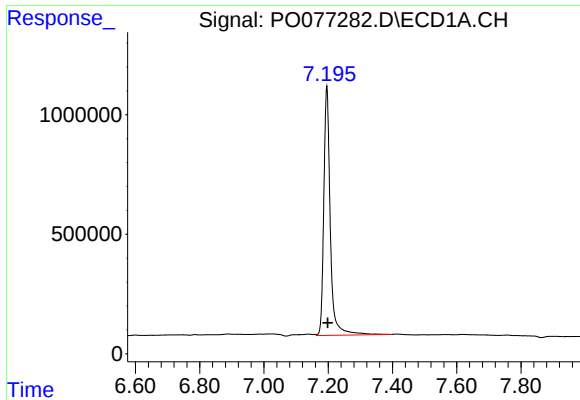

#20 AR-1242-5


R.T.: 7.196 min
Delta R.T.: -0.003 min
Response: 14689735
Conc: 6353.01 ng/ml

Instrument :
ECD_O
ClientSampleId :

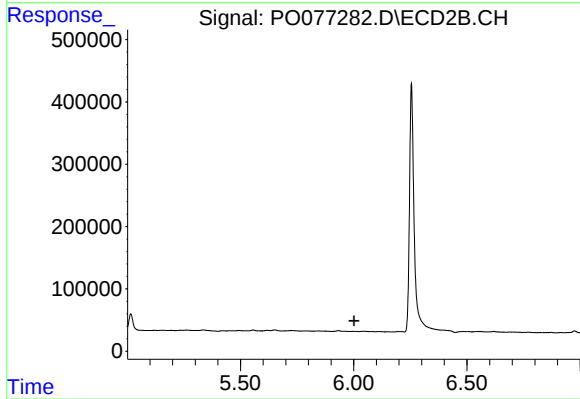


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 6.001 min
Response: 0
Conc: N.D.

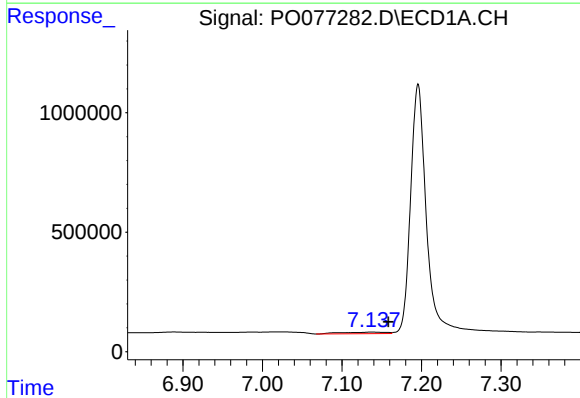


#24 AR-1248-4

R.T.: 7.137 min
Delta R.T.: -0.021 min
Response: 262603
Conc: 64.98 ng/ml

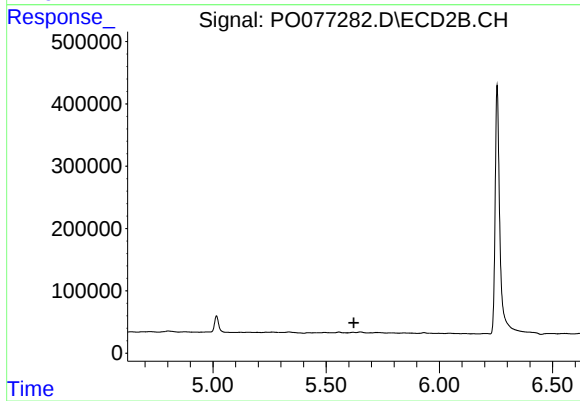

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.622 min
Response: 0
Conc: N.D.

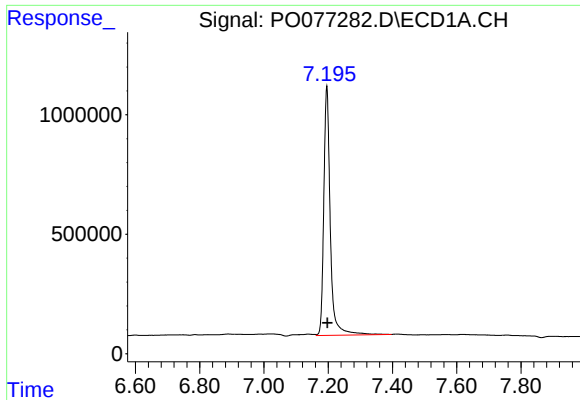

#25 AR-1248-5


R.T.: 7.196 min
Delta R.T.: -0.002 min
Response: 14689735
Conc: 3595.71 ng/ml

Instrument :
ECD_O
ClientSampleId :

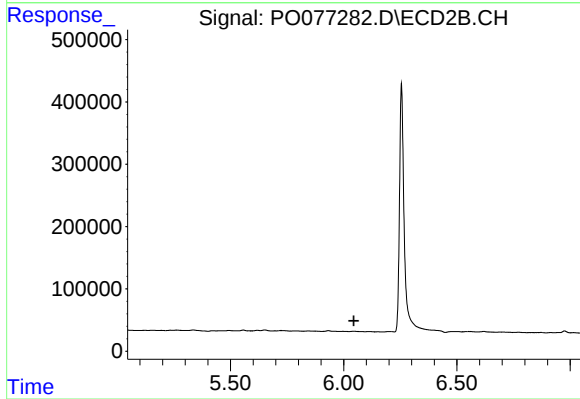


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 6.045 min
Response: 0
Conc: N.D.

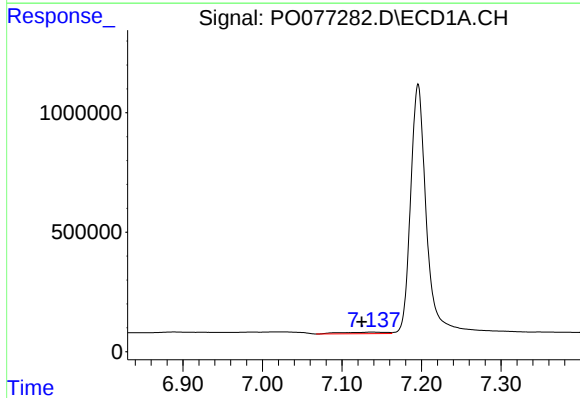


#26 AR-1254-1

R.T.: 7.137 min
Delta R.T.: 0.012 min
Response: 262603
Conc: 63.86 ng/ml

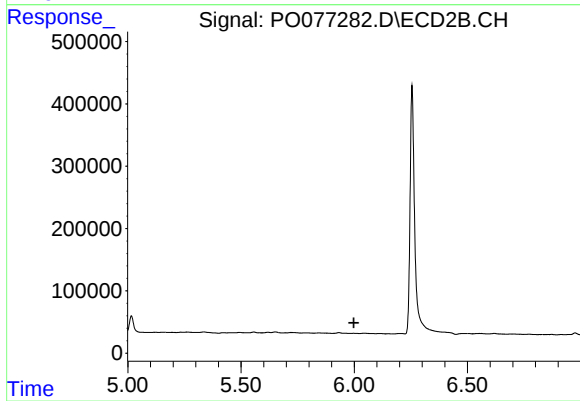

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 5.999 min
Response: 0
Conc: N.D.

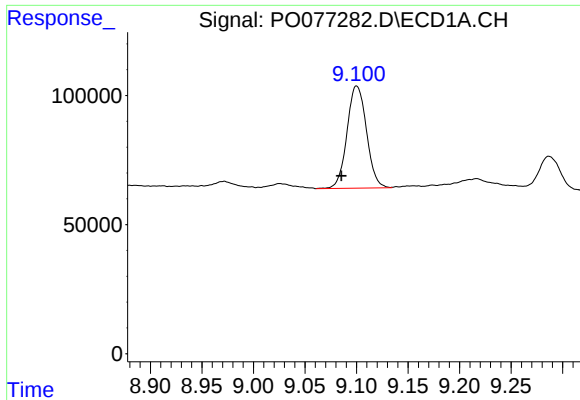

#35 AR-1260-5


R.T.: 9.100 min
Delta R.T.: 0.015 min
Response: 521451
Conc: 56.08 ng/ml

Instrument :
ECD_O
ClientSampleId :

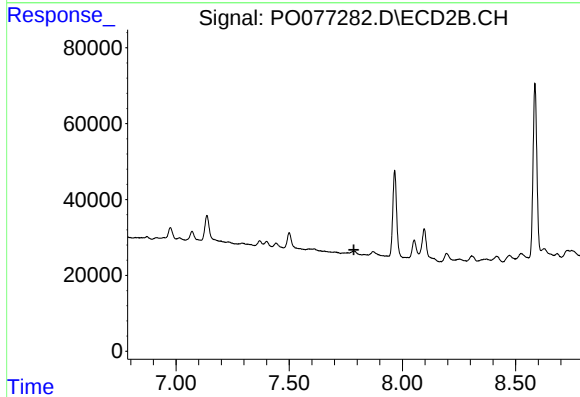


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.786 min
Response: 0
Conc: N.D.

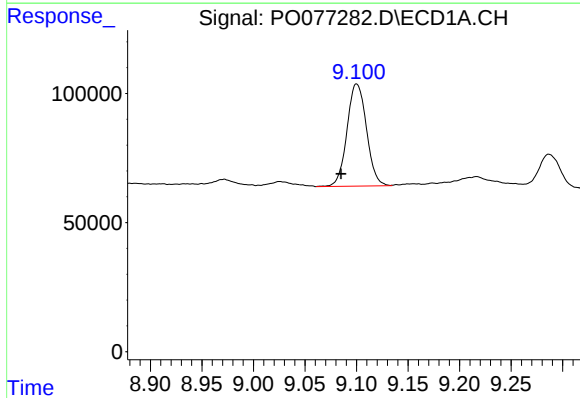


#37 AR-1262-2

R.T.: 9.100 min
Delta R.T.: 0.015 min
Response: 521451
Conc: 44.89 ng/ml

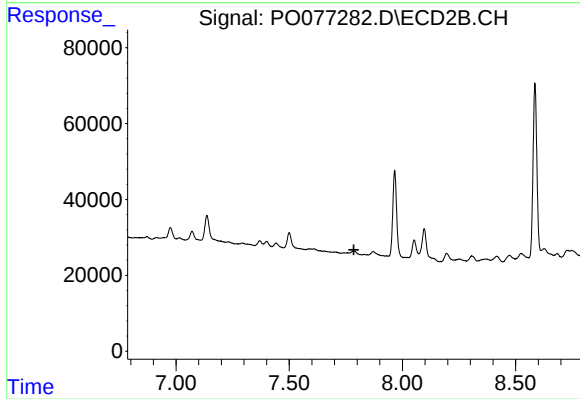

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 7.785 min
Response: 0
Conc: N.D.

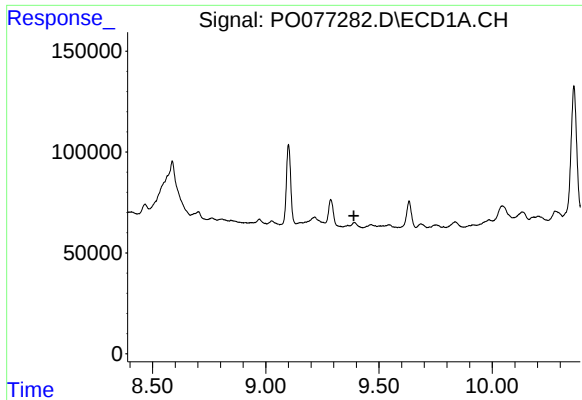

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 9.389 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

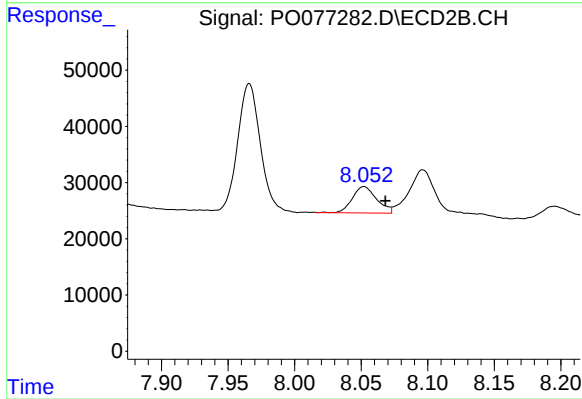


#38 AR-1262-3

R.T.: 8.052 min
Delta R.T.: -0.016 min
Response: 59587
Conc: 24.65 ng/ml

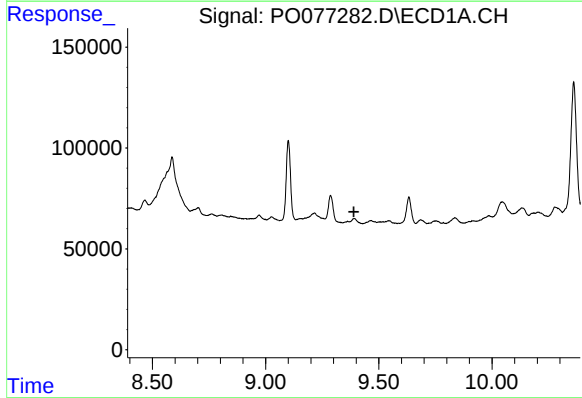

#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 9.390 min
Response: 0
Conc: N.D.

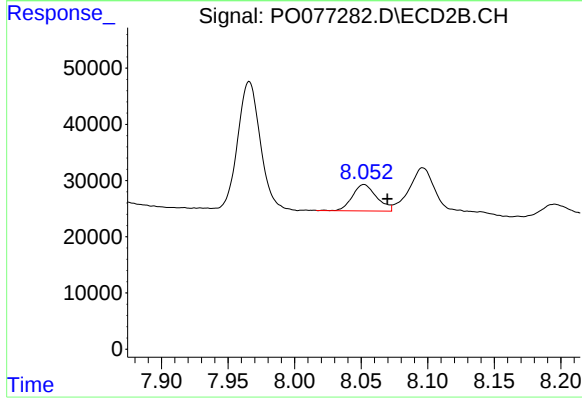

#41 AR-1268-1

R.T.: 8.052 min
Delta R.T.: -0.018 min
Response: 59587
Conc: 8.45 ng/ml