

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042421\
 Data File : P0077234.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Apr 2021 12:23
 Operator : DD\AJ
 Sample : M2043-02RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FS-WC-WATERRE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 14:03:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 09:50:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.896	3.892	441273	203536	4.175	3.869
2) SA Decachlor...	10.862	9.127	199398	59607	1.921	1.580

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042421\
Data File : P0077234.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Apr 2021 12:23
Operator : DD\AJ
Sample : M2043-02RE
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FS-WC-WATERRE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 14:03:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 09:50:22 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

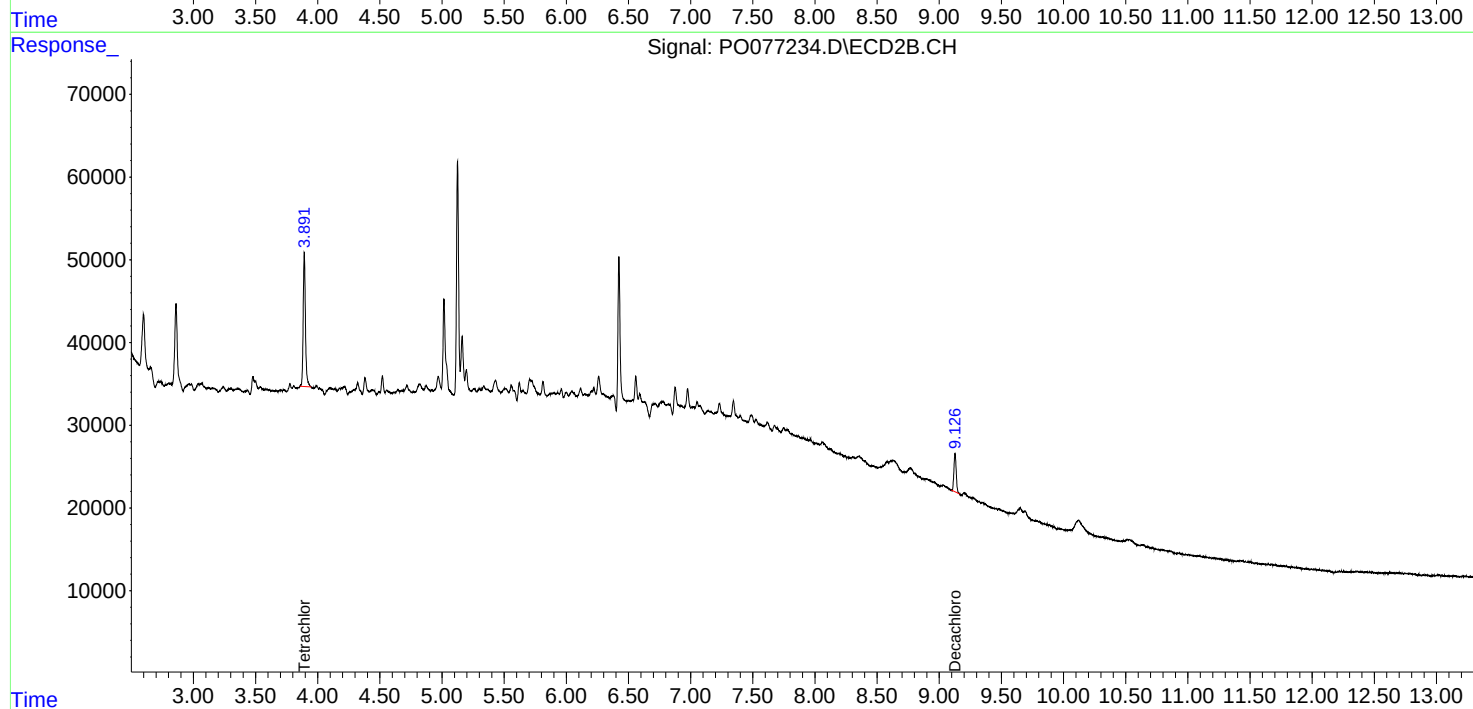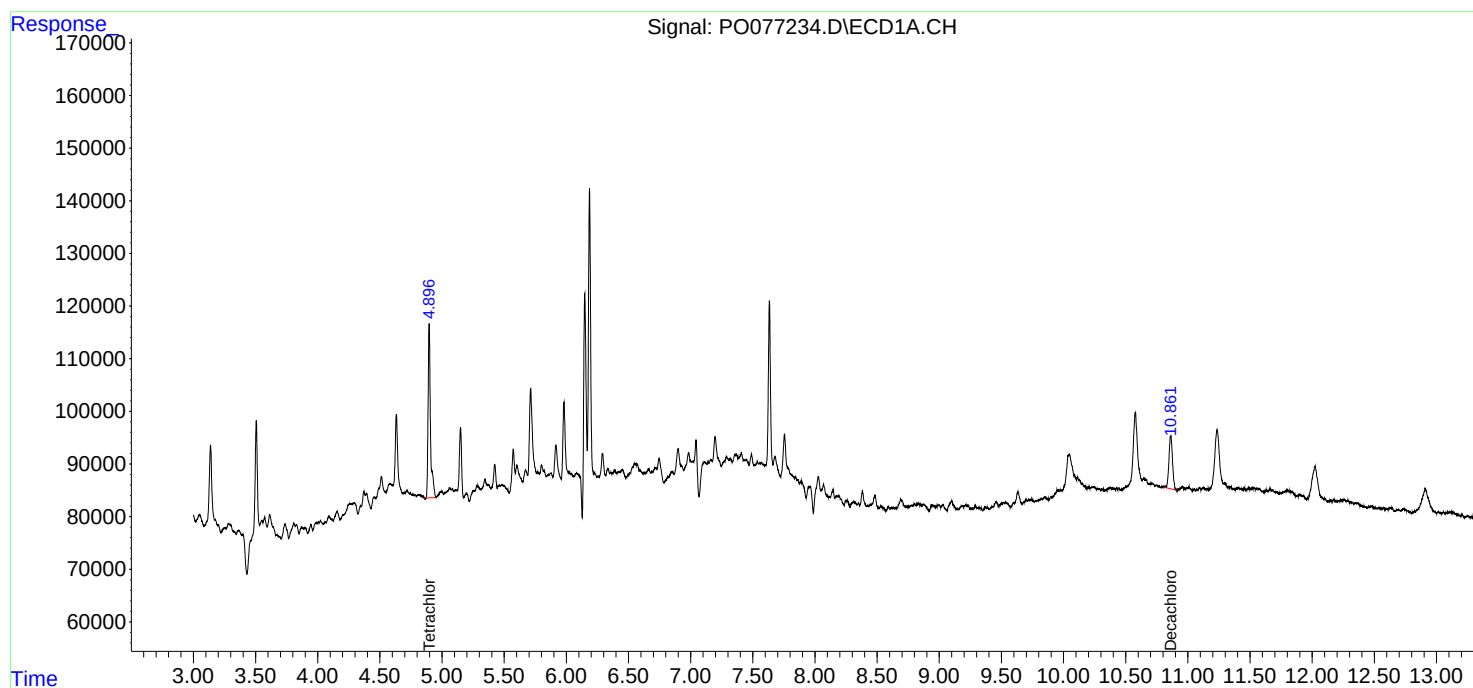


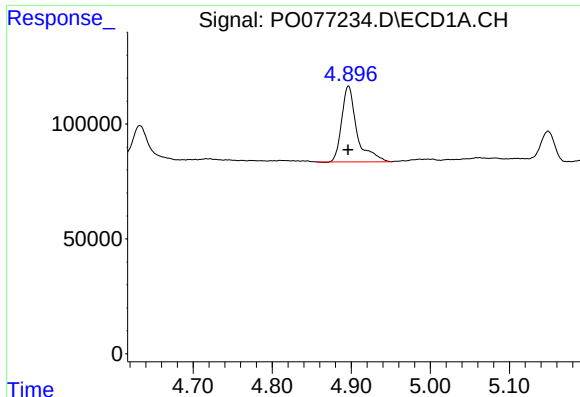

#1 Tetrachloro-m-xylene


R.T.: 4.896 min
Delta R.T.: 0.000 min
Response: 441273
Conc: 4.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
FS-WC-WATERRE

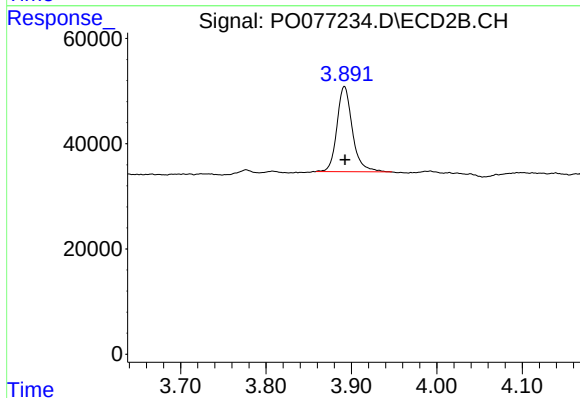


#1 Tetrachloro-m-xylene

R.T.: 3.892 min
Delta R.T.: 0.000 min
Response: 203536
Conc: 3.87 ng/ml

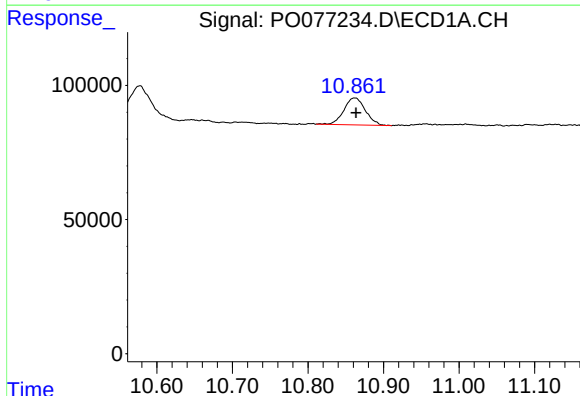

#2 Decachlorobiphenyl

R.T.: 10.862 min
Delta R.T.: -0.002 min
Response: 199398
Conc: 1.92 ng/ml

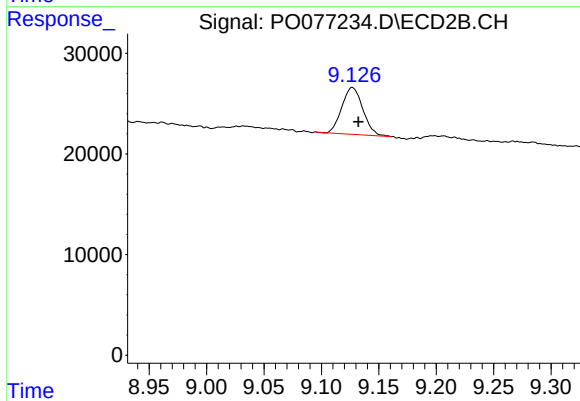

#2 Decachlorobiphenyl

R.T.: 9.127 min
Delta R.T.: -0.005 min
Response: 59607
Conc: 1.58 ng/ml