

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042425\
 Data File : P0110682.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2025 14:14
 Operator : YP/AJ
 Sample : Q1860-13
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 P001-SS010-01

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/25/2025
 Supervised By :mohammad ahmed 04/26/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 00:26:05 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0041025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 11 02:12:41 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.685	3.683	134.7E6	69988860	15.396	14.026
2) SA Decachlor...	8.726	8.679	74110575	26896579	9.387m	13.972m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO042425\
Data File : PO110682.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2025 14:14
Operator : YP/AJ
Sample : Q1860-13
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
P001-SS010-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/25/2025
Supervised By :mohammad ahmed 04/26/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 25 00:26:05 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO041025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 11 02:12:41 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

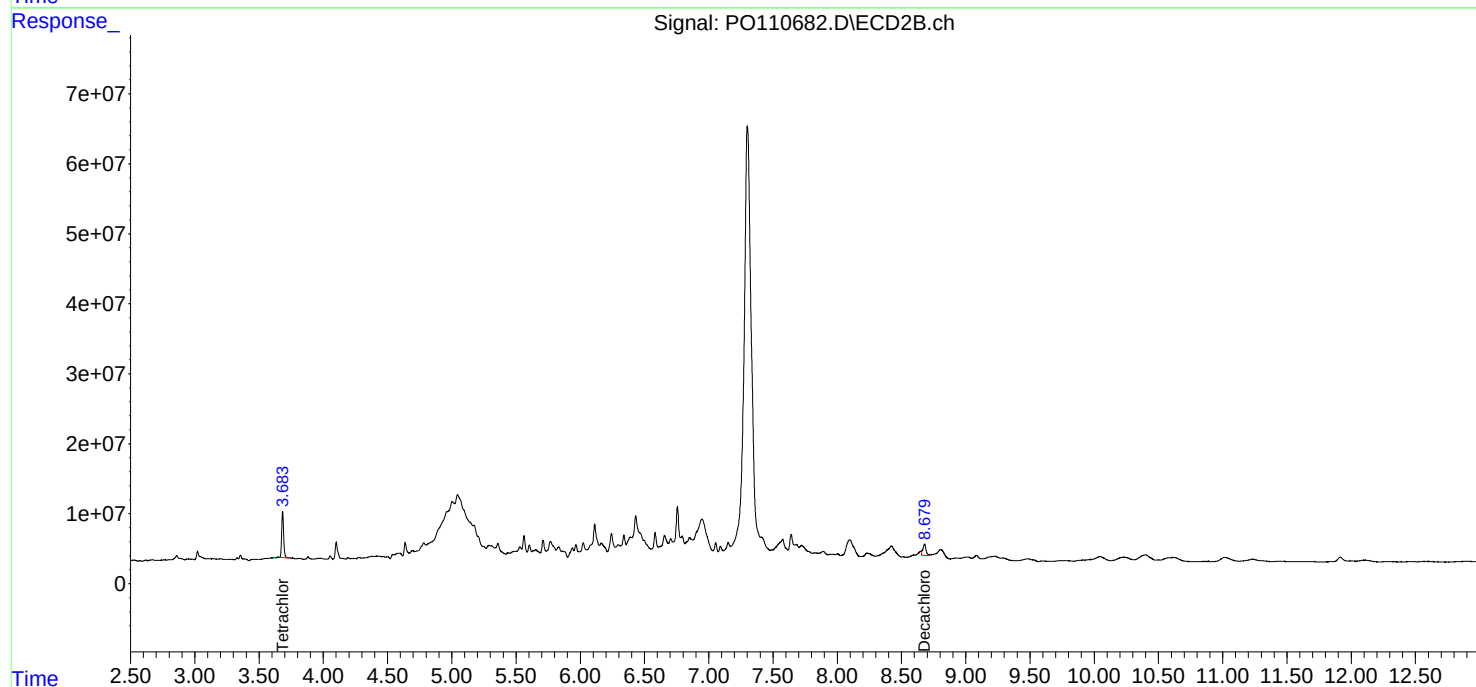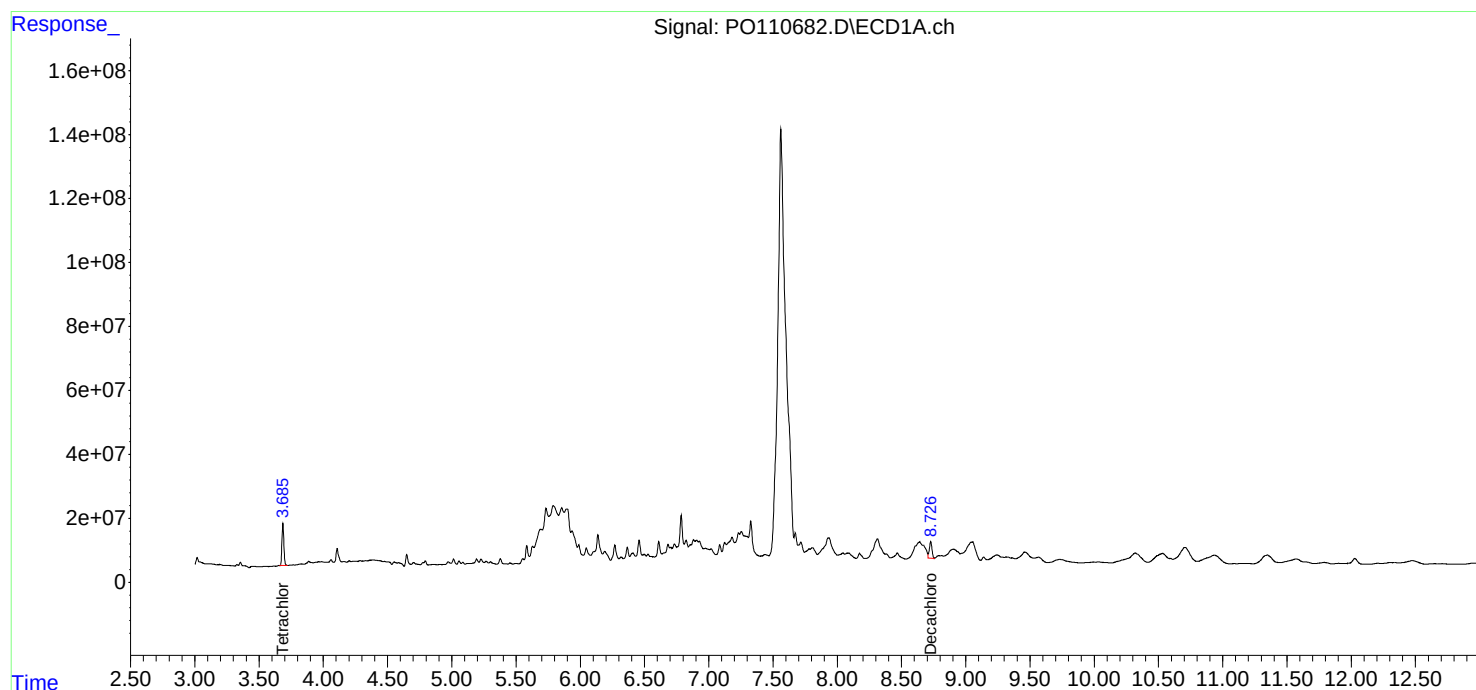

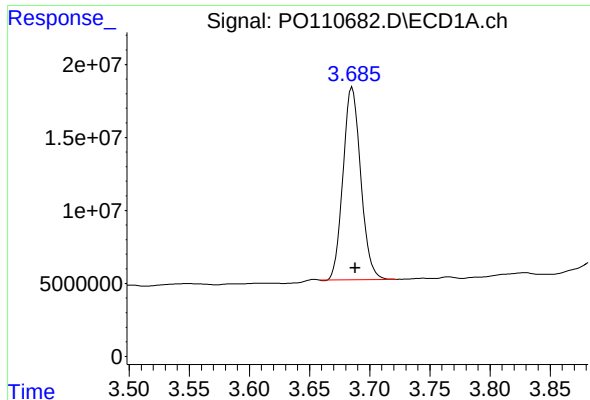


#1 Tetrachloro-m-xylene

R.T.: 3.685 min
Delta R.T.: -0.003 min
Response: 134700941
Conc: 15.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
P001-SS010-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/25/2025
Supervised By :mohammad ahmed 04/26/2025

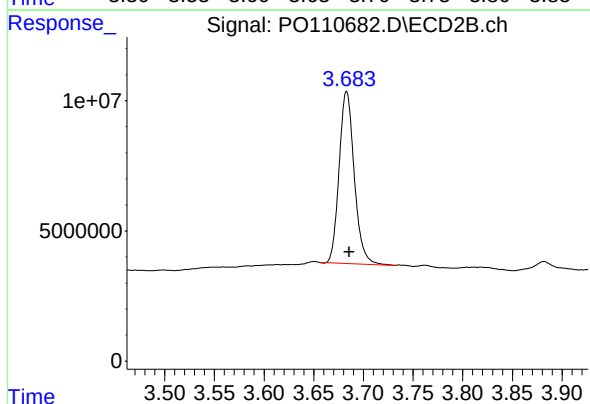


#1 Tetrachloro-m-xylene

R.T.: 3.683 min
Delta R.T.: -0.003 min
Response: 69988860
Conc: 14.03 ng/ml

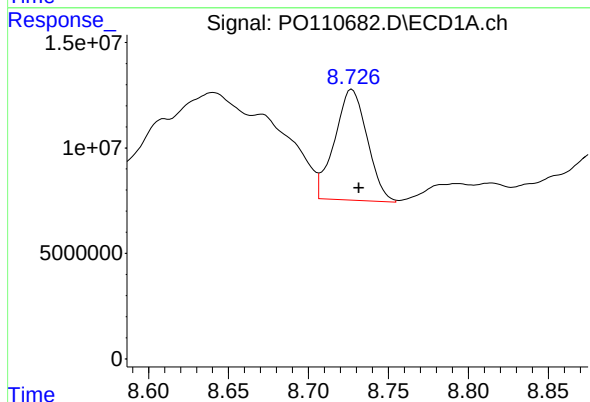

#2 Decachlorobiphenyl

R.T.: 8.726 min
Delta R.T.: -0.005 min
Response: 74110575
Conc: 9.39 ng/ml m

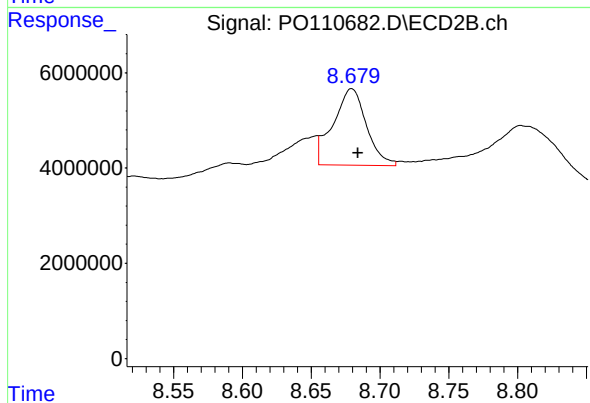

#2 Decachlorobiphenyl

R.T.: 8.679 min
Delta R.T.: -0.005 min
Response: 26896579
Conc: 13.97 ng/ml m